

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121419\
 Data File : VV014059.D
 Acq On : 13 Dec 2019 18:14
 Operator : SY/MD
 Sample : K4649-01ME
 Misc : 5.00µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A5167ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM080619W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	85	rVB	162781	156568	12.79%	1.414%
2	2.126	311	322	336	rBV3	497617	826958	67.56%	7.471%
3	2.646	476	484	495	rVB2	6912	12610	1.03%	0.114%
4	2.962	580	582	584	rBV2	422	277	0.02%	0.003%
5	3.032	603	604	605	rBV2	152	47	0.00%	0.000%
6	3.042	605	607	608	rVV	237	84	0.01%	0.001%
7	3.129	632	634	637	rBV2	311	221	0.02%	0.002%
8	3.299	685	687	689	rBV	304	199	0.02%	0.002%
9	3.331	694	697	698	rBV2	346	174	0.01%	0.002%
10	3.498	746	749	752	rVB3	394	213	0.02%	0.002%
11	3.521	752	756	759	rBV3	297	279	0.02%	0.003%
12	3.605	780	782	786	rVB2	297	198	0.02%	0.002%
13	3.627	786	789	794	rBV3	457	308	0.03%	0.003%
14	3.656	794	798	802	rBV3	474	405	0.03%	0.004%
15	3.698	807	811	814	rBV2	494	328	0.03%	0.003%
16	3.778	833	836	839	rVB2	689	452	0.04%	0.004%
17	3.804	841	844	845	rBV	460	185	0.02%	0.002%
18	3.833	851	853	855	rVB	661	172	0.01%	0.002%
19	3.852	855	859	861	rVB2	296	195	0.02%	0.002%
20	3.868	862	864	870	rVB2	323	186	0.02%	0.002%
21	3.923	870	881	909	rBV	93493	262563	21.45%	2.372%
22	4.392	1009	1027	1051	rBV2	210750	499847	40.84%	4.516%
23	4.566	1079	1081	1083	rBV3	530	319	0.03%	0.003%
24	4.601	1089	1092	1094	rBV	480	319	0.03%	0.003%
25	4.733	1131	1133	1137	rVB3	597	368	0.03%	0.003%
26	4.769	1142	1144	1146	rBV2	357	179	0.01%	0.002%
27	4.868	1170	1175	1181	rBV4	463	697	0.06%	0.006%
28	4.916	1187	1190	1192	rBV2	517	350	0.03%	0.003%
29	5.019	1219	1222	1224	rBV2	417	260	0.02%	0.002%
30	5.087	1225	1243	1252	rBV2	491362	1223954	100.00%	11.057%
31	5.505	1372	1373	1380	rBV3	518	543	0.04%	0.005%
32	5.540	1383	1384	1386	rBV2	404	160	0.01%	0.001%
33	5.656	1407	1420	1450	rBV	365456	716409	58.53%	6.472%
34	5.952	1496	1512	1533	rBV3	340534	696251	56.89%	6.290%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121419\
 Data File : VV014059.D
 Acq On : 13 Dec 2019 18:14
 Operator : SY/MD
 Sample : K4649-01ME
 Misc : 5.00µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A5167ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM080619W.M
 Title : VOC Analysis

35	6.109	1548	1561	1586	rBV	281142	565669	46.22%	5.110%
36	6.293	1616	1618	1620	rBV3	498	273	0.02%	0.002%
37	6.386	1644	1647	1648	rBV2	329	170	0.01%	0.002%
38	6.444	1658	1665	1670	rBV3	586	680	0.06%	0.006%
39	6.476	1673	1675	1678	rVB2	306	185	0.02%	0.002%
40	6.498	1680	1682	1684	rBV	200	80	0.01%	0.001%
41	6.540	1690	1695	1698	rBV3	411	452	0.04%	0.004%
42	6.556	1698	1700	1704	rVB4	571	403	0.03%	0.004%
43	6.653	1722	1730	1735	rBV7	2206	3941	0.32%	0.036%
44	6.765	1763	1765	1768	rVB	385	188	0.02%	0.002%
45	6.781	1768	1770	1774	rBV2	281	218	0.02%	0.002%
46	6.881	1799	1801	1802	rBV	294	146	0.01%	0.001%
47	6.926	1813	1815	1817	rVB	251	79	0.01%	0.001%
48	6.945	1819	1821	1824	rVB2	363	148	0.01%	0.001%
49	6.981	1831	1832	1834	rBV	254	68	0.01%	0.001%
50	7.022	1834	1845	1869	rBV	136063	247290	20.20%	2.234%
51	7.354	1936	1948	1960	rBV	530350	910836	74.42%	8.229%
52	7.428	1961	1971	1994	rVB	647367	1089144	88.99%	9.839%
53	7.656	2032	2042	2061	rBV	101235	170888	13.96%	1.544%
54	7.826	2092	2095	2099	rBV4	465	311	0.03%	0.003%
55	7.897	2115	2117	2120	rBV2	378	211	0.02%	0.002%
56	7.977	2141	2142	2145	rBV	290	181	0.01%	0.002%
57	8.006	2149	2151	2152	rBV	673	273	0.02%	0.002%
58	8.129	2178	2189	2230	rBV2	281265	611838	49.99%	5.527%
59	8.479	2297	2298	2301	rVB	311	143	0.01%	0.001%
60	8.743	2378	2380	2383	rBV	287	221	0.02%	0.002%
61	8.756	2383	2384	2387	rVV	248	118	0.01%	0.001%
62	8.891	2414	2426	2430	rBV	552339	826690	67.54%	7.468%
63	9.103	2490	2492	2495	rBV	345	102	0.01%	0.001%
64	9.116	2495	2496	2498	rBV2	287	108	0.01%	0.001%
65	9.132	2498	2501	2503	rBV3	506	337	0.03%	0.003%
66	9.267	2539	2543	2544	rBV	261	181	0.01%	0.002%
67	9.437	2594	2596	2598	rBV2	281	135	0.01%	0.001%
68	9.498	2613	2615	2616	rBV	308	105	0.01%	0.001%
69	9.524	2621	2623	2624	rBV	313	133	0.01%	0.001%
70	9.585	2640	2642	2644	rBV2	912	610	0.05%	0.006%
71	9.659	2661	2665	2666	rBV	378	319	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121419\
 Data File : VV014059.D
 Acq On : 13 Dec 2019 18:14
 Operator : SY/MD
 Sample : K4649-01ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A5167ME

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM080619W.M
 Title : VOC Analysis

72	9.688	2671	2674	2675	rBV	362	159	0.01%	0.001%
73	9.701	2675	2678	2680	rVV2	447	184	0.02%	0.002%
74	9.971	2759	2762	2770	rVB5	961	1087	0.09%	0.010%
75	10.042	2781	2784	2788	rBV3	524	319	0.03%	0.003%
76	10.067	2788	2792	2796	rBV3	682	719	0.06%	0.006%
77	10.119	2804	2808	2810	rBV3	480	354	0.03%	0.003%
78	10.257	2838	2851	2870	rBV	364879	569036	46.49%	5.141%
79	10.485	2919	2922	2925	rBV2	330	196	0.02%	0.002%
80	10.569	2946	2948	2950	rBV2	424	234	0.02%	0.002%
81	10.624	2963	2965	2967	rBV2	346	163	0.01%	0.001%
82	10.640	2968	2970	2973	rVB	390	192	0.02%	0.002%
83	10.698	2984	2988	2993	rBV4	529	558	0.05%	0.005%
84	10.897	3047	3050	3052	rBV3	394	209	0.02%	0.002%
85	10.961	3067	3070	3074	rVB3	1009	661	0.05%	0.006%
86	11.019	3082	3088	3090	rBV3	235	220	0.02%	0.002%
87	11.035	3090	3093	3105	rVV3	478	613	0.05%	0.006%
88	11.202	3142	3145	3147	rBV3	550	328	0.03%	0.003%
89	11.218	3147	3150	3151	rBV	1018	485	0.04%	0.004%
90	11.289	3160	3172	3192	rBV	490766	755897	61.76%	6.829%
91	11.665	3277	3289	3315	rBV	563699	901972	73.69%	8.148%
92	12.067	3412	3414	3417	rVB	420	206	0.02%	0.002%
93	12.251	3468	3471	3473	rBV3	451	237	0.02%	0.002%


Sum of corrected areas: 11069181

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121419\
Data File : VV014059.D
Acq On : 13 Dec 2019 18:14
Operator : SY/MD
Sample : K4649-01ME
Misc : 5.00µ/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A5167ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM080619W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

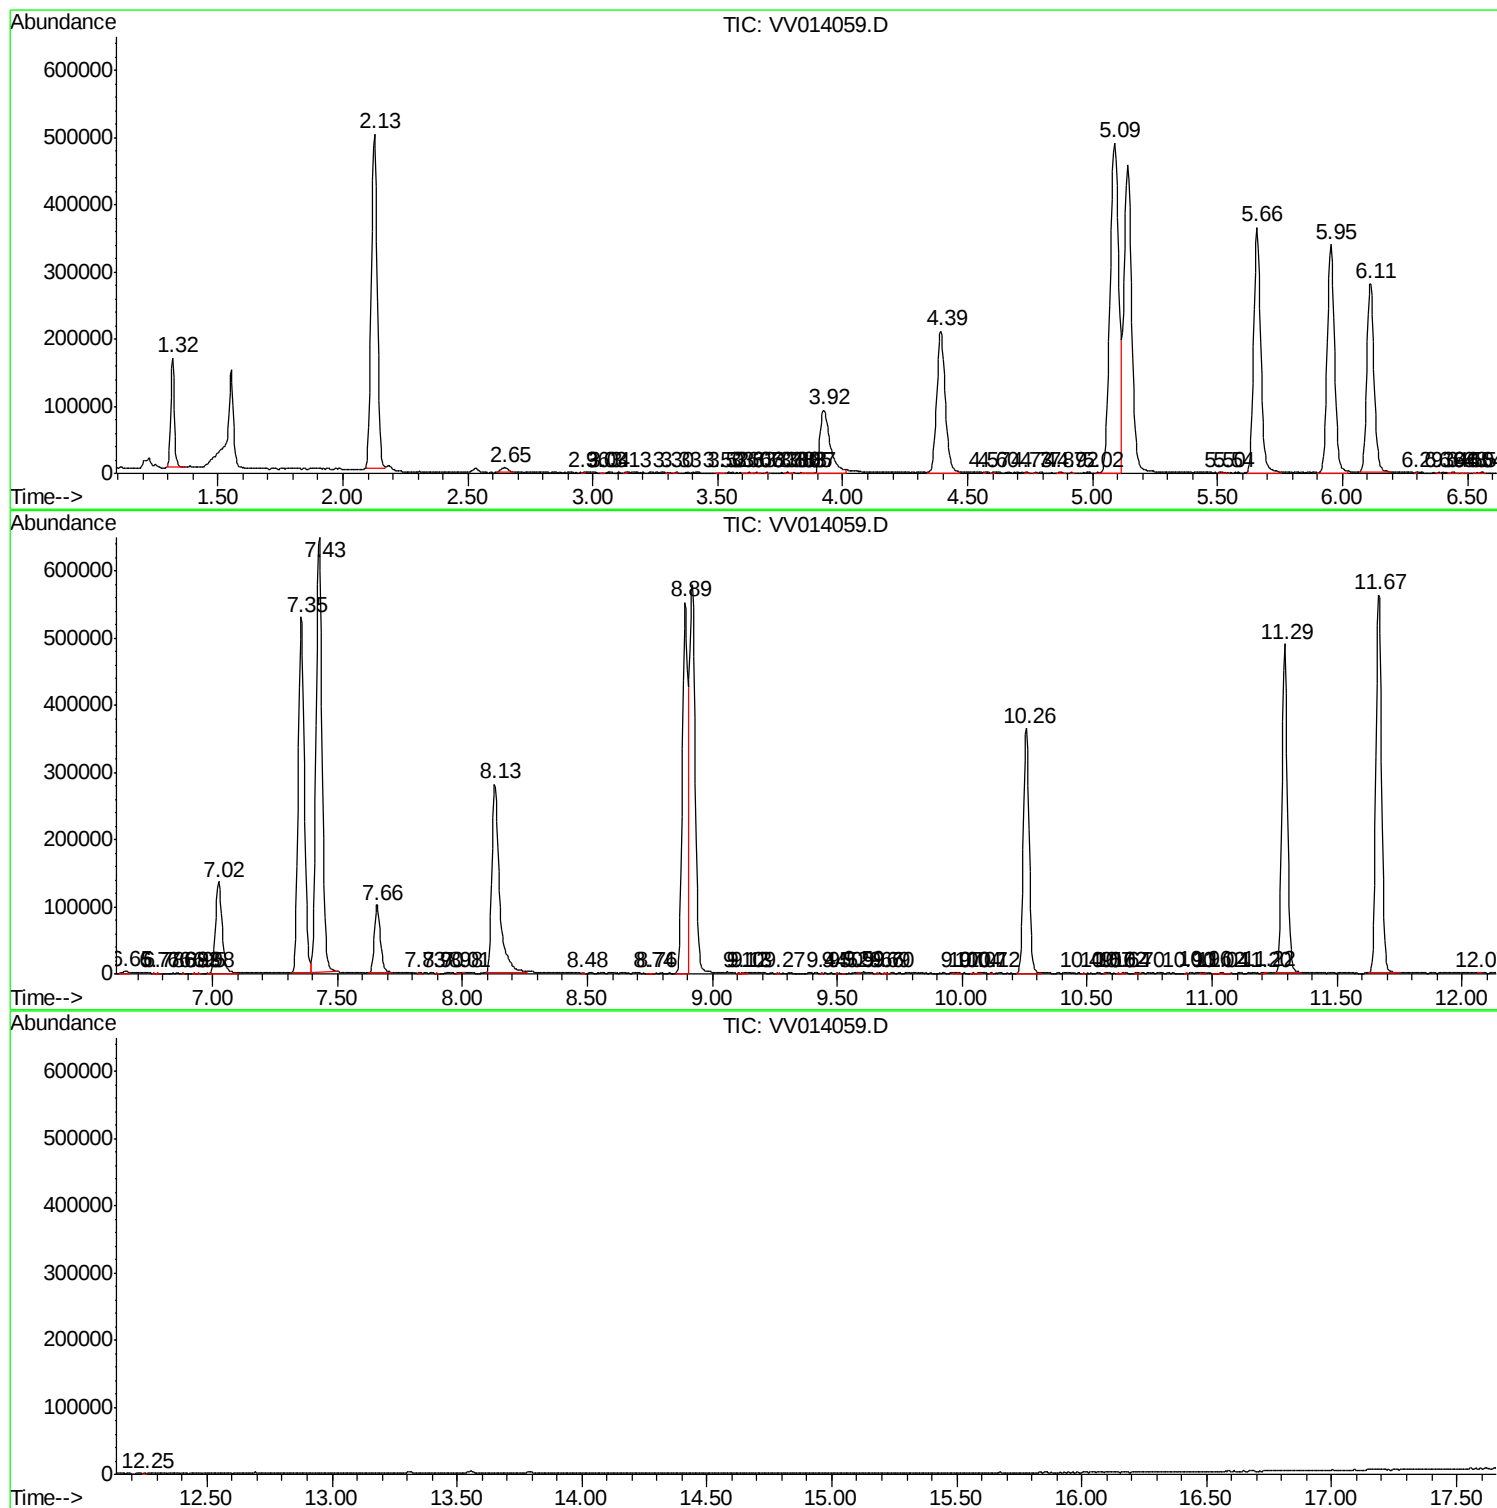

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121419\
Data File : VV014059.D
Acq On : 13 Dec 2019 18:14
Operator : SY/MD
Sample : K4649-01ME
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A5167ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM080619W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121419\
Data File : VV014059.D
Acq On : 13 Dec 2019 18:14
Operator : SY/MD
Sample : K4649-01ME
Misc : 5.00g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
A5167ME

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SFAMVLM080619W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc