


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121419\
 Data File : VV014056.D
 Acq On : 13 Dec 2019 16:54
 Operator : SY/MD
 Sample : BFB82
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB822

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM080619W.M
 Title : VOC Analysis
 Last Update : Sat Dec 14 05:36:38 2019

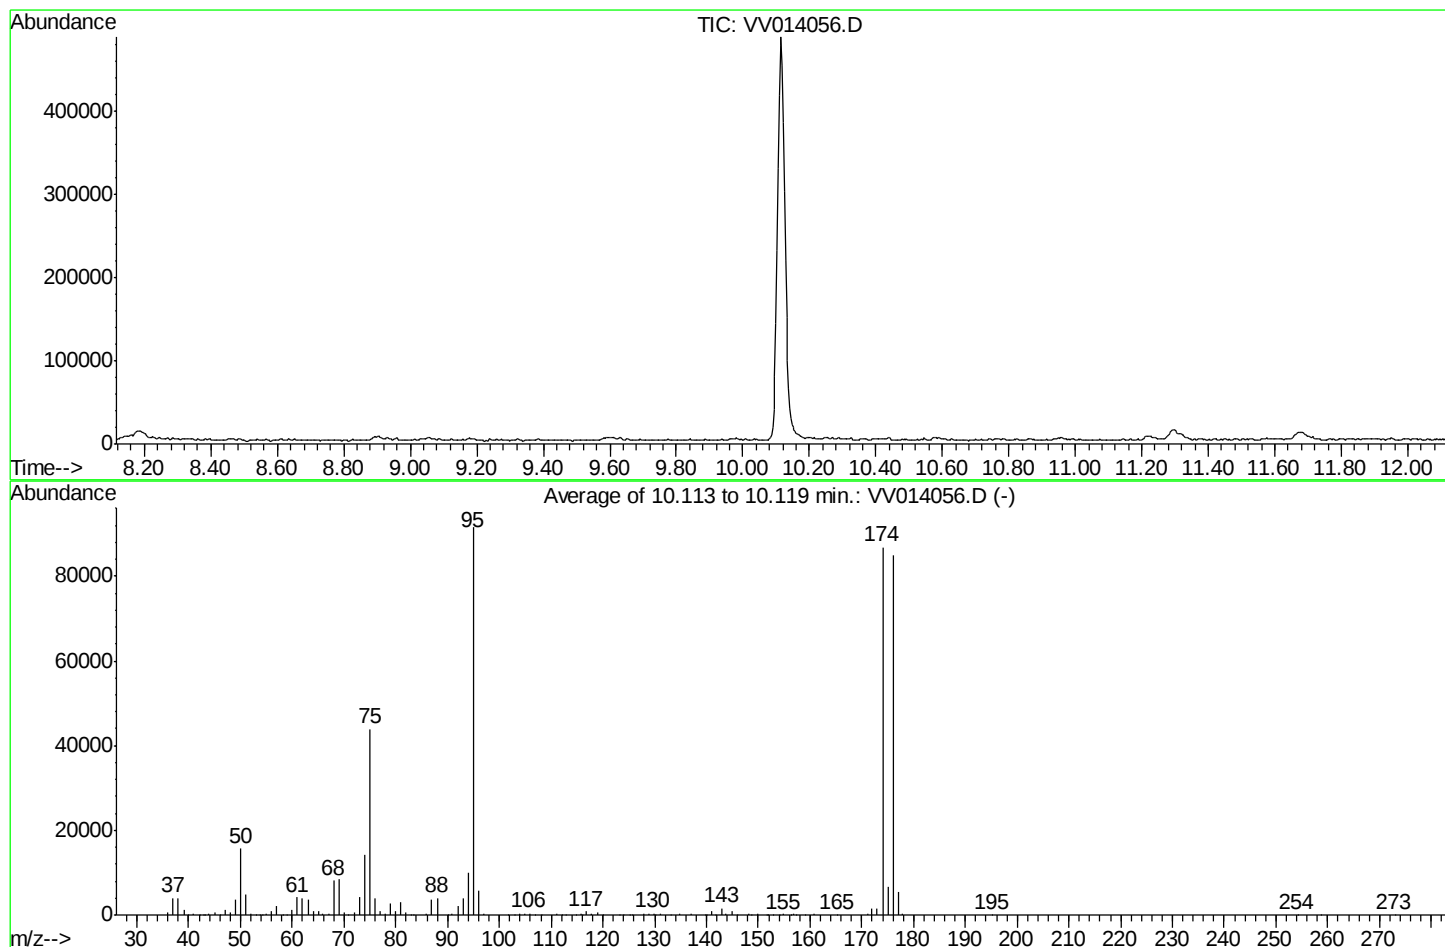

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	15644	PASS
75	95	30	80	48.0	43957	PASS
95	95	100	100	100.0	91562	PASS
96	95	5	9	6.4	5889	PASS
173	174	0.00	2	1.8	1562	PASS
174	95	50	120	94.9	86928	PASS
175	174	5	9	7.5	6536	PASS
176	174	95	101	97.7	84941	PASS
177	176	5	9	6.4	5411	PASS

m/z	Abundance
36.00	702.0
37.00	4264.0
38.00	3846.0
39.10	1280.0
39.90	959.0
40.80	252.0
42.00	176.0
43.10	178.0
44.00	1202.0
45.00	912.0
46.00	218.0
47.00	1427.0
48.10	740.0
49.00	3840.0
50.10	16035.0
51.10	5147.0
52.10	267.0
53.10	193.0
53.70	101.0
54.20	108.0
55.00	235.0
56.00	1043.0
57.00	2302.0
58.10	141.0
58.90	115.0
60.00	960.0
61.00	4287.0
62.00	4259.0
63.00	3771.0
64.10	844.0
65.00	1089.0
66.00	128.0
67.00	333.0
68.00	8703.0
69.10	8663.0
70.00	640.0
72.00	430.0
73.00	4304.0
74.10	14424.0
75.00	44248.0
76.00	3917.0
76.90	814.0
78.00	351.0
78.90	3066.0
79.90	816.0
81.00	3033.0
81.90	583.0
82.80	124.0
85.80	268.0
86.90	3921.0
88.00	4058.0
90.10	113.0
90.90	362.0
92.00	2077.0
93.00	3987.0
94.10	10309.0
95.00	92912.0
96.10	5980.0
97.00	311.0
101.80	143.0
102.90	106.0
103.90	404.0
105.00	221.0
105.80	450.0
107.00	146.0
111.00	192.0
112.20	114.0
112.70	131.0
115.80	371.0
116.90	846.0
117.80	179.0
119.00	671.0
120.10	114.0
127.90	394.0
129.00	226.0
129.90	415.0
131.00	211.0
133.10	111.0
134.70	181.0
137.00	266.0
140.10	231.0
141.10	972.0
141.80	212.0
143.00	1683.0
143.80	363.0
144.90	928.0
146.00	151.0
148.10	306.0
149.90	155.0
151.60	101.0
152.80	120.0
154.90	306.0

Instrument :
MSVOA_V
ClientSampleId :
BFB822

156.30	151.0
156.80	207.0
158.90	151.0
160.80	214.0
165.30	109.0
171.10	318.0
172.00	1435.0
173.00	1586.0
174.00	86360.0
175.00	6405.0
176.00	83792.0
177.00	5117.0
178.00	246.0
195.20	123.0
258.60	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB822

m/z	Abundance
36.00	827.0
37.00	4215.0
38.00	4064.0
39.10	1526.0
39.90	980.0
40.90	231.0
42.00	169.0
42.80	198.0
44.00	1039.0
45.10	906.0
46.00	231.0
47.00	1469.0
48.10	752.0
49.00	3700.0
50.10	16074.0
51.10	5025.0
52.00	287.0
53.20	213.0
53.80	118.0
54.20	146.0
55.00	254.0
56.00	974.0
57.00	2249.0
58.20	159.0
58.80	122.0
60.00	1170.0
61.00	4174.0
62.00	4031.0
63.00	3812.0
64.00	919.0
65.00	1063.0
65.90	187.0
67.00	286.0
68.00	8328.0
69.00	8752.0
70.00	635.0
72.00	535.0
73.00	4516.0
74.10	14564.0
75.00	45480.0
76.00	4057.0
76.90	852.0
78.00	328.0
79.00	2879.0
80.00	828.0
81.00	2984.0
81.90	560.0
83.30	129.0
85.70	300.0
87.00	3859.0
88.00	4113.0
90.80	390.0
92.00	2199.0
93.00	3914.0
94.10	10430.0
95.00	94632.0
96.10	6073.0
97.00	320.0
103.90	457.0
105.00	201.0
105.80	469.0
107.00	119.0
111.10	187.0
112.10	153.0
112.70	110.0
115.80	332.0
116.90	819.0
117.80	189.0
119.10	623.0
124.00	121.0
127.90	370.0
129.00	175.0
129.90	346.0
131.00	171.0
134.70	224.0
137.00	263.0
140.10	180.0
141.10	976.0
141.80	159.0
143.00	1628.0
143.80	293.0
144.90	987.0
146.00	134.0
148.00	325.0
148.70	103.0
149.90	207.0
152.80	106.0
154.00	120.0
154.90	277.0
156.70	180.0
157.20	157.0
159.00	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB822

160.80	193.0
171.10	345.0
171.90	1463.0
172.90	1604.0
174.00	89800.0
175.00	6810.0
176.00	87736.0
177.00	5617.0
177.90	277.0
272.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB822

m/z	Abundance
36.10	821.0
37.00	3801.0
38.00	3942.0
39.10	1575.0
39.80	978.0
40.90	187.0
42.00	133.0
42.90	179.0
44.00	902.0
45.10	769.0
45.90	212.0
47.00	1215.0
48.10	627.0
49.00	3114.0
50.00	14825.0
51.10	4469.0
52.00	305.0
53.20	182.0
54.20	228.0
55.00	270.0
56.10	1052.0
57.00	2119.0
58.30	187.0
58.80	115.0
59.90	1109.0
61.00	3855.0
62.00	3514.0
63.00	3487.0
64.00	905.0
65.10	922.0
66.00	214.0
67.00	236.0
68.00	7421.0
69.00	8140.0
70.10	626.0
70.80	114.0
72.00	552.0
73.10	4165.0
74.10	13355.0
75.00	42144.0
76.00	3848.0
76.90	712.0
78.10	282.0
78.90	2579.0
80.00	750.0
81.00	2718.0
81.90	446.0
83.30	137.0
85.70	238.0
87.00	3435.0
88.00	3640.0
90.80	418.0
92.00	2170.0
93.00	3530.0
94.00	9381.0
95.00	87144.0
96.10	5616.0
97.10	285.0
103.90	400.0
105.00	184.0
105.80	370.0
107.00	102.0
108.20	113.0
111.10	124.0
112.10	180.0
114.70	107.0
116.00	304.0
116.80	699.0
117.70	182.0
119.10	545.0
123.10	114.0
124.00	125.0
125.20	117.0
125.60	110.0
128.00	286.0
129.00	142.0
129.80	258.0
130.10	231.0
131.00	137.0
134.70	184.0
136.80	234.0
139.80	117.0
141.00	930.0
143.00	1498.0
143.90	172.0
144.90	962.0
146.00	138.0
148.00	328.0
148.70	135.0
150.00	196.0
151.80	102.0
154.10	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB822

154.90	177.0
156.70	178.0
159.00	165.0
160.90	134.0
171.00	367.0
171.90	1435.0
172.90	1496.0
174.00	84624.0
175.00	6393.0
176.00	83296.0
177.00	5500.0
177.90	230.0
254.20	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB822

m/z	Abundance
36.20	222.0
37.00	134.0
38.00	125.0
38.90	121.0
39.90	812.0
42.10	114.0
42.70	107.0
43.90	677.0
45.00	118.0
46.00	183.0
46.50	143.0
47.10	108.0
48.10	159.0
53.10	114.0
62.40	107.0
63.90	114.0
77.20	173.0
79.40	124.0
80.20	108.0
81.40	108.0
85.00	121.0
114.10	110.0
122.30	114.0
122.70	103.0
127.90	121.0
206.90	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB822