

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019613.D
 Acq On : 14 Dec 2020 18:41
 Operator : SY/MD
 Sample : L4928-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4J0

Quant Time: Dec 15 08:23:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 15 07:21:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.62	114	614226	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.86	117	573679	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.25	152	263489	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	222712	50.56	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	101.12%
7) Chloroethane-d5	1.57	69	188350	54.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	108.44%
11) 1,1-Dichloroethene-d2	2.11	63	328760	40.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.44%
21) 2-Butanone-d5	3.89	46	275423	115.05	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	115.05%
24) Chloroform-d	4.35	84	411981	51.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.80%
26) 1,2-Dichloroethane-d4	5.04	65	287353	55.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.78%
32) Benzene-d6	5.05	84	828360	54.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.28%
36) 1,2-Dichloropropane-d6	6.07	67	262494	54.77	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	109.54%
41) Toluene-d8	7.32	98	736134	53.44	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.88%
43) trans-1,3-Dichloropropene-	7.62	79	127830	46.89	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.78%
47) 2-Hexanone-d5	8.09	63	197520	105.00	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.00%
57) 1,1,2,2-Tetrachloroethane-	10.22	84	328953	50.74	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.48%
64) 1,2-Dichlorobenzene-d4	11.63	152	266563	54.12	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.24%


Target Compounds					Ovalue
13) Acetone	2.19	43	15033	7.371 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121420\
Data File : VV019613.D
Acq On : 14 Dec 2020 18:41
Operator : SY/MD
Sample : L4928-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4J0

Quant Time: Dec 15 08:23:16 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 15 07:21:43 2020
Response via : Initial Calibration

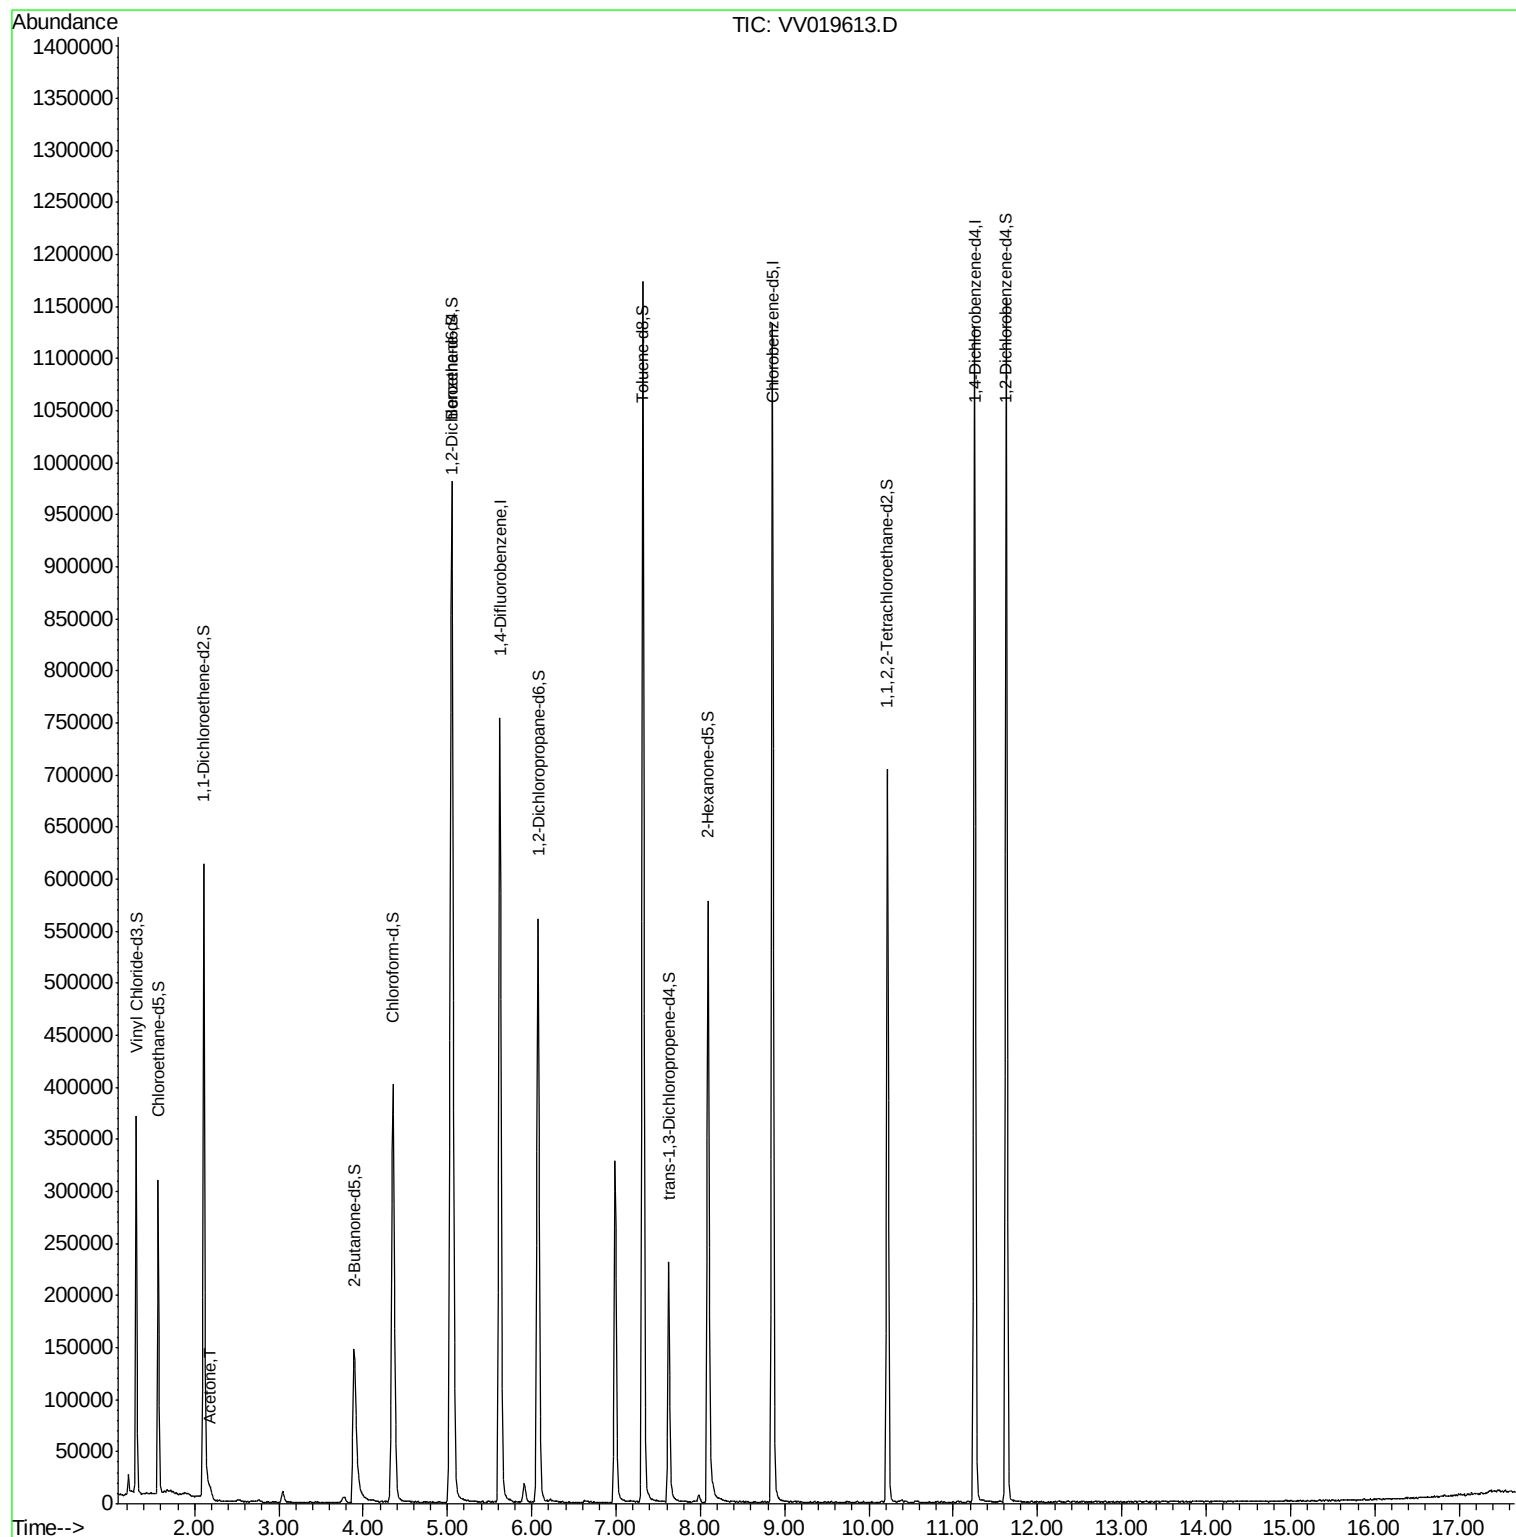

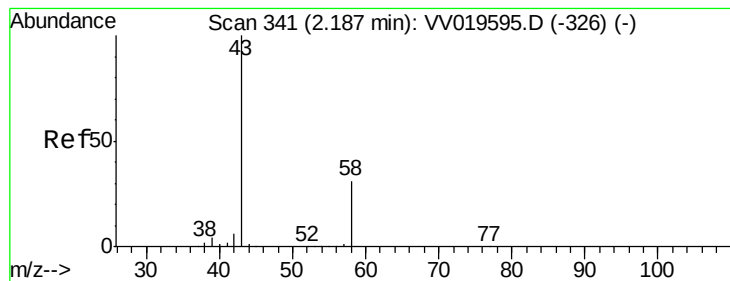

#13
Acetone
Concen: 7.371 ug/L
RT: 2.19 min Scan# 342
Delta R.T. 0.00 min
Lab File: VV019613.D
Acq: 14 Dec 2020 18:41

Instrument :
MSVOA_V
ClientSampleId :
BG4J0

Tot Ion: 43 Resp: 15033
Ion Ratio Lower Upper
43 100
58 28.2 0.0 61.6

