

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019598.D
 Acq On : 14 Dec 2020 12:40
 Operator : SY/MD
 Sample : L4928-03 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.110	3	6	16	rVB2	15644	13797	0.38%	0.058%
2	1.309	61	68	81	rVB	410262	403294	11.25%	1.690%
3	1.569	141	149	164	rBV	322169	367665	10.25%	1.540%
4	2.109	306	317	352	rVB	661378	1018121	28.40%	4.266%
5	2.511	435	442	444	rBV5	2955	3432	0.10%	0.014%
6	2.724	505	508	510	rBV2	775	382	0.01%	0.002%
7	2.765	511	521	531	rVB5	3620	7255	0.20%	0.030%
8	2.836	541	543	548	rBV3	623	473	0.01%	0.002%
9	2.955	577	580	582	rBV2	854	490	0.01%	0.002%
10	3.045	597	608	617	rVV5	7414	14544	0.41%	0.061%
11	3.209	656	659	663	rVV3	567	406	0.01%	0.002%
12	3.251	669	672	676	rBV4	665	515	0.01%	0.002%
13	3.315	688	692	696	rVB4	656	650	0.02%	0.003%
14	3.363	702	707	708	rBV3	574	401	0.01%	0.002%
15	3.495	743	748	752	rVB5	535	523	0.01%	0.002%
16	3.608	780	783	787	rVB3	881	685	0.02%	0.003%
17	3.634	787	791	794	rBV4	577	617	0.02%	0.003%
18	3.653	794	797	799	rVV3	578	394	0.01%	0.002%
19	3.669	799	802	805	rVV4	662	550	0.02%	0.002%
20	3.688	805	808	812	rVV2	578	513	0.01%	0.002%
21	3.717	812	817	819	rVV2	840	705	0.02%	0.003%
22	3.762	819	831	852	rVB6	6479	16991	0.47%	0.071%
23	3.891	859	871	909	rBV2	140106	461043	12.86%	1.932%
24	4.347	996	1013	1045	rVV	423798	1054108	29.40%	4.417%
25	4.633	1099	1102	1107	rBV5	619	646	0.02%	0.003%
26	4.759	1134	1141	1144	rBV4	1028	1322	0.04%	0.006%
27	4.894	1179	1183	1188	rBV4	894	861	0.02%	0.004%
28	5.048	1211	1231	1271	rBV2	1049317	2712455	75.65%	11.365%
29	5.302	1307	1310	1313	rBV4	752	589	0.02%	0.002%
30	5.386	1333	1336	1338	rBV3	697	494	0.01%	0.002%
31	5.489	1367	1368	1373	rVB3	759	444	0.01%	0.002%
32	5.617	1394	1408	1434	rBV	815614	1629992	45.46%	6.830%
33	5.920	1488	1502	1519	rVV6	42242	96542	2.69%	0.405%
34	6.071	1535	1549	1577	rVV	601340	1210211	33.75%	5.071%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019598.D
 Acq On : 14 Dec 2020 12:40
 Operator : SY/MD
 Sample : L4928-03 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.389	1645	1648	1652	rVB3	1089	867	0.02%	0.004%
36	6.617	1712	1719	1720	rBV6	1505	1438	0.04%	0.006%
37	6.752	1758	1761	1765	rVB4	694	451	0.01%	0.002%
38	6.987	1821	1834	1863	rBV	362818	666152	18.58%	2.791%
39	7.315	1924	1936	1958	rBV	1259055	2170566	60.54%	9.095%
40	7.498	1991	1993	1997	rBV4	572	436	0.01%	0.002%
41	7.621	2018	2031	2053	rBV	251610	445607	12.43%	1.867%
42	7.974	2126	2141	2166	rBV	2136379	3585503	100.00%	15.023%
43	8.087	2166	2176	2208	rVV	558039	969578	27.04%	4.062%
44	8.428	2274	2282	2286	rBV5	2435	3018	0.08%	0.013%
45	8.511	2305	2308	2309	rBV	678	400	0.01%	0.002%
46	8.556	2316	2322	2324	rBV2	679	776	0.02%	0.003%
47	8.592	2330	2333	2335	rBV4	629	456	0.01%	0.002%
48	8.746	2379	2381	2385	rVB3	649	448	0.01%	0.002%
49	8.852	2402	2414	2439	rBV	1234512	1971099	54.97%	8.259%
50	9.154	2497	2508	2512	rBV7	1945	3442	0.10%	0.014%
51	9.286	2545	2549	2552	rVB5	653	503	0.01%	0.002%
52	9.550	2627	2631	2636	rBV4	1460	1377	0.04%	0.006%
53	9.659	2662	2665	2667	rBV2	652	400	0.01%	0.002%
54	9.704	2675	2679	2680	rBV2	559	386	0.01%	0.002%
55	9.788	2702	2705	2711	rVB4	453	393	0.01%	0.002%
56	9.820	2711	2715	2717	rBV3	731	663	0.02%	0.003%
57	9.900	2736	2740	2743	rBV2	496	458	0.01%	0.002%
58	10.038	2780	2783	2787	rVB2	535	433	0.01%	0.002%
59	10.218	2825	2839	2859	rVV	755142	1160503	32.37%	4.862%
60	10.334	2871	2875	2879	rVB3	459	459	0.01%	0.002%
61	10.579	2948	2951	2954	rBV4	663	552	0.02%	0.002%
62	10.739	2999	3001	3005	rVV3	519	470	0.01%	0.002%
63	10.849	3032	3035	3036	rBV2	701	428	0.01%	0.002%
64	10.858	3036	3038	3041	rVB3	738	449	0.01%	0.002%
65	10.919	3050	3057	3065	rBV6	3567	5047	0.14%	0.021%
66	11.157	3129	3131	3133	rBV2	977	554	0.02%	0.002%
67	11.251	3148	3160	3182	rBV	1239243	1919072	53.52%	8.041%
68	11.466	3225	3227	3230	rBV2	848	425	0.01%	0.002%
69	11.527	3242	3246	3247	rBV4	815	566	0.02%	0.002%
70	11.627	3264	3277	3300	rBV	1219330	1908026	53.22%	7.994%
71	11.797	3326	3330	3333	rBV5	657	639	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019598.D
 Acq On : 14 Dec 2020 12:40
 Operator : SY/MD
 Sample : L4928-03 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	11.916	3363	3367	3370	rBV3	642	449	0.01%	0.002%
73	12.109	3423	3427	3429	rBV2	542	477	0.01%	0.002%
74	12.302	3485	3487	3494	rVV3	573	567	0.02%	0.002%
75	12.395	3514	3516	3519	rVB3	939	432	0.01%	0.002%
76	12.469	3534	3539	3547	rBV5	939	1233	0.03%	0.005%
77	12.652	3589	3596	3603	rBV8	1682	2175	0.06%	0.009%
78	12.701	3608	3611	3615	rBV3	718	537	0.01%	0.002%
79	12.733	3615	3621	3625	rBV3	1096	872	0.02%	0.004%
80	12.755	3625	3628	3630	rBV3	696	438	0.01%	0.002%
81	12.916	3676	3678	3681	rBV2	817	614	0.02%	0.003%
82	12.951	3686	3689	3691	rVV2	808	398	0.01%	0.002%
83	13.045	3714	3718	3719	rBV3	837	446	0.01%	0.002%
84	13.209	3767	3769	3773	rVB	875	446	0.01%	0.002%
85	13.231	3773	3776	3779	rBV2	583	453	0.01%	0.002%
86	13.273	3784	3789	3795	rVB6	2159	2570	0.07%	0.011%
87	13.350	3811	3813	3815	rBV2	881	410	0.01%	0.002%
88	13.434	3836	3839	3842	rBV4	745	549	0.02%	0.002%
89	13.460	3843	3847	3850	rBV3	691	543	0.02%	0.002%
90	13.505	3854	3861	3862	rBV3	1578	1609	0.04%	0.007%
91	13.556	3875	3877	3885	rVB7	1040	787	0.02%	0.003%
92	13.591	3885	3888	3891	rBV3	503	484	0.01%	0.002%
93	13.746	3932	3936	3945	rVB9	1858	2622	0.07%	0.011%
94	13.787	3946	3949	3954	rVB3	765	570	0.02%	0.002%
95	13.813	3954	3957	3960	rBV4	715	717	0.02%	0.003%
96	13.968	4003	4005	4011	rVB4	737	783	0.02%	0.003%
97	13.996	4011	4014	4017	rBV3	639	444	0.01%	0.002%
98	14.897	4292	4294	4301	rBV4	1020	914	0.03%	0.004%
99	15.080	4349	4351	4353	rBV2	942	526	0.01%	0.002%
100	15.308	4420	4422	4425	rBV3	768	537	0.01%	0.002%


Sum of corrected areas: 23866752

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121420\
Data File : VV019598.D
Acq On : 14 Dec 2020 12:40
Operator : SY/MD
Sample : L4928-03 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4M0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

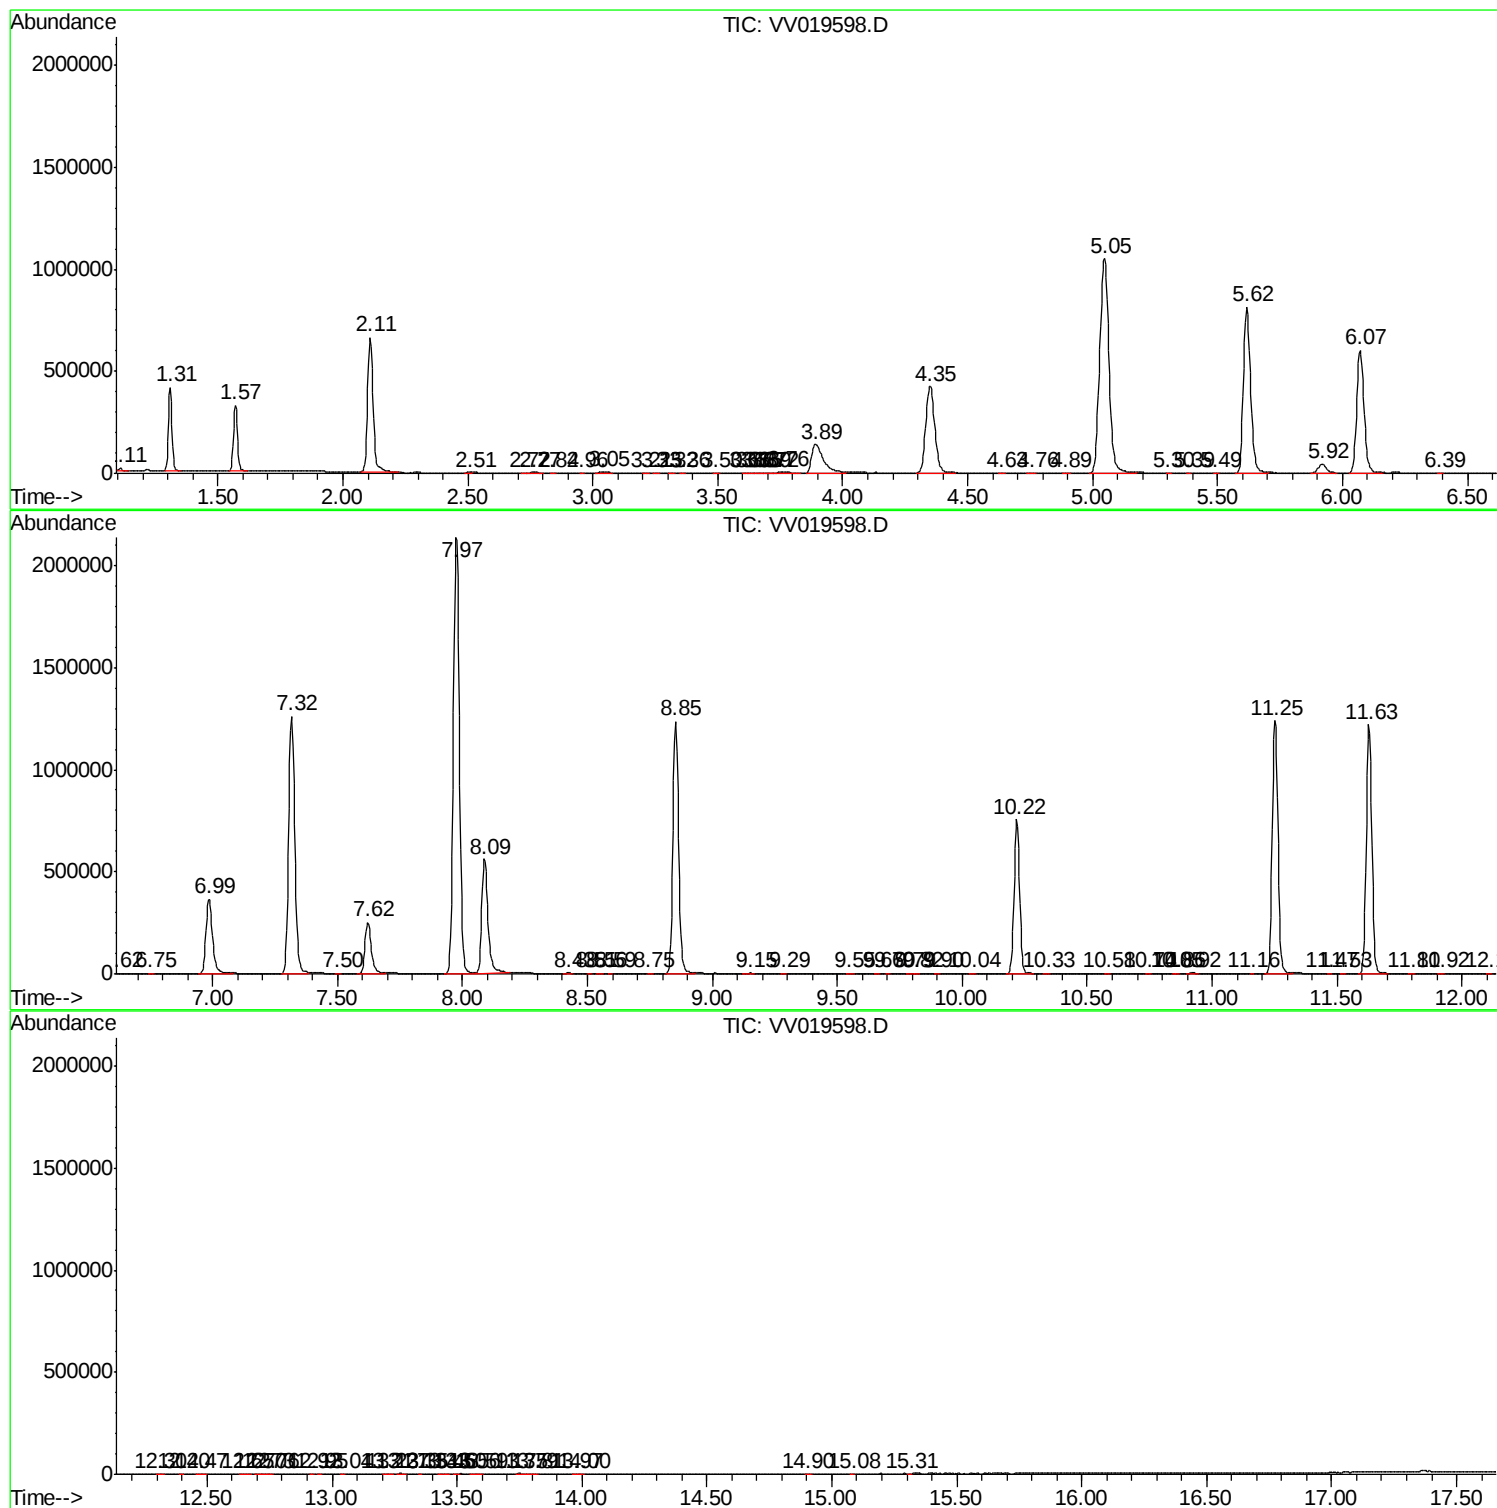

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121420\
Data File : VV019598.D
Acq On : 14 Dec 2020 12:40
Operator : SY/MD
Sample : L4928-03 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4M0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121420\
Data File : VV019598.D
Acq On : 14 Dec 2020 12:40
Operator : SY/MD
Sample : L4928-03 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4M0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc