

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019605.D
 Acq On : 14 Dec 2020 15:28
 Operator : SY/MD
 Sample : L4928-04DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	370950	361460	14.06%	1.746%
2	1.569	142	149	161	rBV	296367	337374	13.13%	1.630%
3	2.110	308	317	354	rVB	607081	941741	36.64%	4.549%
4	2.942	574	576	579	rBV2	495	360	0.01%	0.002%
5	3.000	592	594	596	rBV2	408	147	0.01%	0.001%
6	3.190	650	653	654	rBV3	705	368	0.01%	0.002%
7	3.245	669	670	675	rVB3	425	236	0.01%	0.001%
8	3.267	675	677	679	rBV2	346	161	0.01%	0.001%
9	3.280	679	681	684	rBV3	546	335	0.01%	0.002%
10	3.447	731	733	734	rBV2	334	135	0.01%	0.001%
11	3.486	741	745	747	rVB2	461	342	0.01%	0.002%
12	3.499	747	749	750	rBV2	217	120	0.00%	0.001%
13	3.527	754	758	761	rBB3	784	454	0.02%	0.002%
14	3.544	761	763	765	rBV2	359	201	0.01%	0.001%
15	3.592	776	778	779	rBV	390	167	0.01%	0.001%
16	3.624	785	788	794	rBV4	716	620	0.02%	0.003%
17	3.650	794	796	799	rBV2	439	216	0.01%	0.001%
18	3.714	812	816	818	rBV3	554	316	0.01%	0.002%
19	3.769	821	833	845	rBV5	2073	4773	0.19%	0.023%
20	3.897	861	873	915	rBV2	152931	501486	19.51%	2.422%
21	4.354	1000	1015	1044	rVB	409902	997599	38.81%	4.819%
22	4.971	1204	1207	1212	rVB4	555	452	0.02%	0.002%
23	5.052	1212	1232	1260	rBV2	1005852	2570411	100.00%	12.416%
24	5.531	1379	1381	1383	rBV4	530	272	0.01%	0.001%
25	5.621	1396	1409	1448	rBV	792400	1590969	61.90%	7.685%
26	5.849	1478	1480	1482	rVB2	611	240	0.01%	0.001%
27	5.916	1490	1501	1518	rVB5	14895	37217	1.45%	0.180%
28	6.023	1529	1534	1535	rBV5	970	743	0.03%	0.004%
29	6.074	1536	1550	1581	rVV	573774	1163968	45.28%	5.622%
30	6.302	1618	1621	1624	rBV4	498	369	0.01%	0.002%
31	6.318	1624	1626	1628	rBV2	545	234	0.01%	0.001%
32	6.373	1640	1643	1646	rBV4	577	494	0.02%	0.002%
33	6.434	1659	1662	1665	rBV2	489	363	0.01%	0.002%
34	6.466	1669	1672	1675	rVB2	607	384	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019605.D
 Acq On : 14 Dec 2020 15:28
 Operator : SY/MD
 Sample : L4928-04DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.486	1676	1678	1680	rVV	450	192	0.01%	0.001%
36	6.518	1684	1688	1689	rBV3	591	343	0.01%	0.002%
37	6.531	1689	1692	1700	rVB5	568	698	0.03%	0.003%
38	6.563	1700	1702	1706	rVB3	636	366	0.01%	0.002%
39	6.585	1706	1709	1712	rBV2	680	439	0.02%	0.002%
40	6.714	1746	1749	1751	rBV2	828	560	0.02%	0.003%
41	6.846	1783	1790	1791	rBV4	771	734	0.03%	0.004%
42	6.865	1794	1796	1797	rVV	421	134	0.01%	0.001%
43	6.884	1801	1802	1803	rVB	118	23	0.00%	0.000%
44	6.891	1803	1804	1806	rBV	262	120	0.00%	0.001%
45	6.916	1808	1812	1815	rBV2	584	382	0.01%	0.002%
46	6.929	1815	1816	1817	rBV	251	76	0.00%	0.000%
47	6.987	1822	1834	1864	rBV	342117	626067	24.36%	3.024%
48	7.318	1924	1937	1962	rBV	1168166	2041884	79.44%	9.863%
49	7.624	2022	2032	2066	rBV	244404	420670	16.37%	2.032%
50	7.881	2108	2112	2114	rBV3	515	447	0.02%	0.002%
51	7.977	2129	2142	2166	rBV	721170	1216610	47.33%	5.876%
52	8.090	2167	2177	2210	rBV	610593	1056035	41.08%	5.101%
53	8.418	2274	2279	2283	rBV7	1387	1630	0.06%	0.008%
54	8.627	2339	2344	2347	rBV3	853	1053	0.04%	0.005%
55	8.685	2359	2362	2364	rBV3	692	392	0.02%	0.002%
56	8.855	2402	2415	2445	rBV	1195790	1934080	75.24%	9.342%
57	9.016	2459	2465	2472	rBV6	1083	1572	0.06%	0.008%
58	9.103	2490	2492	2494	rVB2	687	274	0.01%	0.001%
59	9.379	2576	2578	2581	rBV3	388	194	0.01%	0.001%
60	9.415	2587	2589	2592	rVB4	699	337	0.01%	0.002%
61	9.476	2602	2608	2610	rBV2	918	816	0.03%	0.004%
62	9.521	2619	2622	2624	rBV2	401	282	0.01%	0.001%
63	9.534	2624	2626	2630	rVV3	565	437	0.02%	0.002%
64	9.559	2630	2634	2637	rVV3	790	626	0.02%	0.003%
65	9.572	2637	2638	2641	rVB2	767	320	0.01%	0.002%
66	9.588	2641	2643	2644	rBV	551	184	0.01%	0.001%
67	9.601	2645	2647	2651	rBV3	429	234	0.01%	0.001%
68	9.685	2671	2673	2675	rVB	317	111	0.00%	0.001%
69	9.736	2685	2689	2691	rBV2	307	261	0.01%	0.001%
70	9.817	2712	2714	2716	rBV2	702	352	0.01%	0.002%
71	10.013	2773	2775	2777	rBV2	317	127	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019605.D
 Acq On : 14 Dec 2020 15:28
 Operator : SY/MD
 Sample : L4928-04DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.042	2782	2784	2787	rBV2	362	217	0.01%	0.001%
73	10.219	2827	2839	2859	rBV	747404	1183552	46.05%	5.717%
74	10.440	2906	2908	2910	rBV2	394	218	0.01%	0.001%
75	10.495	2922	2925	2927	rBV2	363	215	0.01%	0.001%
76	10.543	2937	2940	2943	rBV3	551	391	0.02%	0.002%
77	10.701	2987	2989	2991	rBV	233	89	0.00%	0.000%
78	10.804	3019	3021	3022	rBV	599	236	0.01%	0.001%
79	10.852	3032	3036	3038	rBV	1043	713	0.03%	0.003%
80	11.035	3092	3093	3097	rVB2	362	153	0.01%	0.001%
81	11.061	3097	3101	3103	rBV3	932	592	0.02%	0.003%
82	11.096	3108	3112	3115	rVB2	747	590	0.02%	0.003%
83	11.122	3115	3120	3126	rBV3	538	714	0.03%	0.003%
84	11.167	3132	3134	3136	rBV2	753	382	0.01%	0.002%
85	11.254	3147	3161	3182	rBV	1208264	1863097	72.48%	8.999%
86	11.630	3265	3278	3298	rBV	1173454	1825054	71.00%	8.815%
87	12.280	3478	3480	3482	rBV	554	343	0.01%	0.002%
88	12.302	3485	3487	3489	rBV2	272	151	0.01%	0.001%
89	12.440	3526	3530	3532	rBV2	1075	717	0.03%	0.003%
90	12.514	3550	3553	3555	rBV3	637	419	0.02%	0.002%
91	12.916	3675	3678	3679	rBV	662	416	0.02%	0.002%
92	12.964	3690	3693	3694	rBV	618	356	0.01%	0.002%
93	13.013	3704	3708	3709	rBV2	866	661	0.03%	0.003%


Sum of corrected areas: 20703065

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121420\
Data File : VV019605.D
Acq On : 14 Dec 2020 15:28
Operator : SY/MD
Sample : L4928-04DL 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4M1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

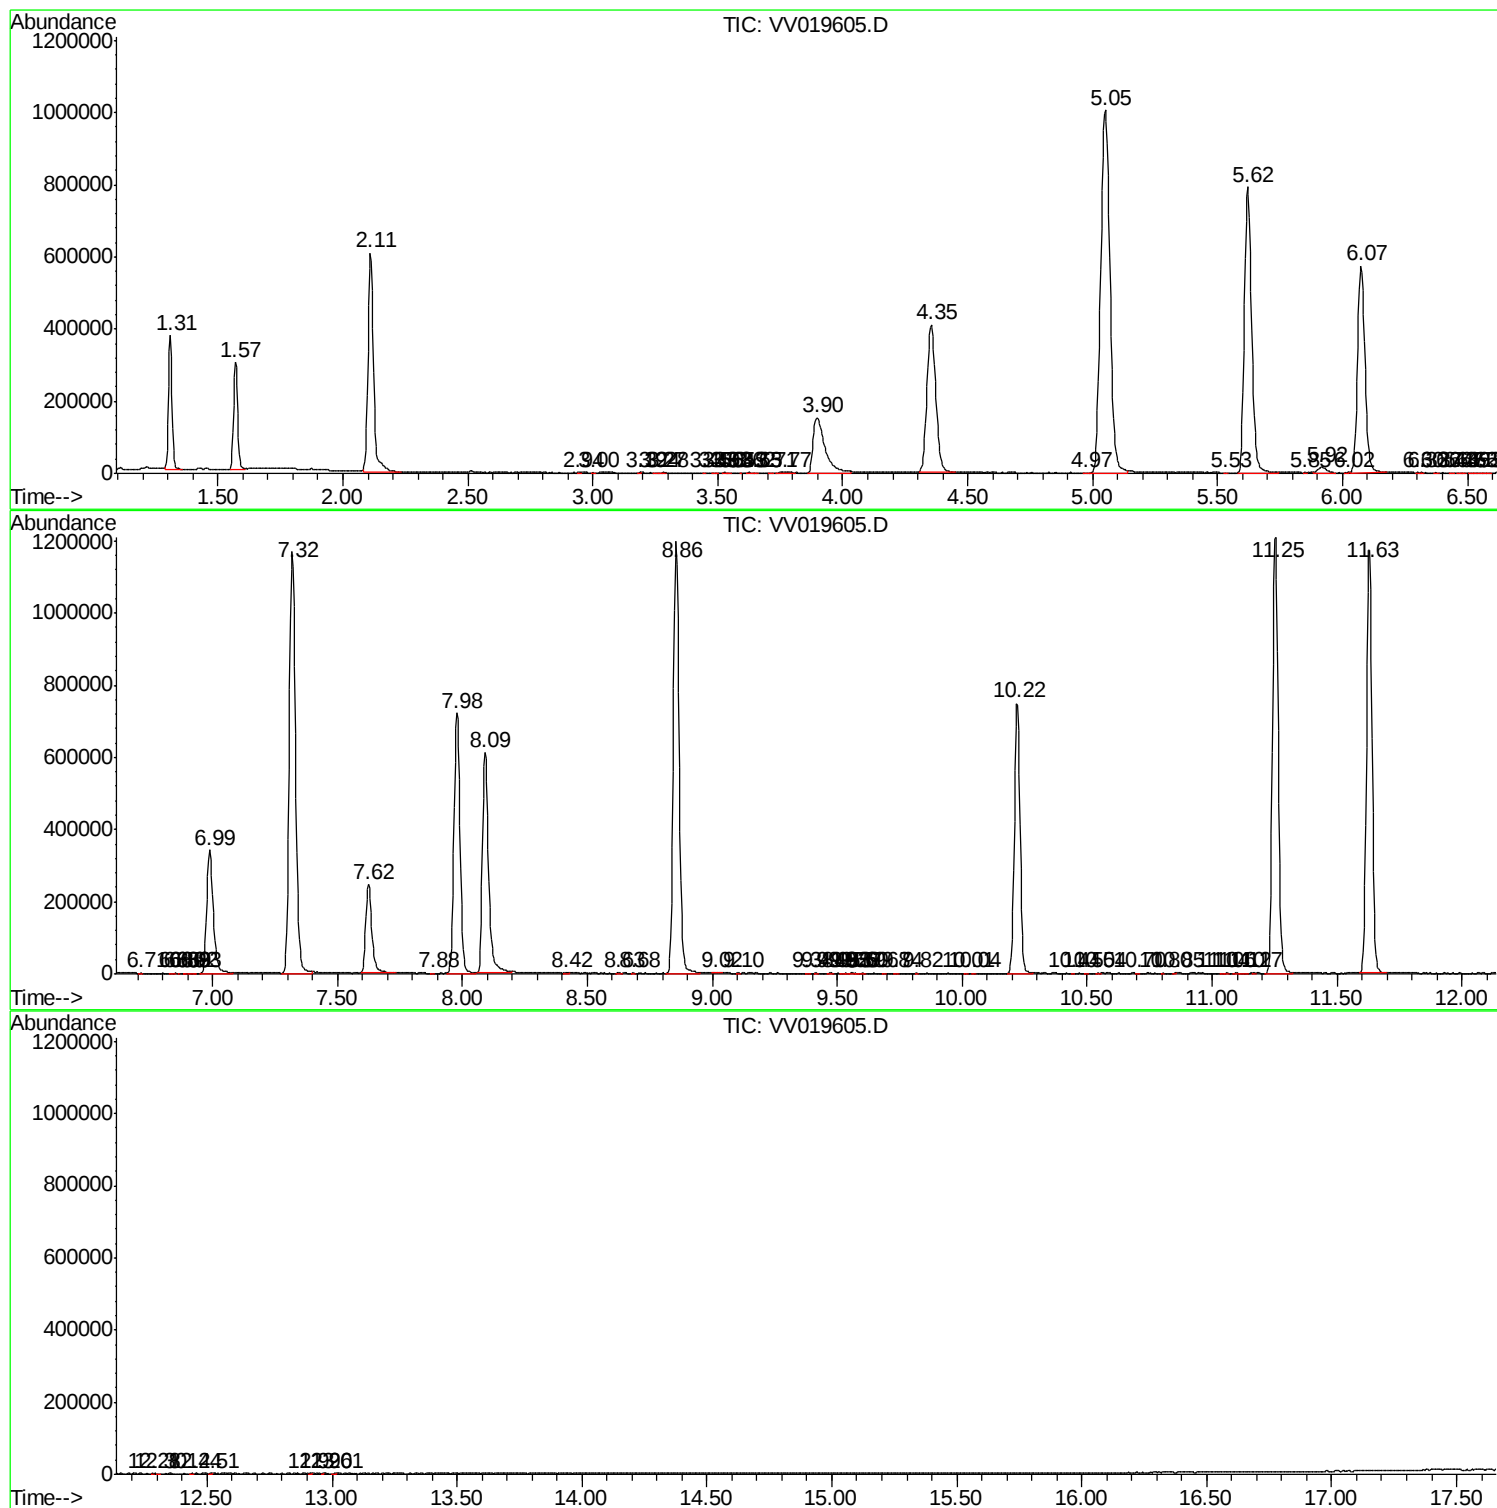

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121420\
Data File : VV019605.D
Acq On : 14 Dec 2020 15:28
Operator : SY/MD
Sample : L4928-04DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4M1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121420\
Data File : VV019605.D
Acq On : 14 Dec 2020 15:28
Operator : SY/MD
Sample : L4928-04DL 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4M1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc