

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019613.D
 Acq On : 14 Dec 2020 18:41
 Operator : SY/MD
 Sample : L4928-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4J0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	362848	366903	14.52%	1.941%
2	1.569	142	149	165	rBV	300855	341774	13.53%	1.808%
3	2.110	308	317	360	rVB	612052	973270	38.53%	5.149%
4	2.942	574	576	578	rBV2	478	208	0.01%	0.001%
5	2.997	592	593	596	rVB3	423	194	0.01%	0.001%
6	3.048	598	609	622	rVV3	10705	21945	0.87%	0.116%
7	3.177	647	649	653	rBV2	558	331	0.01%	0.002%
8	3.228	662	665	667	rBV3	576	361	0.01%	0.002%
9	3.277	676	680	682	rBV4	446	326	0.01%	0.002%
10	3.312	689	691	694	rBV3	276	121	0.00%	0.001%
11	3.367	705	708	712	rBV3	846	814	0.03%	0.004%
12	3.405	716	720	721	rBV	328	235	0.01%	0.001%
13	3.437	727	730	734	rBV3	614	394	0.02%	0.002%
14	3.460	734	737	743	rVB4	613	474	0.02%	0.003%
15	3.502	746	750	751	rBV2	386	193	0.01%	0.001%
16	3.515	751	754	755	rBV	453	275	0.01%	0.001%
17	3.582	772	775	779	rVB3	435	361	0.01%	0.002%
18	3.605	779	782	784	rBV2	474	356	0.01%	0.002%
19	3.640	790	793	796	rBV2	424	289	0.01%	0.002%
20	3.656	796	798	805	rVB3	642	618	0.02%	0.003%
21	3.685	805	807	808	rBV	266	103	0.00%	0.001%
22	3.704	811	813	814	rBV	221	71	0.00%	0.000%
23	3.762	820	831	833	rBV7	4334	6563	0.26%	0.035%
24	3.826	849	851	855	rVB3	413	252	0.01%	0.001%
25	3.846	855	857	860	rVB2	173	95	0.00%	0.001%
26	3.894	860	872	911	rBV	147163	455219	18.02%	2.408%
27	4.354	996	1015	1048	rBV	401647	995820	39.42%	5.268%
28	4.704	1119	1124	1127	rBV7	568	588	0.02%	0.003%
29	4.756	1138	1140	1141	rBV	492	204	0.01%	0.001%
30	4.785	1146	1149	1150	rBV2	286	180	0.01%	0.001%
31	4.862	1171	1173	1174	rBV	369	127	0.01%	0.001%
32	4.894	1178	1183	1185	rBV3	722	654	0.03%	0.003%
33	4.929	1192	1194	1196	rVB2	521	194	0.01%	0.001%
34	4.958	1201	1203	1204	rBV	300	92	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019613.D
 Acq On : 14 Dec 2020 18:41
 Operator : SY/MD
 Sample : L4928-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4J0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	4.981	1207	1210	1211	rBV2	461	266	0.01%	0.001%
36	5.051	1213	1232	1264	rBV2	980658	2526181	100.00%	13.363%
37	5.621	1396	1409	1437	rBV	753100	1504917	59.57%	7.961%
38	5.910	1486	1499	1513	rBV3	18295	40408	1.60%	0.214%
39	5.981	1518	1521	1523	rBV3	932	516	0.02%	0.003%
40	6.074	1536	1550	1577	rBV	560459	1137256	45.02%	6.016%
41	6.405	1650	1653	1655	rVB	525	258	0.01%	0.001%
42	6.444	1663	1665	1669	rBV2	763	485	0.02%	0.003%
43	6.511	1685	1686	1687	rVB	458	88	0.00%	0.000%
44	6.524	1687	1690	1697	rBV3	427	422	0.02%	0.002%
45	6.736	1755	1756	1761	rVB2	700	440	0.02%	0.002%
46	6.762	1762	1764	1765	rVV	315	85	0.00%	0.000%
47	6.788	1769	1772	1774	rBV2	683	455	0.02%	0.002%
48	6.817	1780	1781	1784	rBV2	288	169	0.01%	0.001%
49	6.852	1788	1792	1794	rVB3	551	405	0.02%	0.002%
50	6.868	1794	1797	1802	rBV3	632	612	0.02%	0.003%
51	6.990	1822	1835	1860	rBV	328064	596938	23.63%	3.158%
52	7.318	1924	1937	1969	rBV	1172575	2025595	80.18%	10.715%
53	7.624	2021	2032	2058	rBV	230127	401750	15.90%	2.125%
54	7.871	2106	2109	2110	rBV2	451	243	0.01%	0.001%
55	8.045	2162	2163	2164	rBV2	495	155	0.01%	0.001%
56	8.090	2167	2177	2209	rVV	577674	1016933	40.26%	5.380%
57	8.688	2360	2363	2364	rBV3	472	287	0.01%	0.002%
58	8.855	2402	2415	2437	rBV	1131669	1813823	71.80%	9.595%
59	9.244	2534	2536	2537	rBV	220	87	0.00%	0.000%
60	9.302	2551	2554	2558	rVB2	961	649	0.03%	0.003%
61	9.328	2559	2562	2563	rVB3	493	206	0.01%	0.001%
62	9.354	2565	2570	2573	rBV5	710	648	0.03%	0.003%
63	9.395	2580	2583	2584	rBV2	946	422	0.02%	0.002%
64	9.469	2602	2606	2607	rBV	683	330	0.01%	0.002%
65	9.514	2618	2620	2626	rVB4	843	678	0.03%	0.004%
66	9.547	2626	2630	2633	rBV4	804	834	0.03%	0.004%
67	9.637	2655	2658	2660	rVB2	406	214	0.01%	0.001%
68	9.656	2660	2664	2668	rBV4	532	575	0.02%	0.003%
69	9.707	2675	2680	2681	rBV3	512	512	0.02%	0.003%
70	9.730	2685	2687	2690	rBV2	488	310	0.01%	0.002%
71	9.836	2718	2720	2722	rBV	518	310	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019613.D
 Acq On : 14 Dec 2020 18:41
 Operator : SY/MD
 Sample : L4928-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4J0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	9.932	2747	2750	2752	rBV4	635	523	0.02%	0.003%
73	9.961	2757	2759	2762	rVV	457	205	0.01%	0.001%
74	10.145	2808	2816	2818	rBV6	719	1041	0.04%	0.006%
75	10.219	2827	2839	2859	rBV	703957	1111245	43.99%	5.878%
76	10.543	2937	2940	2942	rBV4	888	646	0.03%	0.003%
77	10.694	2984	2987	2990	rBV	479	324	0.01%	0.002%
78	10.755	3002	3006	3008	rVB2	615	427	0.02%	0.002%
79	10.781	3008	3014	3015	rBV3	664	546	0.02%	0.003%
80	10.929	3056	3060	3063	rBV3	452	352	0.01%	0.002%
81	10.958	3066	3069	3072	rBV2	333	240	0.01%	0.001%
82	10.974	3072	3074	3076	rBV2	312	92	0.00%	0.000%
83	11.051	3093	3098	3099	rBV5	1307	1057	0.04%	0.006%
84	11.122	3119	3120	3125	rBV2	403	303	0.01%	0.002%
85	11.254	3147	3161	3183	rBV	1129619	1749375	69.25%	9.254%
86	11.505	3237	3239	3242	rBV3	538	362	0.01%	0.002%
87	11.627	3265	3277	3297	rBV	1155097	1789015	70.82%	9.464%
88	11.913	3363	3366	3367	rBV2	581	336	0.01%	0.002%
89	11.987	3386	3389	3390	rBV2	616	359	0.01%	0.002%
90	12.344	3494	3500	3501	rBV	602	549	0.02%	0.003%
91	12.675	3600	3603	3605	rBV3	706	465	0.02%	0.002%
92	12.929	3679	3682	3683	rBV2	800	370	0.01%	0.002%
93	13.315	3800	3802	3803	rBV	486	233	0.01%	0.001%
94	13.755	3937	3939	3942	rBV2	741	490	0.02%	0.003%
95	13.804	3952	3954	3955	rBV2	589	227	0.01%	0.001%
96	14.083	4037	4041	4042	rBV2	1092	808	0.03%	0.004%


Sum of corrected areas: 18903656

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121420\
Data File : VV019613.D
Acq On : 14 Dec 2020 18:41
Operator : SY/MD
Sample : L4928-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4J0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

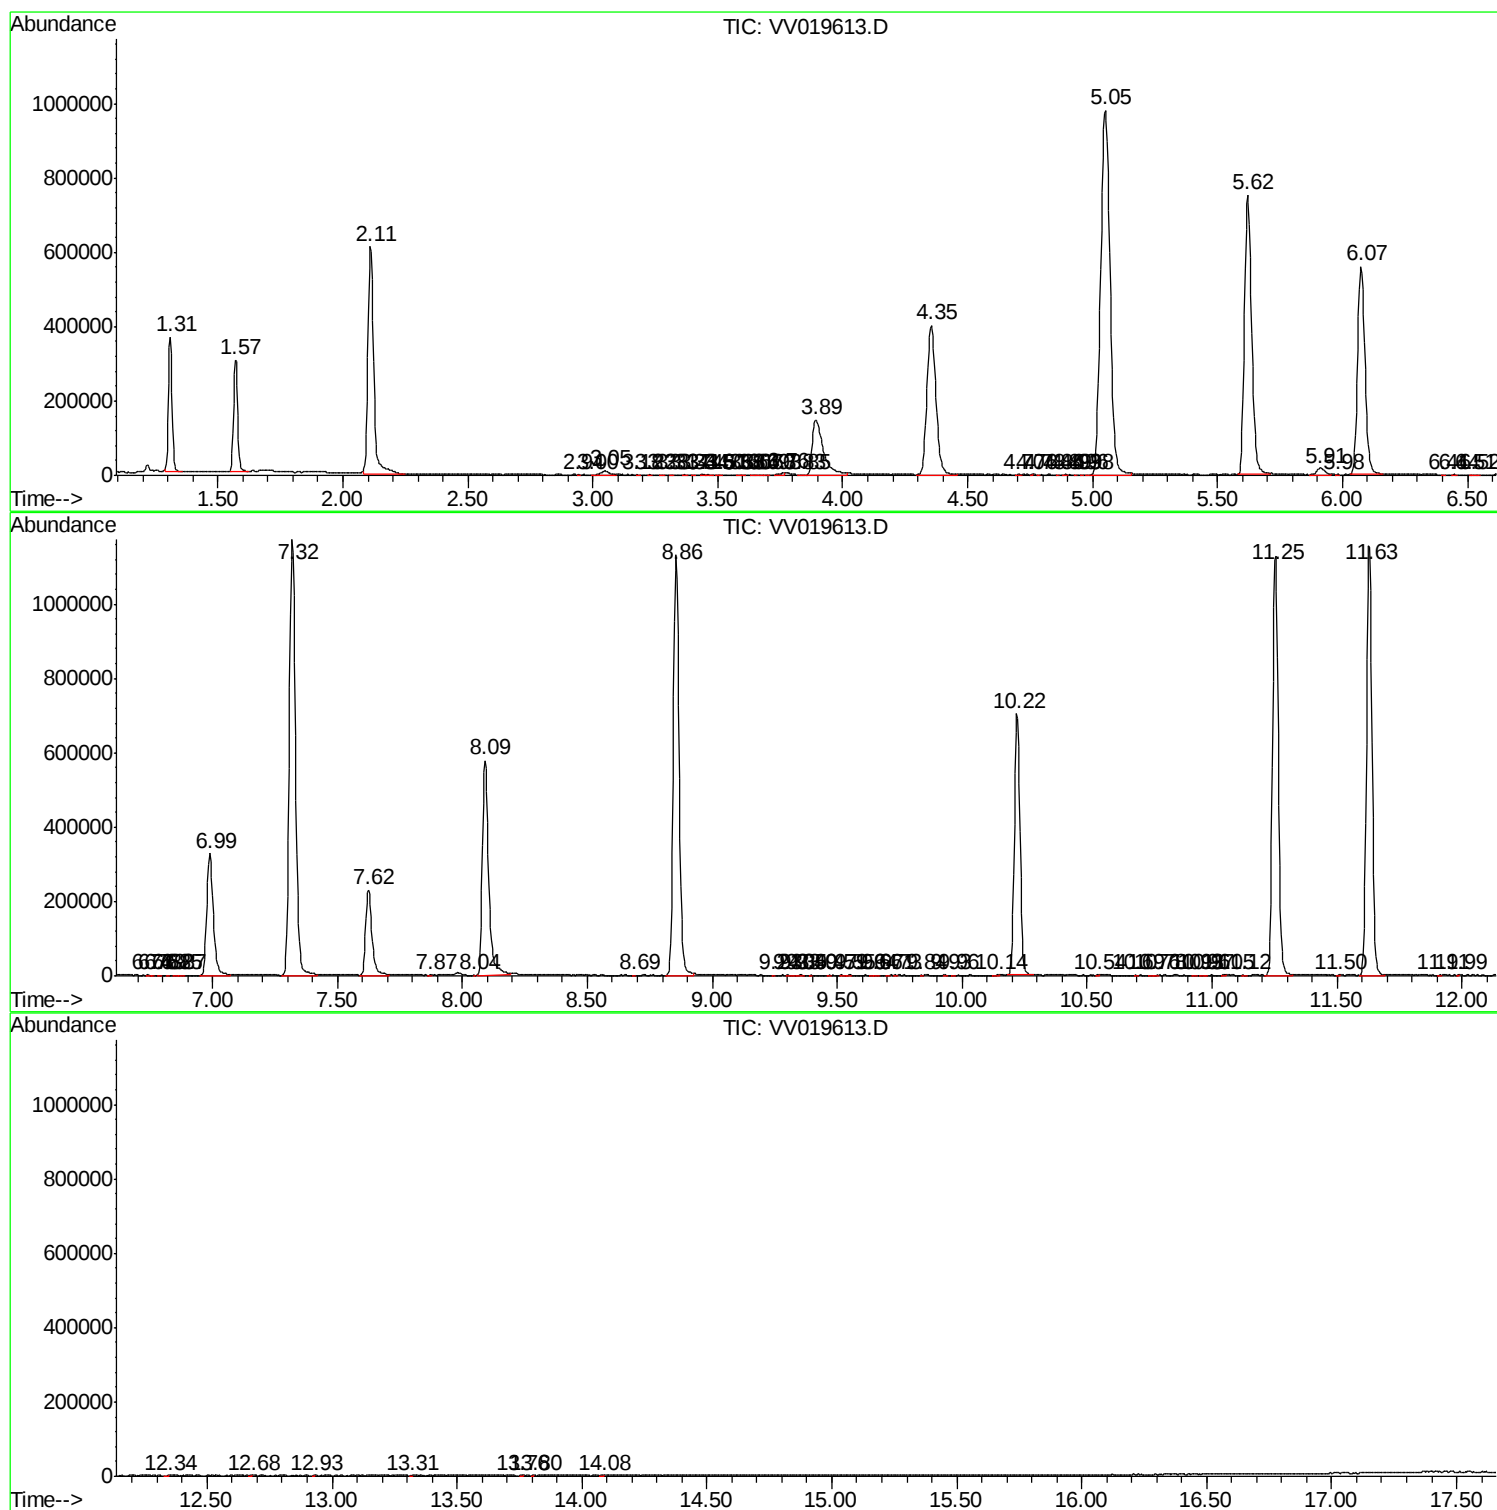

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121420\
Data File : VV019613.D
Acq On : 14 Dec 2020 18:41
Operator : SY/MD
Sample : L4928-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4J0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121420\
Data File : VV019613.D
Acq On : 14 Dec 2020 18:41
Operator : SY/MD
Sample : L4928-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4J0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc