

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019625.D
 Acq On : 15 Dec 2020 00:17
 Operator : SY/MD
 Sample : L5024-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	85	rVB	330207	327560	13.72%	1.814%
2	1.569	141	149	161	rBV	273669	308813	12.93%	1.711%
3	2.110	307	317	362	rVB	557557	898865	37.64%	4.979%
4	2.946	572	577	581	rBV3	875	1048	0.04%	0.006%
5	2.968	582	584	589	rVB2	881	607	0.03%	0.003%
6	3.042	599	607	611	rBV5	1318	1909	0.08%	0.011%
7	3.113	627	629	633	rVV3	629	443	0.02%	0.002%
8	3.132	633	635	640	rVB4	606	480	0.02%	0.003%
9	3.505	746	751	754	rBV4	687	632	0.03%	0.004%
10	3.675	795	804	808	rBV4	752	1215	0.05%	0.007%
11	3.782	834	837	843	rVB4	635	652	0.03%	0.004%
12	3.901	857	874	904	rBV2	149730	527820	22.10%	2.924%
13	4.354	997	1015	1042	rBV	386297	957403	40.09%	5.303%
14	4.849	1167	1169	1174	rVV4	483	452	0.02%	0.003%
15	4.891	1177	1182	1190	rVB8	732	1207	0.05%	0.007%
16	4.939	1190	1197	1198	rBV3	610	624	0.03%	0.003%
17	5.052	1213	1232	1269	rBV2	929341	2388034	100.00%	13.228%
18	5.331	1315	1319	1322	rBV4	762	577	0.02%	0.003%
19	5.527	1378	1380	1384	rBV3	689	478	0.02%	0.003%
20	5.556	1384	1389	1394	rBV5	1166	1173	0.05%	0.006%
21	5.621	1396	1409	1442	rBV	717723	1430722	59.91%	7.925%
22	5.804	1463	1466	1469	rBV5	772	512	0.02%	0.003%
23	5.910	1488	1499	1513	rBV4	16081	35883	1.50%	0.199%
24	6.074	1535	1550	1574	rBV	535240	1083729	45.38%	6.003%
25	6.325	1620	1628	1631	rBV6	1235	1624	0.07%	0.009%
26	6.518	1685	1688	1689	rBV3	1051	629	0.03%	0.003%
27	6.540	1689	1695	1697	rBV4	1652	1925	0.08%	0.011%
28	6.624	1715	1721	1722	rBV5	1668	1427	0.06%	0.008%
29	6.862	1789	1795	1800	rBV6	632	783	0.03%	0.004%
30	6.987	1821	1834	1864	rBV	306280	559163	23.42%	3.097%
31	7.244	1908	1914	1916	rBV5	1207	1267	0.05%	0.007%
32	7.318	1923	1937	1956	rBV	1086761	1867661	78.21%	10.345%
33	7.624	2019	2032	2056	rBV	215937	377194	15.80%	2.089%
34	7.926	2119	2126	2129	rBV6	808	907	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019625.D
 Acq On : 15 Dec 2020 00:17
 Operator : SY/MD
 Sample : L5024-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	7.945	2129	2132	2135	rBV4	721	473	0.02%	0.003%
36	7.981	2135	2143	2151	rVB10	4674	8011	0.34%	0.044%
37	8.039	2155	2161	2167	rBV6	4310	6483	0.27%	0.036%
38	8.090	2167	2177	2211	rBV	547790	986813	41.32%	5.466%
39	8.251	2220	2227	2241	rVB6	10712	20547	0.86%	0.114%
40	8.492	2296	2302	2305	rBV4	514	556	0.02%	0.003%
41	8.563	2320	2324	2331	rBV4	684	689	0.03%	0.004%
42	8.675	2356	2359	2364	rBV5	549	590	0.02%	0.003%
43	8.711	2364	2370	2373	rBV4	587	648	0.03%	0.004%
44	8.765	2384	2387	2392	rVB4	569	439	0.02%	0.002%
45	8.855	2402	2415	2441	rBV	1086386	1734290	72.62%	9.607%
46	9.019	2462	2466	2469	rVV3	1348	1157	0.05%	0.006%
47	9.151	2498	2507	2515	rVV7	4531	7794	0.33%	0.043%
48	9.238	2531	2534	2538	rVB5	573	492	0.02%	0.003%
49	9.260	2538	2541	2544	rVB4	603	464	0.02%	0.003%
50	9.296	2546	2552	2556	rBV4	935	1080	0.05%	0.006%
51	9.322	2558	2560	2563	rVB3	949	544	0.02%	0.003%
52	9.376	2570	2577	2581	rBV4	1034	1290	0.05%	0.007%
53	9.402	2583	2585	2591	rVB4	578	450	0.02%	0.002%
54	9.431	2591	2594	2597	rBV	786	571	0.02%	0.003%
55	9.576	2624	2639	2648	rBV5	8163	16967	0.71%	0.094%
56	9.659	2663	2665	2669	rBV2	636	473	0.02%	0.003%
57	9.685	2669	2673	2676	rBV4	571	539	0.02%	0.003%
58	9.727	2683	2686	2688	rBV3	678	504	0.02%	0.003%
59	9.823	2707	2716	2728	rBV8	3480	6560	0.27%	0.036%
60	9.929	2744	2749	2750	rVV2	544	436	0.02%	0.002%
61	10.219	2826	2839	2856	rBV	681223	1077005	45.10%	5.966%
62	10.363	2881	2884	2888	rVB3	919	511	0.02%	0.003%
63	10.450	2903	2911	2916	rVV7	1444	2014	0.08%	0.011%
64	10.547	2934	2941	2943	rBV5	591	725	0.03%	0.004%
65	10.701	2984	2989	2993	rBV3	907	729	0.03%	0.004%
66	10.752	3001	3005	3008	rBV3	521	456	0.02%	0.003%
67	10.794	3015	3018	3024	rBV	17451	10311	0.43%	0.057%
68	10.932	3054	3061	3062	rBV3	4860	4629	0.19%	0.026%
69	11.051	3090	3098	3103	rBV8	1262	1908	0.08%	0.011%
70	11.093	3107	3111	3115	rBV2	1223	1003	0.04%	0.006%
71	11.157	3123	3131	3133	rBV6	3260	3362	0.14%	0.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019625.D
 Acq On : 15 Dec 2020 00:17
 Operator : SY/MD
 Sample : L5024-16
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	11.193	3139	3142	3146	rVB4	1055	878	0.04%	0.005%
73	11.254	3148	3161	3184	rBV	1090588	1649013	69.05%	9.134%
74	11.424	3210	3214	3218	rBV6	524	562	0.02%	0.003%
75	11.537	3241	3249	3258	rBV6	4003	7429	0.31%	0.041%
76	11.630	3265	3278	3301	rBV	1072881	1687572	70.67%	9.348%
77	11.894	3354	3360	3363	rBV4	945	997	0.04%	0.006%
78	12.026	3398	3401	3406	rVV3	734	729	0.03%	0.004%
79	12.354	3494	3503	3513	rVV6	4108	7141	0.30%	0.040%
80	12.608	3579	3582	3586	rBV2	679	556	0.02%	0.003%
81	12.662	3594	3599	3603	rBV3	991	1242	0.05%	0.007%
82	12.768	3628	3632	3634	rBV3	910	920	0.04%	0.005%
83	12.884	3662	3668	3670	rVV2	727	692	0.03%	0.004%
84	12.900	3670	3673	3675	rVB3	826	481	0.02%	0.003%
85	13.048	3716	3719	3723	rVB2	707	562	0.02%	0.003%
86	13.083	3727	3730	3734	rBV3	774	630	0.03%	0.003%
87	13.341	3806	3810	3813	rBV4	995	787	0.03%	0.004%
88	13.366	3813	3818	3822	rVV4	498	485	0.02%	0.003%
89	13.402	3825	3829	3834	rVB4	713	547	0.02%	0.003%
90	13.518	3860	3865	3866	rBV3	997	697	0.03%	0.004%
91	13.656	3904	3908	3913	rVB4	641	615	0.03%	0.003%
92	13.759	3936	3940	3942	rVB3	878	622	0.03%	0.003%
93	14.280	4099	4102	4107	rBV5	846	934	0.04%	0.005%
94	14.649	4214	4217	4219	rBV3	791	468	0.02%	0.003%
95	14.797	4260	4263	4266	rBV3	753	496	0.02%	0.003%
96	14.974	4314	4318	4321	rBV3	720	755	0.03%	0.004%
97	15.022	4330	4333	4336	rBV2	885	589	0.02%	0.003%
98	15.116	4360	4362	4365	rVB4	838	451	0.02%	0.002%
99	15.276	4409	4412	4415	rVB3	928	627	0.03%	0.003%
100	15.810	4575	4578	4579	rBV2	977	533	0.02%	0.003%


Sum of corrected areas: 18052941

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121420\
Data File : VV019625.D
Acq On : 15 Dec 2020 00:17
Operator : SY/MD
Sample : L5024-16
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

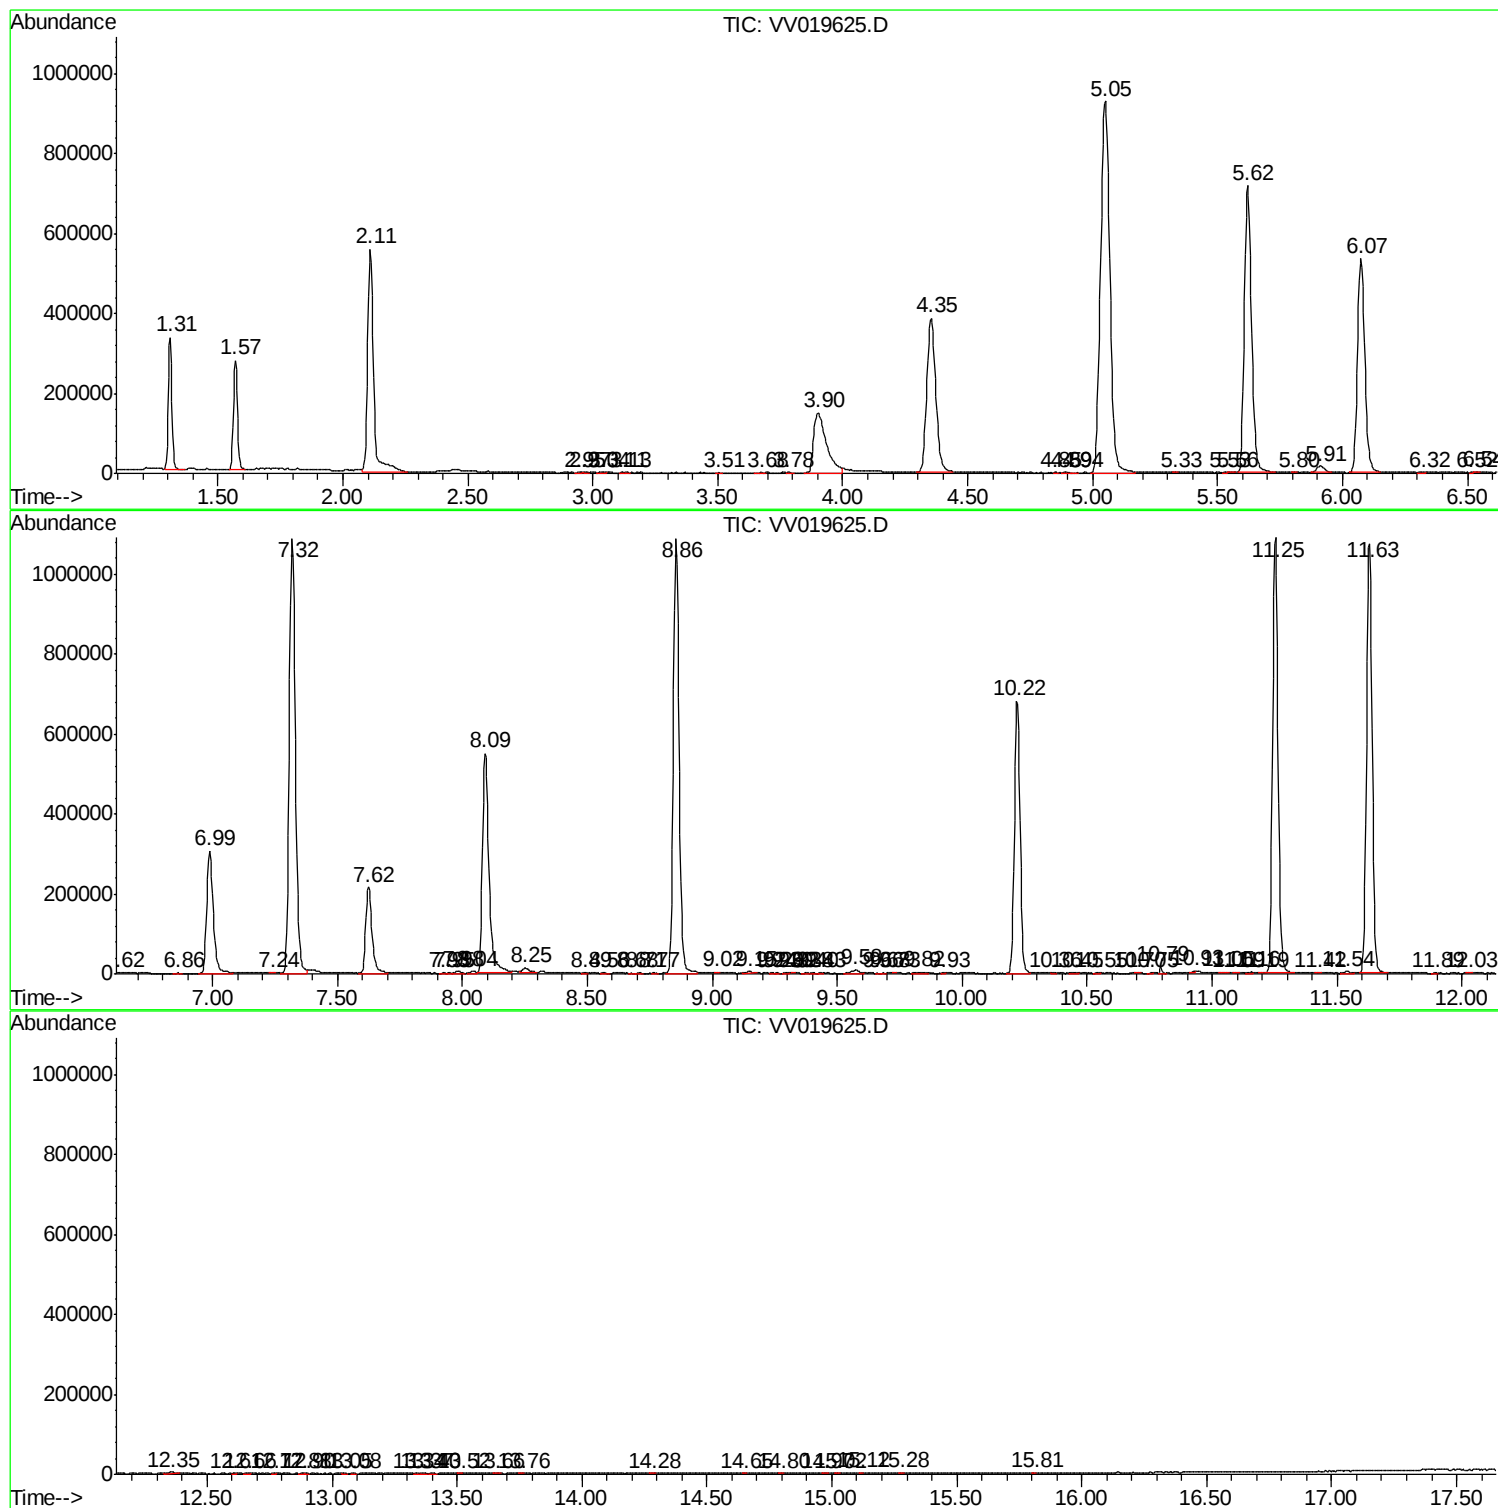

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121420\
Data File : VV019625.D
Acq On : 15 Dec 2020 00:17
Operator : SY/MD
Sample : L5024-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121420\
Data File : VV019625.D
Acq On : 15 Dec 2020 00:17
Operator : SY/MD
Sample : L5024-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc