

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019631.D
 Acq On : 15 Dec 2020 02:41
 Operator : SY/MD
 Sample : L5024-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	81	rVB	326459	316283	13.22%	1.684%
2	1.569	142	149	162	rBV	272525	308030	12.87%	1.641%
3	2.110	308	317	351	rVB2	558398	878958	36.73%	4.681%
4	2.868	551	553	556	rVB2	441	224	0.01%	0.001%
5	2.884	556	558	560	rBV3	560	342	0.01%	0.002%
6	2.965	581	583	585	rBV2	398	240	0.01%	0.001%
7	3.042	604	607	610	rBV3	1069	987	0.04%	0.005%
8	3.142	637	638	640	rVB	508	129	0.01%	0.001%
9	3.161	640	644	646	rBV2	566	475	0.02%	0.003%
10	3.257	671	674	676	rVB2	308	193	0.01%	0.001%
11	3.273	676	679	681	rBV3	435	292	0.01%	0.002%
12	3.309	688	690	693	rVB	569	287	0.01%	0.002%
13	3.344	699	701	705	rBV2	598	430	0.02%	0.002%
14	3.364	705	707	709	rVV	361	170	0.01%	0.001%
15	3.405	717	720	724	rBV2	511	452	0.02%	0.002%
16	3.425	724	726	727	rBV2	505	191	0.01%	0.001%
17	3.447	731	733	736	rBV2	469	332	0.01%	0.002%
18	3.482	741	744	749	rBV4	687	572	0.02%	0.003%
19	3.511	749	753	756	rBV3	447	314	0.01%	0.002%
20	3.531	756	759	764	rVB3	467	429	0.02%	0.002%
21	3.560	765	768	770	rBV	621	492	0.02%	0.003%
22	3.598	778	780	783	rBV	491	265	0.01%	0.001%
23	3.630	788	790	793	rBV3	237	97	0.00%	0.001%
24	3.663	798	800	801	rBV	380	184	0.01%	0.001%
25	3.711	812	815	817	rBV2	462	317	0.01%	0.002%
26	3.749	825	827	830	rBV3	414	235	0.01%	0.001%
27	3.765	830	832	833	rBV	276	85	0.00%	0.000%
28	3.778	833	836	838	rBV4	585	277	0.01%	0.001%
29	3.849	856	858	859	rBV4	393	172	0.01%	0.001%
30	3.859	859	861	862	rVV2	510	193	0.01%	0.001%
31	3.900	862	874	914	rVV	144766	505736	21.14%	2.693%
32	4.354	999	1015	1042	rBV	386887	943107	39.41%	5.023%
33	4.701	1120	1123	1126	rVB3	894	487	0.02%	0.003%
34	4.759	1135	1141	1147	rVB7	776	996	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019631.D
 Acq On : 15 Dec 2020 02:41
 Operator : SY/MD
 Sample : L5024-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	4.945	1195	1199	1203	rVB4	694	676	0.03%	0.004%
36	4.968	1203	1206	1207	rBV3	369	188	0.01%	0.001%
37	5.052	1214	1232	1268	rBV2	935929	2392791	100.00%	12.744%
38	5.360	1326	1328	1329	rBV2	596	252	0.01%	0.001%
39	5.621	1396	1409	1434	rBV	734049	1458819	60.97%	7.769%
40	5.920	1487	1502	1531	rBV	408775	825775	34.51%	4.398%
41	6.074	1536	1550	1579	rVV	539302	1089502	45.53%	5.802%
42	6.283	1613	1615	1617	rBV2	503	259	0.01%	0.001%
43	6.322	1625	1627	1628	rBV2	661	245	0.01%	0.001%
44	6.470	1670	1673	1674	rBV2	712	425	0.02%	0.002%
45	6.553	1697	1699	1700	rBV	276	70	0.00%	0.000%
46	6.727	1752	1753	1754	rBV	305	106	0.00%	0.001%
47	6.830	1782	1785	1789	rVB4	712	543	0.02%	0.003%
48	6.849	1789	1791	1794	rBV2	254	159	0.01%	0.001%
49	6.871	1795	1798	1801	rBV3	627	474	0.02%	0.003%
50	6.904	1805	1808	1810	rBV3	594	283	0.01%	0.002%
51	6.987	1822	1834	1858	rBV	306959	558124	23.33%	2.972%
52	7.318	1924	1937	1969	rBV	1086668	1887681	78.89%	10.053%
53	7.624	2022	2032	2058	rBV	214284	373282	15.60%	1.988%
54	7.839	2095	2099	2102	rBV3	876	797	0.03%	0.004%
55	7.981	2138	2143	2154	rVB7	4144	6454	0.27%	0.034%
56	8.090	2163	2177	2211	rBV	541146	974487	40.73%	5.190%
57	8.669	2353	2357	2360	rBV4	590	402	0.02%	0.002%
58	8.791	2391	2395	2398	rBV2	565	419	0.02%	0.002%
59	8.807	2398	2400	2403	rBV3	562	367	0.02%	0.002%
60	8.855	2403	2415	2436	rBV	1101773	1770611	74.00%	9.430%
61	9.238	2532	2534	2537	rBV2	538	373	0.02%	0.002%
62	9.283	2545	2548	2549	rBV2	516	246	0.01%	0.001%
63	9.325	2559	2561	2563	rBV2	413	240	0.01%	0.001%
64	9.434	2590	2595	2596	rBV2	494	411	0.02%	0.002%
65	9.579	2638	2640	2642	rVB	542	175	0.01%	0.001%
66	9.598	2642	2646	2648	rBV2	502	482	0.02%	0.003%
67	9.672	2668	2669	2670	rBV	382	132	0.01%	0.001%
68	9.714	2681	2682	2683	rBV	213	63	0.00%	0.000%
69	9.730	2685	2687	2688	rBV	414	170	0.01%	0.001%
70	9.781	2701	2703	2708	rVB3	798	506	0.02%	0.003%
71	9.813	2708	2713	2715	rBV2	456	447	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019631.D
 Acq On : 15 Dec 2020 02:41
 Operator : SY/MD
 Sample : L5024-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.045	2783	2785	2787	rBV2	336	203	0.01%	0.001%
73	10.093	2798	2800	2802	rBV2	318	161	0.01%	0.001%
74	10.151	2815	2818	2820	rBV3	459	270	0.01%	0.001%
75	10.219	2827	2839	2861	rBV	697791	1090185	45.56%	5.806%
76	10.415	2898	2900	2901	rBV2	340	152	0.01%	0.001%
77	10.569	2945	2948	2949	rBV3	578	315	0.01%	0.002%
78	10.685	2982	2984	2986	rBV	454	273	0.01%	0.001%
79	10.781	3011	3014	3016	rBV2	685	465	0.02%	0.002%
80	10.881	3042	3045	3046	rBV	514	251	0.01%	0.001%
81	10.968	3070	3072	3074	rBV	486	317	0.01%	0.002%
82	11.022	3086	3089	3092	rBV2	567	386	0.02%	0.002%
83	11.254	3149	3161	3180	rBV	1099764	1683109	70.34%	8.964%
84	11.460	3223	3225	3227	rBV	402	142	0.01%	0.001%
85	11.550	3247	3253	3255	rBV3	1720	1402	0.06%	0.007%
86	11.630	3266	3278	3298	rBV	1094967	1686410	70.48%	8.982%
87	11.890	3356	3359	3364	rBV5	638	639	0.03%	0.003%
88	12.016	3396	3398	3399	rBV	500	200	0.01%	0.001%
89	12.093	3420	3422	3424	rBV2	478	198	0.01%	0.001%
90	12.148	3433	3439	3441	rBV3	491	485	0.02%	0.003%
91	12.260	3471	3474	3479	rBV5	825	830	0.03%	0.004%
92	12.450	3531	3533	3537	rBV2	588	476	0.02%	0.003%
93	13.726	3928	3930	3934	rBV2	754	571	0.02%	0.003%
94	13.797	3950	3952	3955	rVB2	664	259	0.01%	0.001%
95	13.906	3984	3986	3988	rBV2	595	354	0.01%	0.002%


Sum of corrected areas: 18776462

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
Data File : VV019631.D
Acq On : 15 Dec 2020 02:41
Operator : SY/MD
Sample : L5024-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

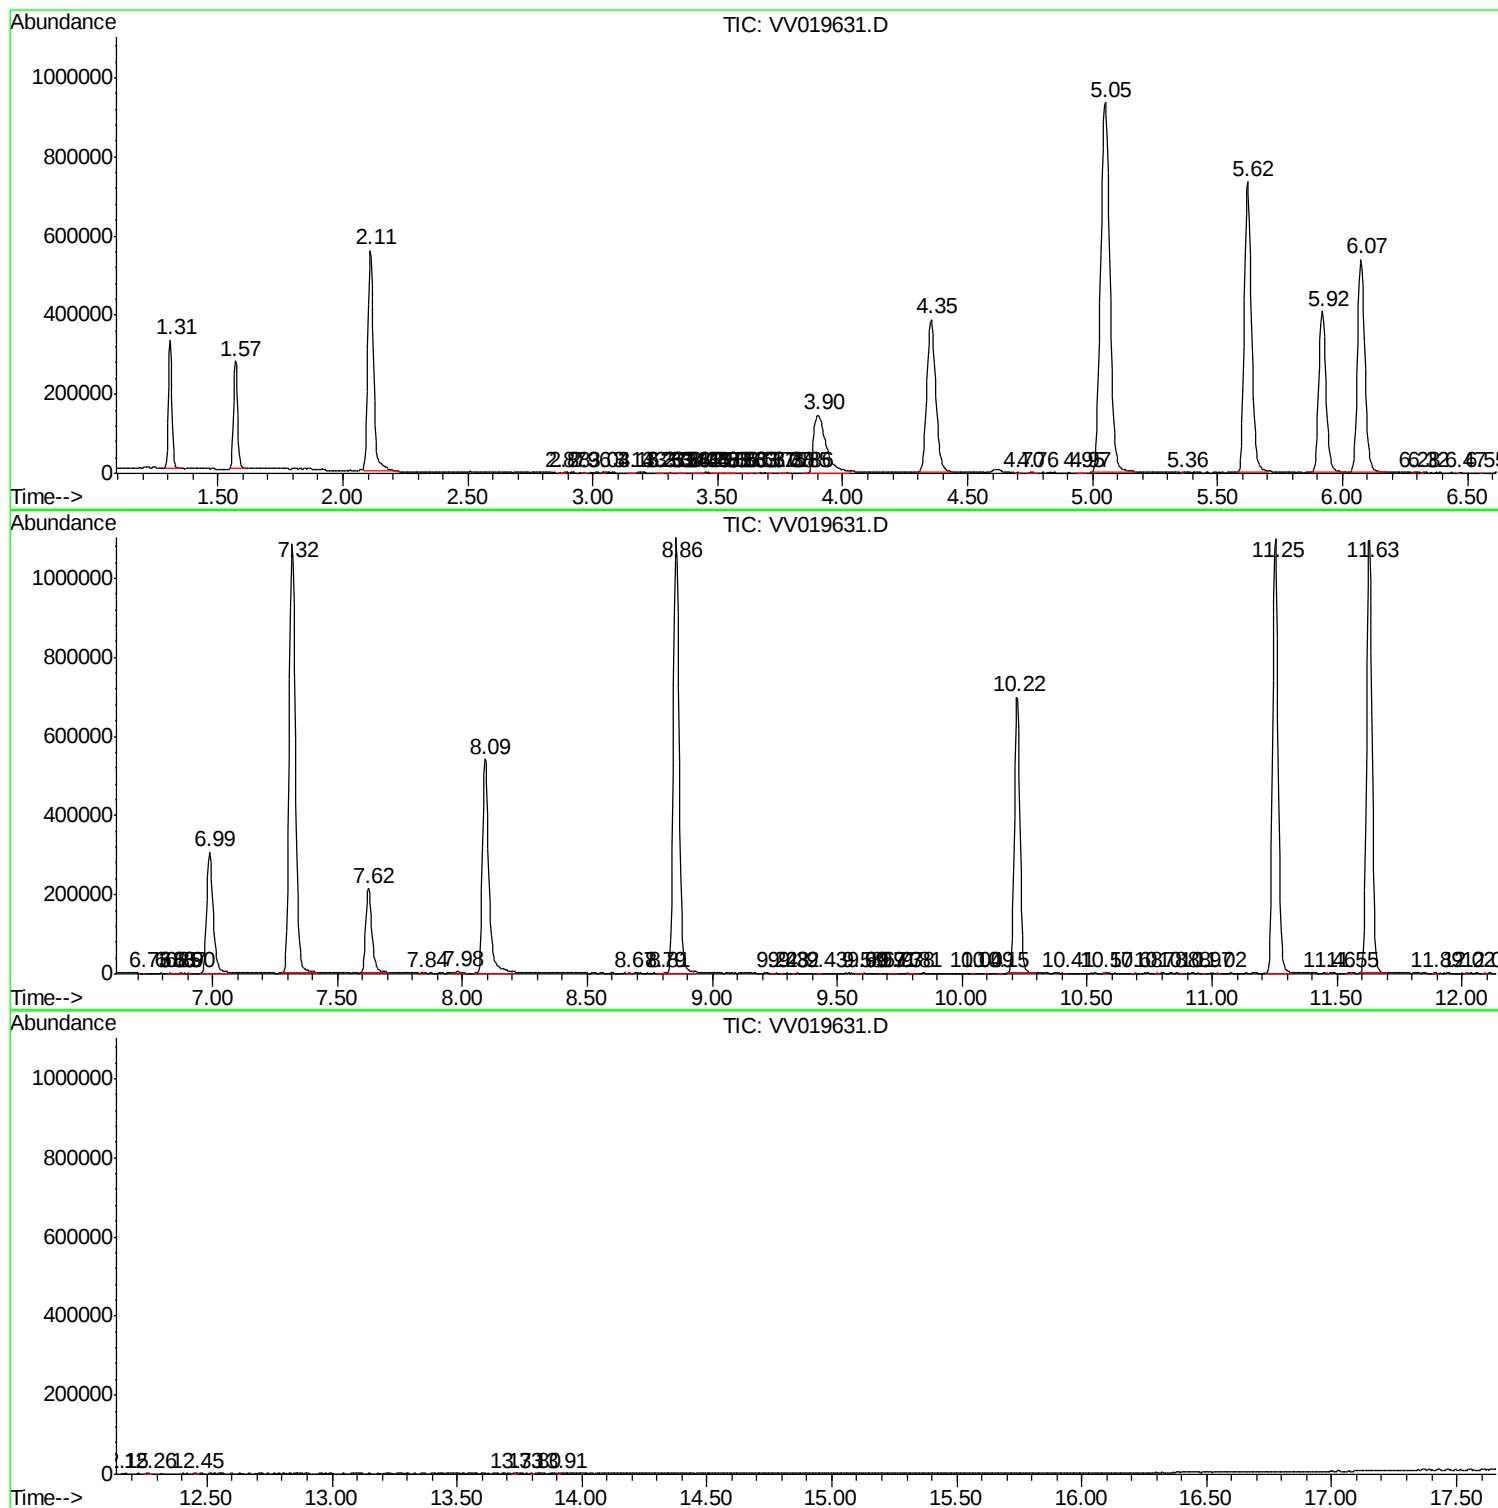

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121420\
Data File : VV019631.D
Acq On : 15 Dec 2020 02:41
Operator : SY/MD
Sample : L5024-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121420\
Data File : VV019631.D
Acq On : 15 Dec 2020 02:41
Operator : SY/MD
Sample : L5024-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AX1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc