

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019636.D
 Acq On : 15 Dec 2020 04:40
 Operator : SY/MD
 Sample : L5024-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	84	rVB	315396	310253	13.24%	1.748%
2	1.569	142	149	161	rBV	267713	307681	13.13%	1.734%
3	2.110	308	317	352	rVB	523746	820716	35.02%	4.625%
4	3.010	595	597	600	rBB2	481	179	0.01%	0.001%
5	3.093	622	623	624	rBV	437	138	0.01%	0.001%
6	3.200	654	656	658	rVB2	648	194	0.01%	0.001%
7	3.241	665	669	671	rBV3	354	284	0.01%	0.002%
8	3.296	681	686	692	rBV4	663	914	0.04%	0.005%
9	3.338	696	699	700	rBV2	291	171	0.01%	0.001%
10	3.418	722	724	725	rBV2	248	83	0.00%	0.000%
11	3.495	746	748	749	rBV	349	147	0.01%	0.001%
12	3.511	749	753	756	rVV2	508	324	0.01%	0.002%
13	3.582	773	775	777	rBV	225	110	0.00%	0.001%
14	3.598	777	780	783	rBV2	402	361	0.02%	0.002%
15	3.647	793	795	799	rVB2	495	225	0.01%	0.001%
16	3.663	799	800	802	rBV2	275	97	0.00%	0.001%
17	3.717	815	817	821	rBV2	523	210	0.01%	0.001%
18	3.772	829	834	838	rBV3	624	699	0.03%	0.004%
19	3.807	842	845	846	rBV2	484	278	0.01%	0.002%
20	3.836	851	854	858	rBV4	490	420	0.02%	0.002%
21	3.897	861	873	916	rBV2	152091	518309	22.12%	2.921%
22	4.354	999	1015	1040	rBV	376093	932020	39.77%	5.252%
23	4.791	1149	1151	1153	rVB	449	215	0.01%	0.001%
24	4.807	1153	1156	1158	rBV2	539	366	0.02%	0.002%
25	4.843	1164	1167	1169	rBV2	718	358	0.02%	0.002%
26	4.897	1180	1184	1187	rBV4	839	705	0.03%	0.004%
27	4.939	1195	1197	1201	rVB2	512	266	0.01%	0.001%
28	4.968	1201	1206	1208	rBV3	681	496	0.02%	0.003%
29	5.052	1214	1232	1264	rBV2	914230	2343261	100.00%	13.204%
30	5.482	1364	1366	1370	rBV3	634	492	0.02%	0.003%
31	5.621	1396	1409	1450	rBV	737775	1469126	62.70%	8.279%
32	5.917	1488	1501	1517	rBV8	16510	41545	1.77%	0.234%
33	6.074	1536	1550	1574	rBV	527016	1067445	45.55%	6.015%
34	6.370	1639	1642	1643	rBV	476	208	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019636.D
 Acq On : 15 Dec 2020 04:40
 Operator : SY/MD
 Sample : L5024-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.524	1688	1690	1694	rBV2	299	207	0.01%	0.001%
36	6.543	1694	1696	1697	rVV	355	118	0.01%	0.001%
37	6.595	1709	1712	1714	rBV	321	217	0.01%	0.001%
38	6.611	1714	1717	1718	rBV	692	321	0.01%	0.002%
39	6.830	1783	1785	1786	rBV	291	108	0.00%	0.001%
40	6.839	1786	1788	1789	rVV	159	74	0.00%	0.000%
41	6.907	1806	1809	1810	rBV	722	376	0.02%	0.002%
42	6.987	1823	1834	1860	rBV	292889	540620	23.07%	3.046%
43	7.318	1925	1937	1961	rBV	1076063	1837624	78.42%	10.355%
44	7.624	2022	2032	2056	rBV	208145	355517	15.17%	2.003%
45	8.090	2166	2177	2212	rBV	540717	964798	41.17%	5.437%
46	8.421	2276	2280	2281	rBV2	1142	846	0.04%	0.005%
47	8.566	2323	2325	2328	rBV2	567	388	0.02%	0.002%
48	8.617	2338	2341	2343	rBV3	688	477	0.02%	0.003%
49	8.743	2377	2380	2381	rBV3	700	317	0.01%	0.002%
50	8.759	2382	2385	2387	rBV2	611	366	0.02%	0.002%
51	8.855	2403	2415	2441	rBV	1105578	1783436	76.11%	10.050%
52	9.199	2520	2522	2524	rBV	393	241	0.01%	0.001%
53	9.241	2533	2535	2537	rBV2	264	107	0.00%	0.001%
54	9.264	2540	2542	2545	rBV	415	333	0.01%	0.002%
55	9.360	2569	2572	2576	rVB3	659	380	0.02%	0.002%
56	9.386	2576	2580	2581	rBV2	345	239	0.01%	0.001%
57	9.527	2620	2624	2626	rBV3	456	371	0.02%	0.002%
58	9.595	2643	2645	2649	rVB	473	292	0.01%	0.002%
59	9.617	2649	2652	2655	rBV2	483	379	0.02%	0.002%
60	9.672	2666	2669	2670	rBV	518	307	0.01%	0.002%
61	9.740	2687	2690	2692	rBV2	459	292	0.01%	0.002%
62	9.752	2692	2694	2696	rVV	646	240	0.01%	0.001%
63	9.788	2699	2705	2707	rBV4	978	944	0.04%	0.005%
64	9.855	2723	2726	2727	rBV	416	193	0.01%	0.001%
65	9.894	2736	2738	2740	rBV	430	257	0.01%	0.001%
66	9.942	2748	2753	2755	rBV3	474	487	0.02%	0.003%
67	10.013	2771	2775	2778	rBV2	244	227	0.01%	0.001%
68	10.035	2778	2782	2783	rBV2	353	288	0.01%	0.002%
69	10.064	2789	2791	2792	rBV	343	120	0.01%	0.001%
70	10.135	2811	2813	2818	rVB2	508	298	0.01%	0.002%
71	10.158	2818	2820	2822	rBV	306	131	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019636.D
 Acq On : 15 Dec 2020 04:40
 Operator : SY/MD
 Sample : L5024-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.177	2822	2826	2827	rBV2	783	470	0.02%	0.003%
73	10.219	2827	2839	2860	rVV	690204	1083147	46.22%	6.104%
74	10.367	2881	2885	2887	rBV2	634	574	0.02%	0.003%
75	10.511	2928	2930	2932	rBV	506	262	0.01%	0.001%
76	10.569	2944	2948	2949	rBV3	631	346	0.01%	0.002%
77	10.752	3004	3005	3007	rBV2	359	105	0.00%	0.001%
78	10.839	3030	3032	3034	rBV4	567	236	0.01%	0.001%
79	10.948	3064	3066	3071	rVB3	590	262	0.01%	0.001%
80	10.977	3071	3075	3076	rBV2	442	283	0.01%	0.002%
81	11.067	3100	3103	3106	rBV4	634	473	0.02%	0.003%
82	11.103	3110	3114	3116	rBV2	646	385	0.02%	0.002%
83	11.122	3116	3120	3123	rBV2	417	298	0.01%	0.002%
84	11.254	3149	3161	3185	rBV	1087041	1683112	71.83%	9.484%
85	11.514	3238	3242	3243	rBV	449	242	0.01%	0.001%
86	11.540	3247	3250	3251	rBV	846	395	0.02%	0.002%
87	11.627	3265	3277	3303	rBV	1046930	1656224	70.68%	9.333%
88	12.180	3446	3449	3452	rBV2	646	460	0.02%	0.003%
89	12.357	3497	3504	3512	rBV4	3393	5166	0.22%	0.029%
90	12.704	3610	3612	3616	rBV2	481	248	0.01%	0.001%
91	12.936	3681	3684	3685	rBV	479	281	0.01%	0.002%
92	13.006	3704	3706	3707	rBV	500	178	0.01%	0.001%
93	13.045	3715	3718	3719	rBV	431	291	0.01%	0.002%
94	13.141	3746	3748	3751	rBV2	692	381	0.02%	0.002%
95	13.270	3784	3788	3794	rBV5	959	1144	0.05%	0.006%
96	13.656	3904	3908	3910	rBV2	721	573	0.02%	0.003%
97	13.784	3946	3948	3954	rBV5	708	513	0.02%	0.003%


Sum of corrected areas: 17746281

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121420\
Data File : VV019636.D
Acq On : 15 Dec 2020 04:40
Operator : SY/MD
Sample : L5024-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0AX6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

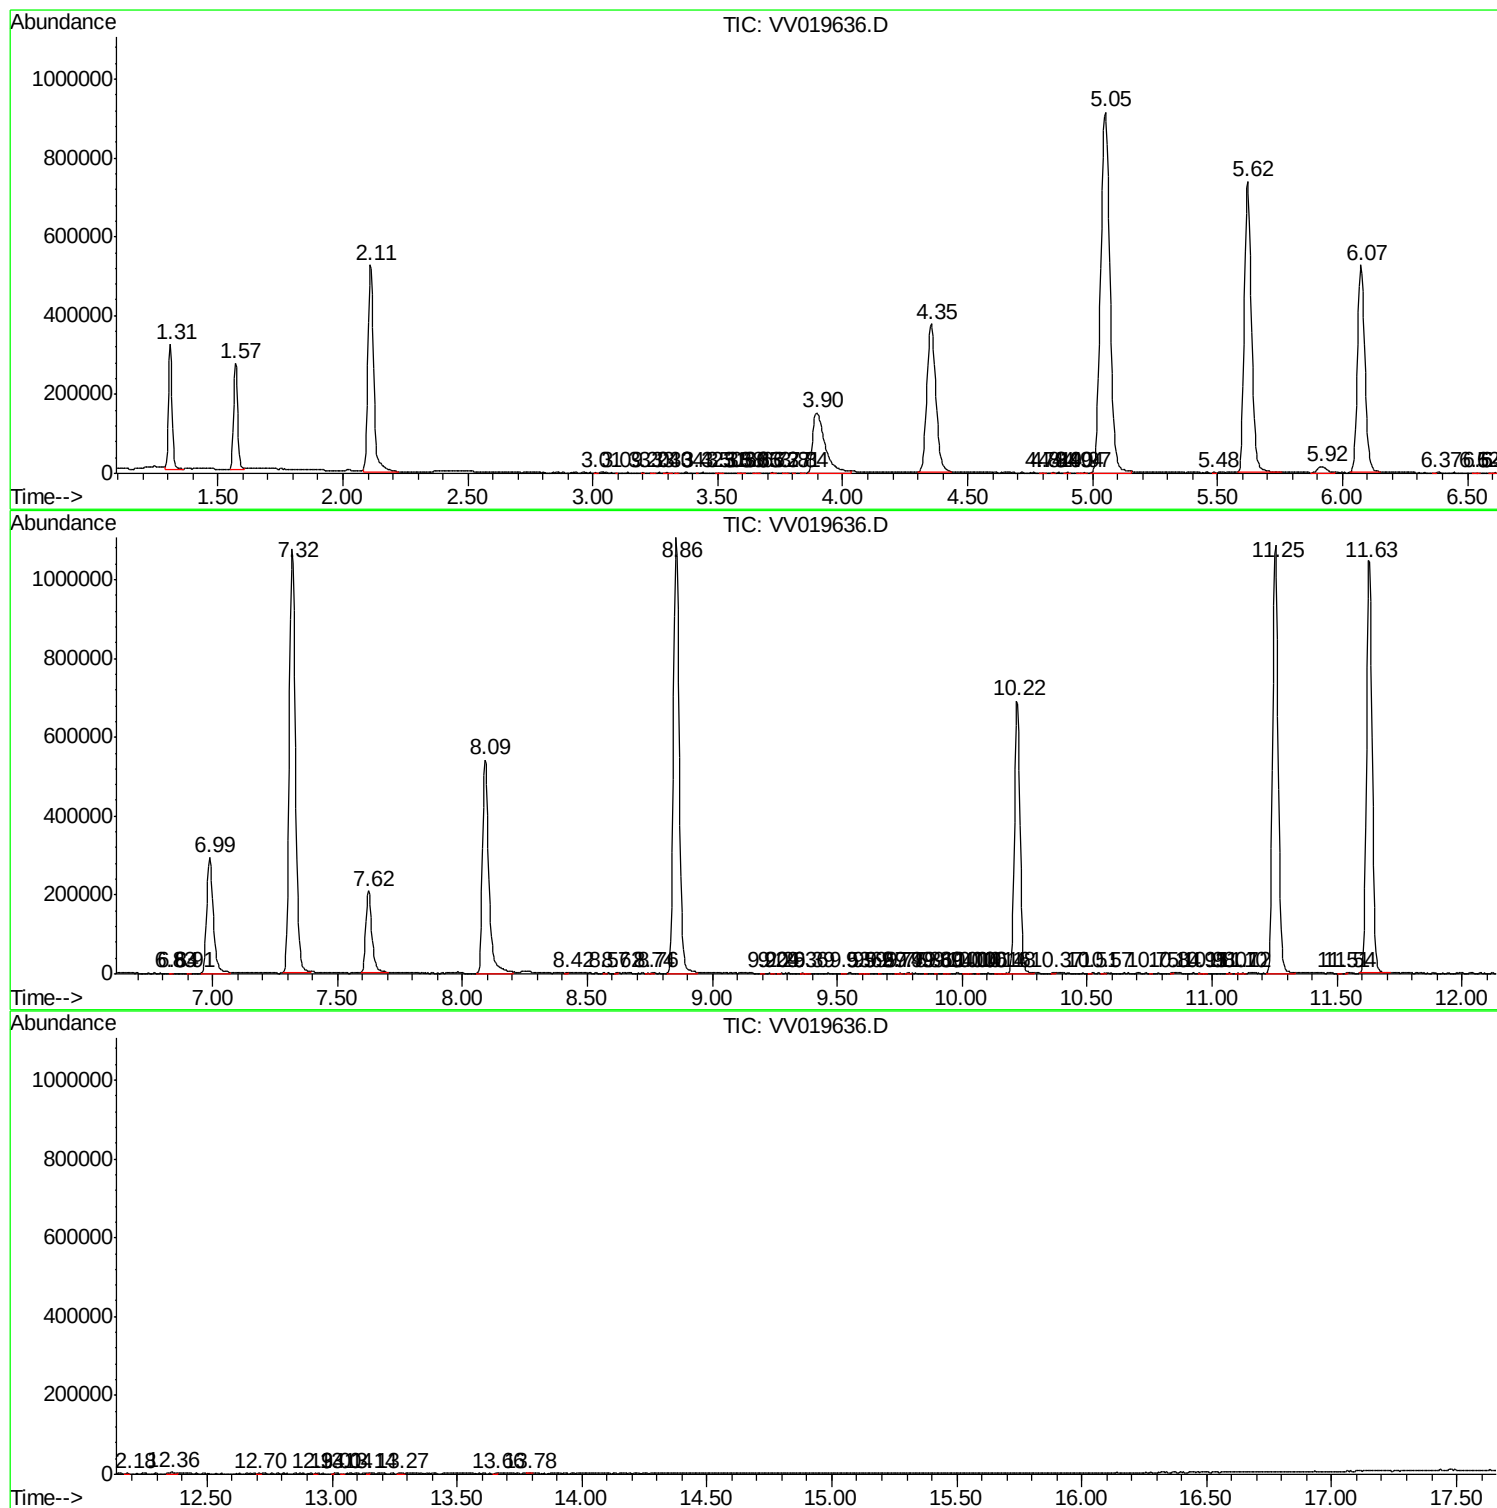

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121420\
Data File : VV019636.D
Acq On : 15 Dec 2020 04:40
Operator : SY/MD
Sample : L5024-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AX6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121420\
Data File : VV019636.D
Acq On : 15 Dec 2020 04:40
Operator : SY/MD
Sample : L5024-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AX6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
