

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019637.D
 Acq On : 15 Dec 2020 05:04
 Operator : SY/MD
 Sample : L5024-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	82	rVB	312597	304911	12.96%	1.716%
2	1.569	142	149	161	rVB	262978	296353	12.60%	1.668%
3	2.110	308	317	360	rVB	525050	824744	35.06%	4.641%
4	2.897	559	562	566	rBV2	701	417	0.02%	0.002%
5	2.965	580	583	586	rVB4	553	335	0.01%	0.002%
6	3.026	599	602	604	rBV3	739	460	0.02%	0.003%
7	3.116	627	630	632	rBV2	578	405	0.02%	0.002%
8	3.225	661	664	669	rBV4	396	374	0.02%	0.002%
9	3.245	669	670	674	rVB2	265	148	0.01%	0.001%
10	3.267	674	677	679	rBV3	433	208	0.01%	0.001%
11	3.319	691	693	696	rBV3	388	240	0.01%	0.001%
12	3.428	725	727	730	rBV	322	179	0.01%	0.001%
13	3.441	730	731	736	rVB4	546	319	0.01%	0.002%
14	3.467	736	739	742	rBV2	355	217	0.01%	0.001%
15	3.486	744	745	746	rBV	240	67	0.00%	0.000%
16	3.534	756	760	765	rBV3	571	533	0.02%	0.003%
17	3.553	765	766	770	rVB2	411	211	0.01%	0.001%
18	3.586	770	776	778	rBV2	459	386	0.02%	0.002%
19	3.605	778	782	785	rBV	665	542	0.02%	0.003%
20	3.627	788	789	790	rBV	377	99	0.00%	0.001%
21	3.663	798	800	803	rVB	787	388	0.02%	0.002%
22	3.682	803	806	807	rBV	361	233	0.01%	0.001%
23	3.711	812	815	818	rBV2	349	245	0.01%	0.001%
24	3.753	826	828	831	rBV2	571	255	0.01%	0.001%
25	3.804	843	844	846	rBV2	255	113	0.00%	0.001%
26	3.840	853	855	857	rBV2	232	110	0.00%	0.001%
27	3.856	857	860	861	rBV	415	212	0.01%	0.001%
28	3.901	862	874	922	rBV2	145591	531372	22.59%	2.990%
29	4.354	1000	1015	1042	rVB	378941	927794	39.44%	5.221%
30	4.666	1110	1112	1113	rBV	689	322	0.01%	0.002%
31	4.740	1131	1135	1136	rBV2	919	654	0.03%	0.004%
32	4.827	1159	1162	1164	rBV	451	293	0.01%	0.002%
33	4.881	1177	1179	1183	rBV3	527	466	0.02%	0.003%
34	4.913	1186	1189	1192	rBV2	559	364	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019637.D
 Acq On : 15 Dec 2020 05:04
 Operator : SY/MD
 Sample : L5024-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	4.933	1192	1195	1196	rBV2	531	259	0.01%	0.001%
36	4.984	1209	1211	1213	rBV2	721	466	0.02%	0.003%
37	5.052	1213	1232	1269	rVV2	915272	2352673	100.00%	13.239%
38	5.463	1356	1360	1361	rBV3	847	646	0.03%	0.004%
39	5.621	1396	1409	1435	rBV	714803	1436538	61.06%	8.084%
40	5.862	1482	1484	1487	rVB2	407	200	0.01%	0.001%
41	5.917	1488	1501	1521	rVV7	20912	50113	2.13%	0.282%
42	6.074	1536	1550	1575	rBV	523618	1069000	45.44%	6.015%
43	6.299	1618	1620	1624	rVB	696	224	0.01%	0.001%
44	6.360	1634	1639	1641	rBV2	774	616	0.03%	0.003%
45	6.405	1651	1653	1655	rBV2	527	279	0.01%	0.002%
46	6.521	1687	1689	1691	rVB	247	113	0.00%	0.001%
47	6.547	1693	1697	1700	rBV3	494	401	0.02%	0.002%
48	6.576	1703	1706	1707	rBV2	710	368	0.02%	0.002%
49	6.598	1712	1713	1714	rBV	346	95	0.00%	0.001%
50	6.765	1761	1765	1768	rBV4	1034	821	0.03%	0.005%
51	6.823	1779	1783	1787	rBV4	694	548	0.02%	0.003%
52	6.843	1787	1789	1793	rVV2	371	266	0.01%	0.001%
53	6.920	1811	1813	1818	rVB2	385	196	0.01%	0.001%
54	6.946	1818	1821	1823	rBV3	486	374	0.02%	0.002%
55	6.987	1823	1834	1862	rBV	295001	537846	22.86%	3.027%
56	7.318	1925	1937	1964	rBV	1069649	1836655	78.07%	10.335%
57	7.624	2021	2032	2057	rBV	207799	364354	15.49%	2.050%
58	7.942	2128	2131	2137	rBV4	1059	931	0.04%	0.005%
59	7.981	2138	2143	2156	rVB7	3977	5576	0.24%	0.031%
60	8.045	2159	2163	2165	rBV3	566	435	0.02%	0.002%
61	8.090	2167	2177	2211	rBV	567829	1016178	43.19%	5.718%
62	8.653	2350	2352	2355	rVB4	592	275	0.01%	0.002%
63	8.720	2371	2373	2375	rBV	279	69	0.00%	0.000%
64	8.855	2403	2415	2448	rBV	1077915	1750920	74.42%	9.853%
65	9.309	2554	2556	2558	rBV3	354	144	0.01%	0.001%
66	9.341	2564	2566	2568	rVB2	414	152	0.01%	0.001%
67	9.450	2597	2600	2602	rBV2	421	243	0.01%	0.001%
68	9.560	2630	2634	2635	rBV3	422	231	0.01%	0.001%
69	9.595	2642	2645	2647	rBV3	528	399	0.02%	0.002%
70	9.646	2659	2661	2664	rVB	423	218	0.01%	0.001%
71	9.717	2678	2683	2684	rBV3	659	508	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121420\
 Data File : VV019637.D
 Acq On : 15 Dec 2020 05:04
 Operator : SY/MD
 Sample : L5024-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	9.942	2749	2753	2755	rBV	555	410	0.02%	0.002%
73	10.003	2769	2772	2775	rBV2	482	257	0.01%	0.001%
74	10.016	2775	2776	2778	rVV2	356	117	0.00%	0.001%
75	10.051	2784	2787	2788	rBV2	253	137	0.01%	0.001%
76	10.100	2798	2802	2805	rBV3	640	438	0.02%	0.002%
77	10.119	2806	2808	2813	rVB2	381	219	0.01%	0.001%
78	10.145	2814	2816	2817	rBV	454	137	0.01%	0.001%
79	10.219	2827	2839	2861	rBV	709922	1110284	47.19%	6.248%
80	10.418	2898	2901	2902	rBV2	341	206	0.01%	0.001%
81	10.441	2906	2908	2910	rBV	403	203	0.01%	0.001%
82	10.534	2934	2937	2938	rBV	391	208	0.01%	0.001%
83	10.553	2942	2943	2944	rBV	298	92	0.00%	0.001%
84	10.685	2980	2984	2988	rBV3	869	968	0.04%	0.005%
85	10.932	3059	3061	3063	rBV	367	164	0.01%	0.001%
86	11.055	3098	3099	3103	rBV2	291	206	0.01%	0.001%
87	11.093	3108	3111	3114	rVB	529	375	0.02%	0.002%
88	11.180	3135	3138	3141	rVB3	998	605	0.03%	0.003%
89	11.254	3149	3161	3186	rBV	1080831	1664459	70.75%	9.366%
90	11.630	3265	3278	3300	rBV	1069857	1666233	70.82%	9.376%
91	12.116	3425	3429	3431	rBV	611	398	0.02%	0.002%
92	12.196	3450	3454	3455	rBV2	634	447	0.02%	0.003%
93	12.791	3636	3639	3641	rBV3	708	436	0.02%	0.002%
94	13.215	3769	3771	3774	rBV3	557	325	0.01%	0.002%
95	13.273	3786	3789	3792	rBV2	777	431	0.02%	0.002%


Sum of corrected areas: 17771054

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121420\
Data File : VV019637.D
Acq On : 15 Dec 2020 05:04
Operator : SY/MD
Sample : L5024-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

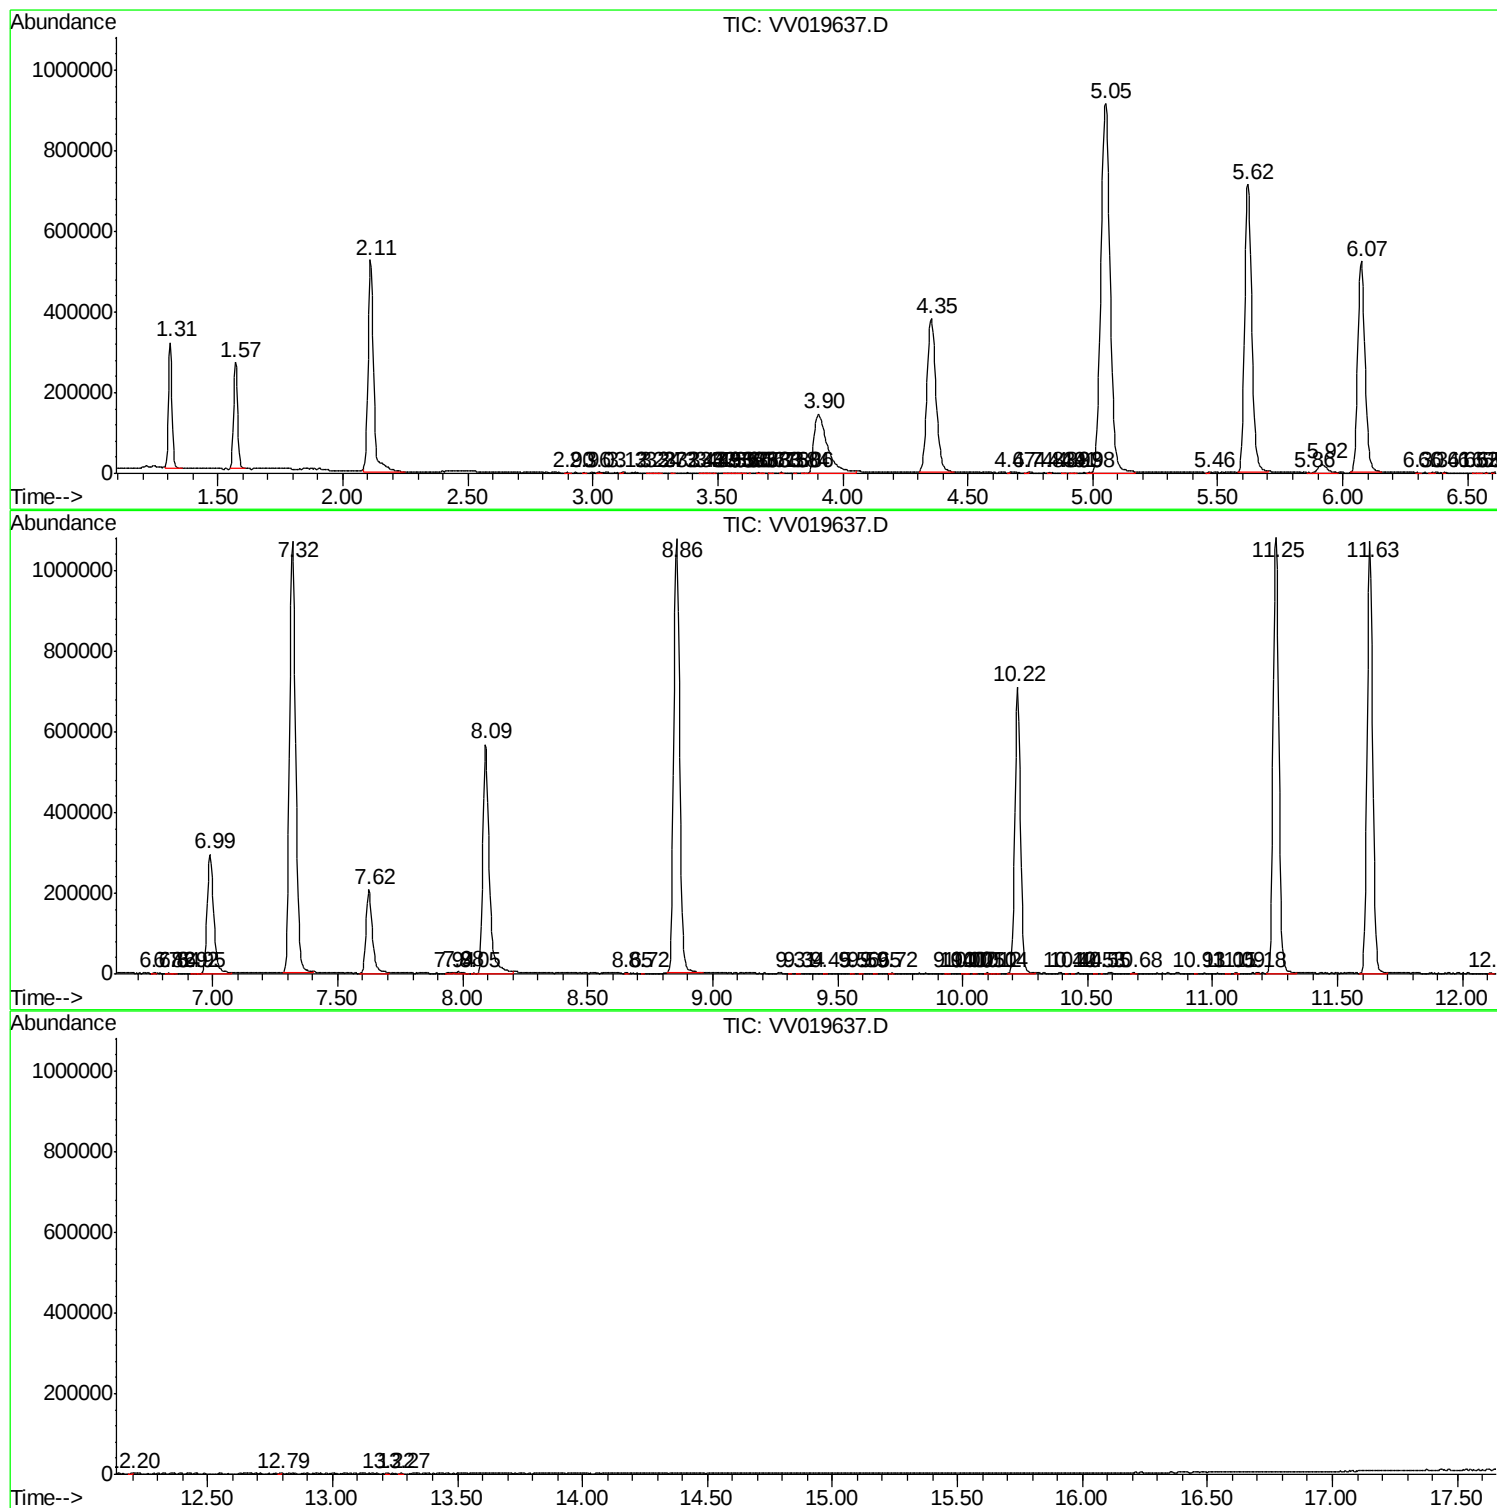

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121420\
Data File : VV019637.D
Acq On : 15 Dec 2020 05:04
Operator : SY/MD
Sample : L5024-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121420\
Data File : VV019637.D
Acq On : 15 Dec 2020 05:04
Operator : SY/MD
Sample : L5024-07
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AX7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc