


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121420\
 Data File : VV019594.D
 Acq On : 14 Dec 2020 09:19
 Operator : SY/MD
 Sample : BFB65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB65

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis
 Last Update : Tue Dec 15 10:26:59 2020

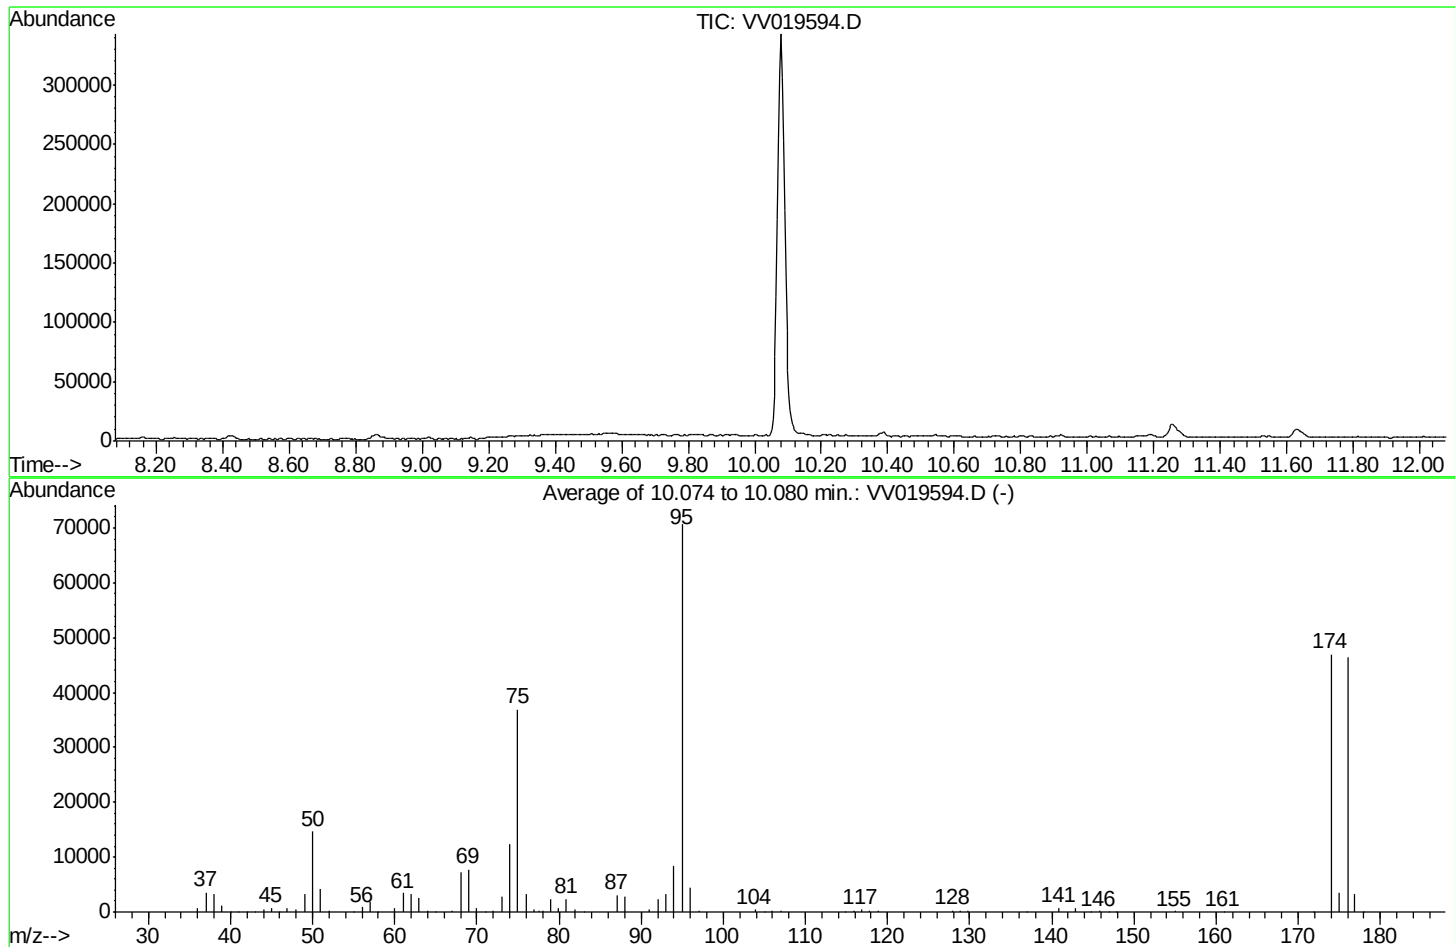

AutoFind: Scans 2794, 2795, 2796; Background Corrected with Scan 2783

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	14608	PASS
75	95	30	80	52.2	36893	PASS
95	95	100	100	100.0	70677	PASS
96	95	5	9	6.4	4553	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	66.4	46909	PASS
175	174	5	9	7.5	3496	PASS
176	174	95	101	98.9	46397	PASS
177	176	5	9	6.9	3191	PASS

m/z	Abundance
36.00	2439.0
37.00	3544.0
38.00	4115.0
39.00	1368.0
40.00	258.0
41.00	117.0
43.00	192.0
44.00	1352.0
45.00	707.0
46.00	134.0
47.00	882.0
47.90	476.0
49.00	3036.0
50.00	14258.0
51.00	4147.0
51.90	218.0
55.00	217.0
56.00	1091.0
57.00	1809.0
60.00	751.0
61.00	3173.0
62.00	3192.0
63.00	2520.0
64.00	227.0
66.90	230.0
68.00	7290.0
69.00	7304.0
70.00	708.0
71.10	110.0
71.90	328.0
73.00	2640.0
74.00	11760.0
75.00	34752.0
76.00	3221.0
76.90	427.0
77.50	222.0
78.10	325.0
78.90	2086.0
79.90	728.0
80.90	2221.0
81.90	448.0
83.00	132.0
87.00	2840.0
88.00	2566.0
91.00	355.0
92.00	2275.0
93.00	3031.0
94.00	7930.0
95.00	66608.0
96.00	4242.0
97.00	179.0
103.90	313.0
106.00	373.0
106.90	139.0
114.90	130.0
115.90	283.0
116.80	418.0
117.80	235.0
118.90	333.0
127.90	241.0
128.90	133.0
129.70	180.0
137.00	104.0
140.90	659.0
142.90	734.0
145.80	151.0
146.80	105.0
154.90	154.0
160.90	110.0
171.70	104.0
174.00	43304.0
175.00	3181.0
176.00	42784.0
176.90	2990.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	2565.0
37.00	3813.0
38.00	4156.0
39.00	1386.0
40.00	308.0
41.00	132.0
42.10	126.0
42.90	209.0
44.00	1326.0
45.00	769.0
46.00	112.0
46.90	776.0
47.90	502.0
49.00	3367.0
50.00	15133.0
51.00	4372.0
51.90	227.0
55.00	249.0
56.00	1038.0
57.00	1874.0
58.00	114.0
60.00	826.0
61.00	3521.0
62.00	3528.0
63.00	2714.0
64.00	261.0
66.90	259.0
68.00	7453.0
69.00	8157.0
70.00	682.0
71.10	136.0
71.90	365.0
73.00	2885.0
74.00	12818.0
75.00	38184.0
76.00	3420.0
76.90	504.0
77.60	210.0
78.10	359.0
78.90	2402.0
79.90	785.0
80.90	2402.0
81.90	471.0
83.00	122.0
87.00	3259.0
88.00	2936.0
90.90	383.0
92.00	2418.0
93.00	3264.0
94.00	8885.0
95.00	72888.0
96.00	4630.0
97.10	158.0
103.80	382.0
105.00	113.0
106.00	313.0
106.90	172.0
114.80	125.0
115.90	365.0
116.80	442.0
117.90	274.0
118.90	350.0
128.00	280.0
128.90	169.0
129.80	202.0
136.90	109.0
140.90	777.0
142.90	792.0
145.80	133.0
146.90	105.0
155.00	208.0
171.80	113.0
174.00	48592.0
175.00	3674.0
176.00	48096.0
176.90	3330.0
177.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	2571.0
37.00	3903.0
38.00	3839.0
39.00	1288.0
40.00	347.0
41.00	138.0
42.10	132.0
42.90	205.0
44.00	1233.0
45.00	723.0
47.00	681.0
47.90	474.0
49.00	3261.0
50.00	14433.0
51.00	4372.0
52.00	222.0
55.00	254.0
56.10	931.0
57.00	1776.0
58.00	120.0
59.90	769.0
61.00	3497.0
62.00	3420.0
63.00	2704.0
64.00	276.0
64.90	134.0
66.90	273.0
68.00	7186.0
69.00	7990.0
70.00	575.0
71.90	367.0
73.00	3001.0
74.00	12590.0
75.00	37744.0
76.00	3322.0
77.00	491.0
78.10	361.0
78.90	2490.0
79.90	754.0
80.90	2420.0
81.90	462.0
82.90	113.0
87.00	3121.0
88.00	2980.0
90.90	378.0
92.00	2216.0
93.00	3218.0
94.00	8700.0
95.00	72536.0
96.00	4787.0
97.10	118.0
103.80	416.0
105.00	108.0
106.00	290.0
107.00	157.0
115.90	423.0
116.80	433.0
117.90	279.0
118.90	321.0
128.00	312.0
128.80	171.0
129.90	229.0
136.90	109.0
140.90	845.0
142.90	737.0
144.80	118.0
145.80	105.0
147.80	102.0
155.00	221.0
171.90	128.0
174.00	48832.0
175.00	3635.0
176.00	48312.0
176.90	3254.0
177.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

Scan 2783 (10.038 min): VV019594.D
BFB65

m/z	Abundance
36.00	1885.0
37.00	158.0
37.90	769.0
39.00	132.0
40.00	208.0
41.00	127.0
43.10	135.0
44.00	784.0
55.00	181.0
56.00	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65