

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121421\
 Data File : VW023961.D
 Acq On : 14 Dec 2021 12:09
 Operator : SY/MD
 Sample : M5005-11 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW215

Quant Time: Dec 15 01:38:35 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 11 04:33:17 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	95941	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	103421	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	50154	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	21859	4.238	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	84.800%	
7) Chloroethane-d5	1.568	69	21943	5.099	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	102.000%	
11) 1,1-Dichloroethene-d2	2.108	63	31260	3.105	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	62.000%	
20) 2-Butanone-d5	3.909	46	47396	47.036	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	94.080%	
24) Chloroform-d	4.349	84	60820	5.206	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.200%	
26) 1,2-Dichloroethane-d4	5.034	65	31080	5.714	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	114.200%	
32) Benzene-d6	5.050	84	94371	4.607	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.200%	
36) 1,2-Dichloropropane-d6	6.069	67	32197	5.210	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.200%	
41) Toluene-d8	7.317	98	71608	3.883	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	77.600%	
43) trans-1,3-Dichloroprop...	7.625	79	11466	4.472	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.400%	
46) 2-Hexanone-d5	8.092	63	54635	47.603	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.200%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	25904	5.053	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	36002	5.374	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.400%	
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	3577	0.425	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
Data File : VV023961.D
Acq On : 14 Dec 2021 12:09
Operator : SY/MD
Sample : M5005-11 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW215

Quant Time: Dec 15 01:38:35 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 11 04:33:17 2021
Response via : Initial Calibration

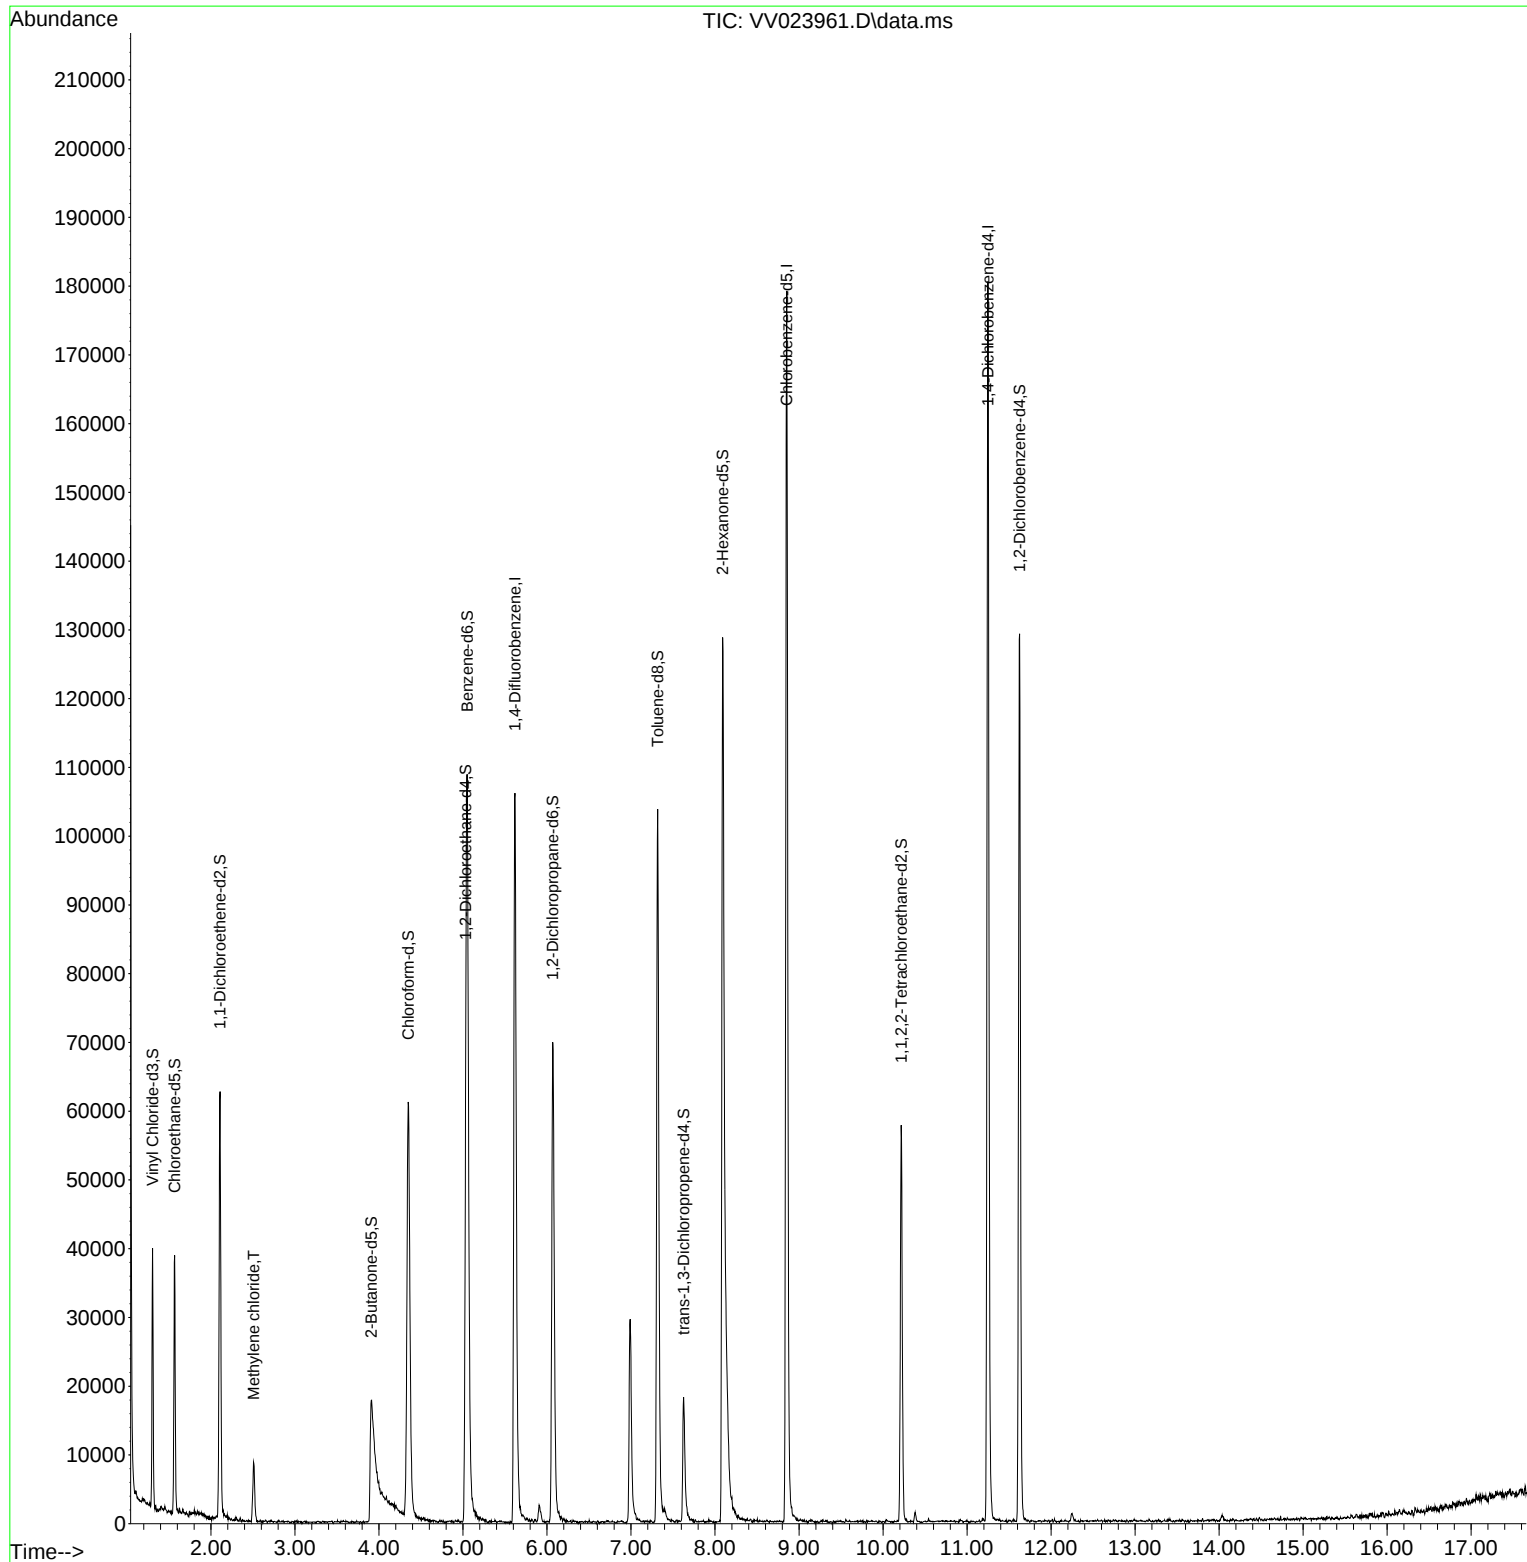

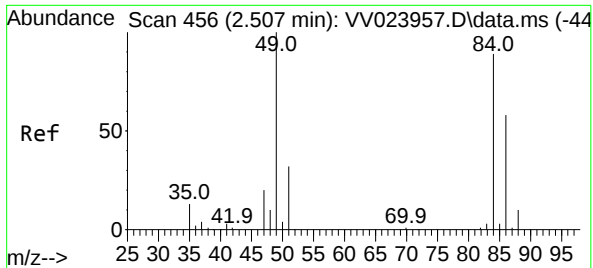

#16
Methylene chloride
Concen: 0.425 ug/L
RT: 2.507 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV023961.D
Acq: 14 Dec 2021 12:09

Instrument :
MSVOA_V
ClientSampleId :
EW215

Tgt Ion: 84	Resp:	3577	
Ion	Ratio	Lower	Upper
84	100		
86	61.7	42.6	79.0
49	101.0	79.7	147.9

