

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV121421\  
 Data File : VV023958.D  
 Acq On : 14 Dec 2021 10:44  
 Operator : SY/MD  
 Sample : VV1214WBL01  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 VBLK277

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023957.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.304       | 76            | 82          | 90           | rBV      | 47927          | 45731         | 15.20%          | 1.870%        |
| 2         | 1.565       | 156           | 163         | 173          | rBV      | 37571          | 42880         | 14.25%          | 1.754%        |
| 3         | 2.105       | 322           | 331         | 347          | rBV      | 80622          | 117894        | 39.19%          | 4.821%        |
| 4         | 2.507       | 446           | 456         | 469          | rVB4     | 6113           | 11406         | 3.79%           | 0.466%        |
| 5         | 3.915       | 884           | 894         | 903          | rBV2     | 10882          | 28727         | 9.55%           | 1.175%        |
| 6         | 4.346       | 1012          | 1028        | 1050         | rBV2     | 53708          | 129272        | 42.97%          | 5.287%        |
| 7         | 5.044       | 1229          | 1245        | 1269         | rBV3     | 111031         | 281038        | 93.42%          | 11.494%       |
| 8         | 5.613       | 1406          | 1422        | 1444         | rBV      | 108133         | 224391        | 74.59%          | 9.177%        |
| 9         | 5.912       | 1506          | 1515        | 1522         | rBV6     | 2679           | 5248          | 1.74%           | 0.215%        |
| 10        | 6.066       | 1549          | 1563        | 1580         | rBV      | 63888          | 132870        | 44.17%          | 5.434%        |
| 11        | 6.989       | 1837          | 1850        | 1862         | rBV2     | 29405          | 56244         | 18.70%          | 2.300%        |
| 12        | 7.314       | 1937          | 1951        | 1971         | rBV      | 134343         | 236089        | 78.48%          | 9.655%        |
| 13        | 7.622       | 2038          | 2047        | 2061         | rBV3     | 17336          | 32492         | 10.80%          | 1.329%        |
| 14        | 8.092       | 2183          | 2193        | 2228         | rBV      | 82619          | 202003        | 67.15%          | 8.261%        |
| 15        | 8.850       | 2418          | 2429        | 2448         | rBV      | 183622         | 300825        | 100.00%         | 12.303%       |
| 16        | 10.214      | 2843          | 2853        | 2876         | rVB      | 43312          | 70038         | 23.28%          | 2.864%        |
| 17        | 11.249      | 3164          | 3175        | 3195         | rVV      | 186125         | 296384        | 98.52%          | 12.121%       |
| 18        | 11.622      | 3281          | 3291        | 3306         | rBV      | 130913         | 210045        | 69.82%          | 8.590%        |
| 19        | 15.609      | 4512          | 4531        | 4535         | rBV      | 7246           | 21605         | 7.18%           | 0.884%        |




Sum of corrected areas: 2445182

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV121421\  
Data File : VV023958.D  
Acq On : 14 Dec 2021 10:44  
Operator : SY/MD  
Sample : VV1214WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR121021WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

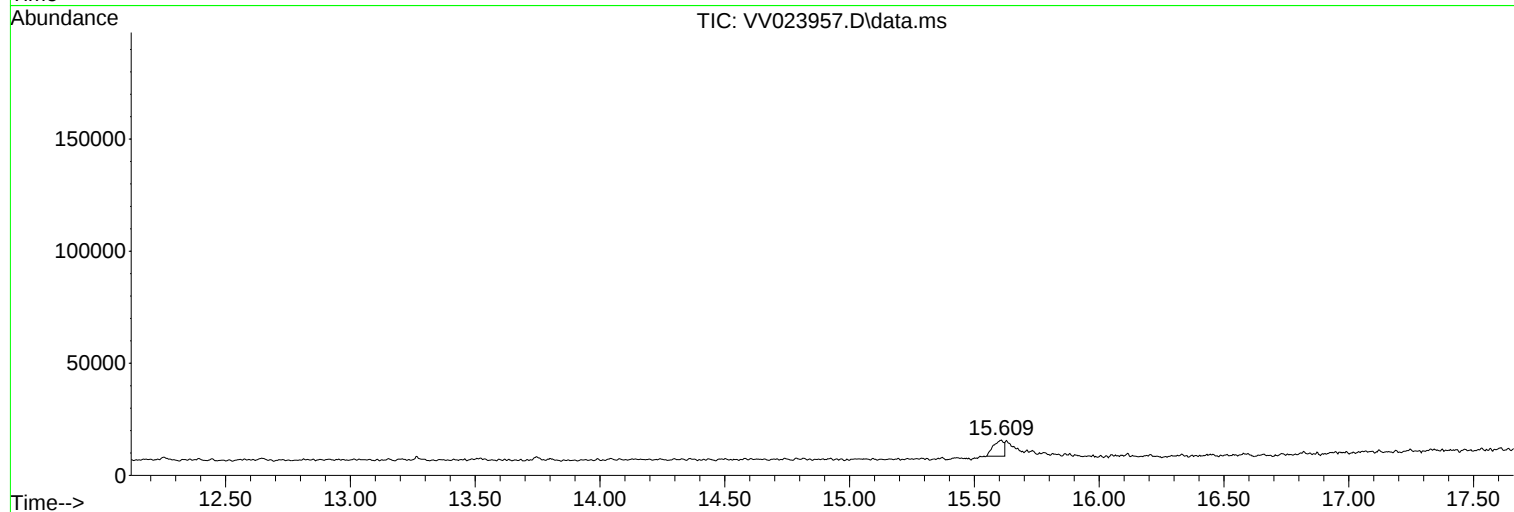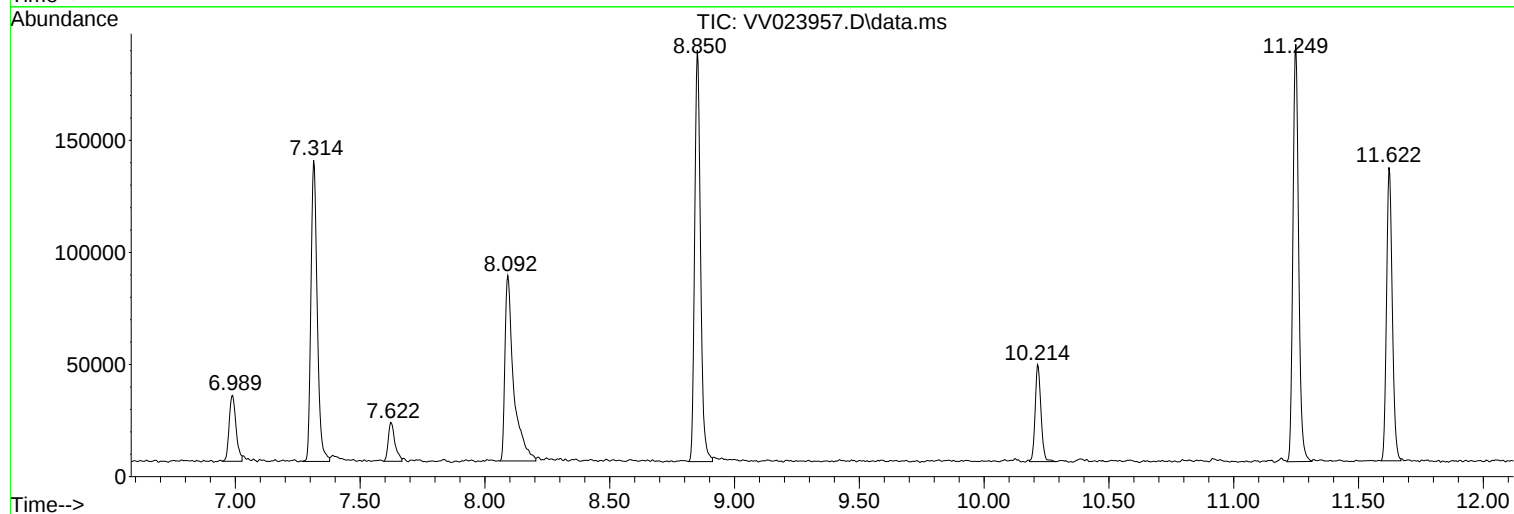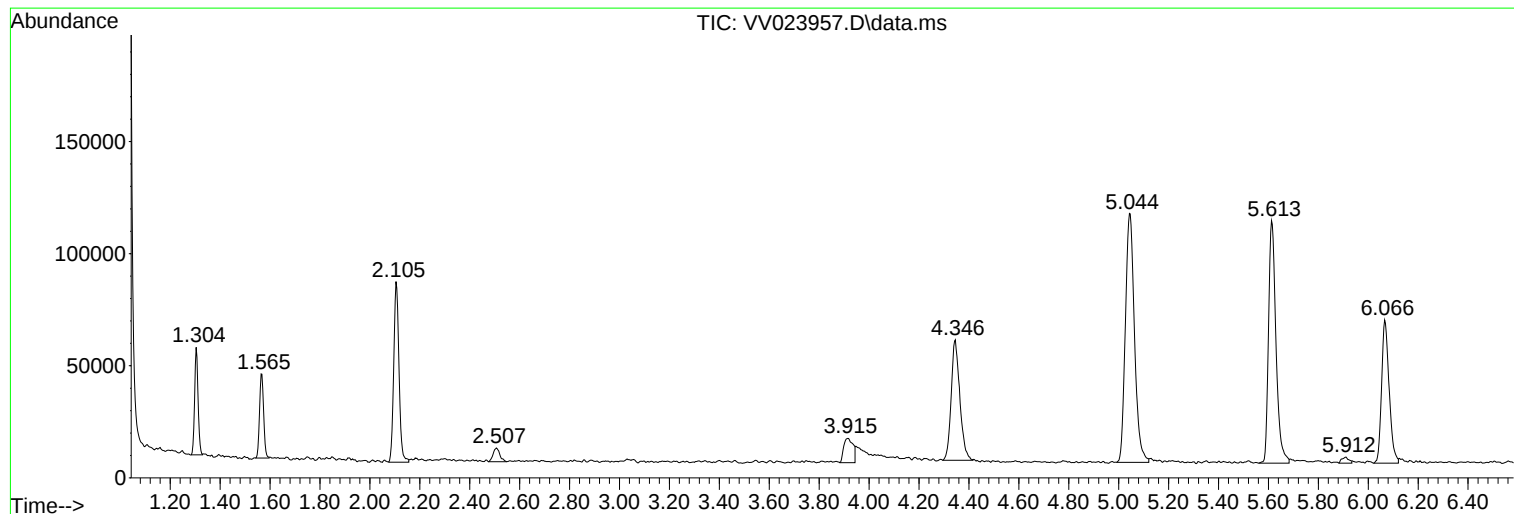

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV121421\  
Data File : VV023958.D  
Acq On : 14 Dec 2021 10:44  
Operator : SY/MD  
Sample : VV1214WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR121021WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV121421\  
Data File : VV023958.D  
Acq On : 14 Dec 2021 10:44  
Operator : SY/MD  
Sample : VV1214WBL01  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR121021WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |