

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
 Data File : VV023970.D
 Acq On : 14 Dec 2021 15:42
 Operator : SY/MD
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK245

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023970.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	93	rVB	43446	43577	15.47%	1.923%
2	1.568	156	164	176	rBV	36301	41840	14.86%	1.846%
3	2.108	321	332	350	rBV	77567	109228	38.78%	4.820%
4	2.506	447	456	470	rBV3	8262	13605	4.83%	0.600%
5	3.921	885	896	924	rBV2	10681	47231	16.77%	2.084%
6	4.349	1014	1029	1030	rBV2	46989	66031	23.44%	2.914%
7	5.047	1229	1246	1278	rBV4	104879	270308	95.97%	11.929%
8	5.619	1408	1424	1448	rBV	100948	210245	74.65%	9.278%
9	5.915	1508	1516	1524	rBV6	1922	3387	1.20%	0.149%
10	6.072	1552	1565	1593	rBV	59651	124886	44.34%	5.511%
11	6.989	1840	1850	1874	rBV2	27825	54887	19.49%	2.422%
12	7.317	1938	1952	1971	rBV	124451	222426	78.97%	9.816%
13	7.625	2033	2048	2073	rBV	16069	32331	11.48%	1.427%
14	8.095	2184	2194	2222	rBV	82986	192961	68.51%	8.516%
15	8.853	2418	2430	2453	rBV	169920	281653	100.00%	12.430%
16	10.217	2844	2854	2869	rBV2	40968	65576	23.28%	2.894%
17	10.381	2896	2905	2915	rBV3	2576	4011	1.42%	0.177%
18	11.249	3165	3175	3194	rBV	174524	276663	98.23%	12.210%
19	11.625	3281	3292	3308	rBV	123191	201881	71.68%	8.909%
20	12.249	3477	3486	3495	rBV2	2360	3230	1.15%	0.143%




Sum of corrected areas: 2265957

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
Data File : VV023970.D
Acq On : 14 Dec 2021 15:42
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

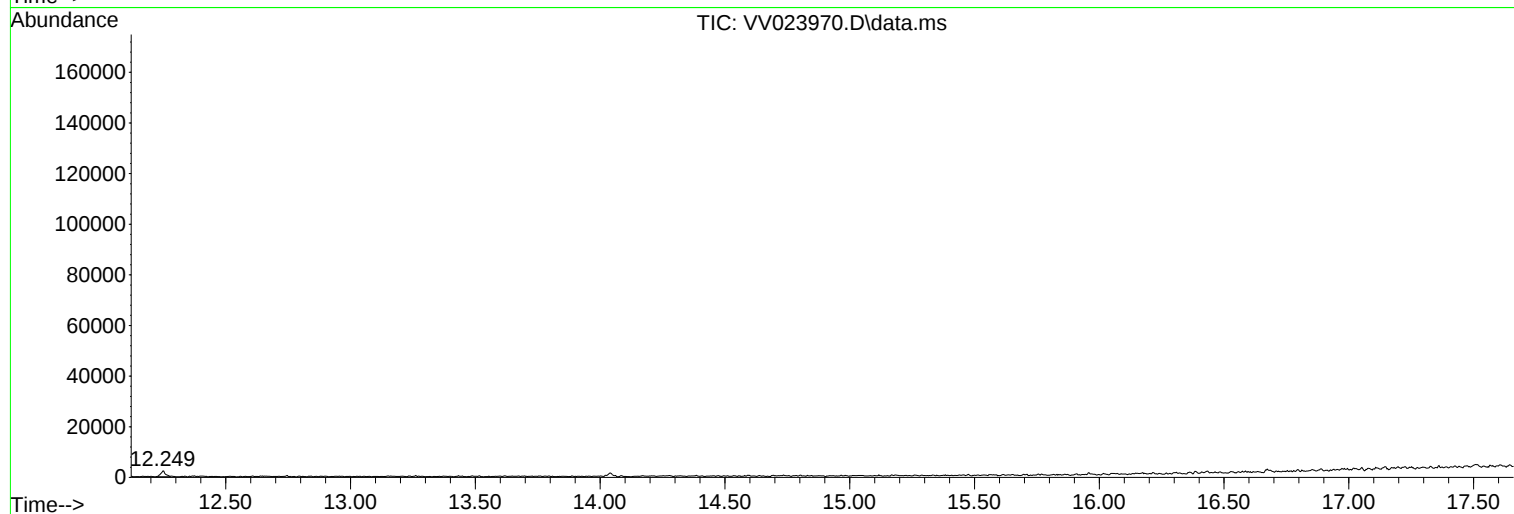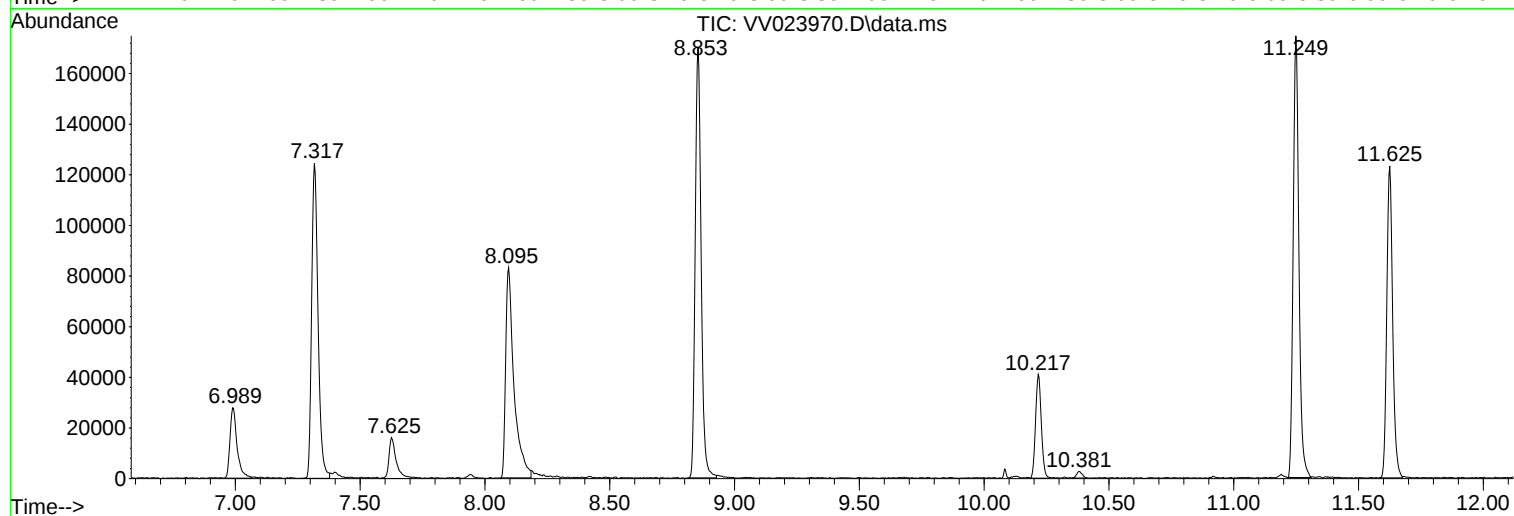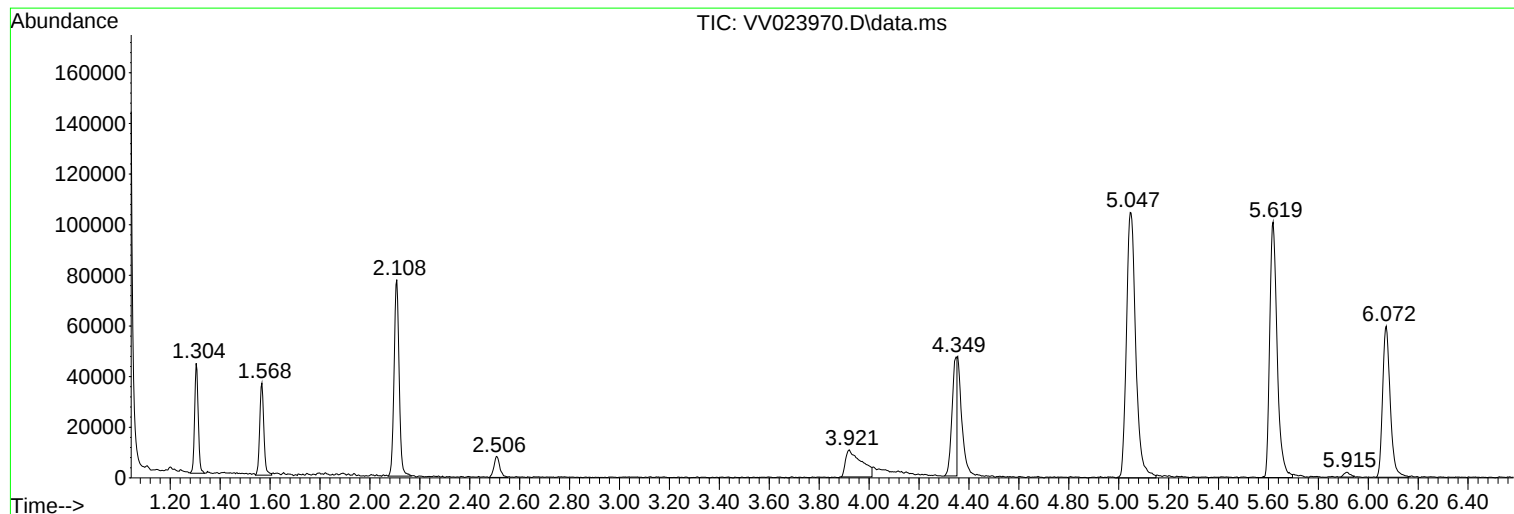

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
Data File : VV023970.D
Acq On : 14 Dec 2021 15:42
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
Data File : VV023970.D
Acq On : 14 Dec 2021 15:42
Operator : SY/MD
Sample : VIBLK
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
