

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
 Data File : VV023975.D
 Acq On : 14 Dec 2021 17:48
 Operator : SY/MD
 Sample : M5005-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	73	82	94	rVB	44824	47574	16.11%	1.977%
2	1.568	155	164	172	rBV	38761	43087	14.59%	1.791%
3	2.108	322	332	346	rBV	79333	110768	37.50%	4.603%
4	2.506	445	456	472	rVB2	9134	15221	5.15%	0.633%
5	3.918	885	895	912	rBV	11255	38504	13.04%	1.600%
6	4.349	1013	1029	1052	rVB2	53473	132122	44.73%	5.491%
7	5.050	1229	1247	1276	rBV3	110872	276826	93.72%	11.504%
8	5.616	1412	1423	1448	rBV	105571	219688	74.37%	9.130%
9	5.911	1507	1515	1522	rBV7	2585	4891	1.66%	0.203%
10	6.072	1553	1565	1594	rBV	64609	133451	45.18%	5.546%
11	6.989	1836	1850	1866	rBV3	29258	55915	18.93%	2.324%
12	7.316	1941	1952	1973	rBV	128533	229436	77.67%	9.535%
13	7.625	2039	2048	2064	rBV2	17599	33422	11.31%	1.389%
14	8.095	2184	2194	2226	rBV	84269	207759	70.34%	8.634%
15	8.853	2415	2430	2454	rBV	175375	295383	100.00%	12.275%
16	10.217	2843	2854	2869	rBV	41894	67869	22.98%	2.820%
17	10.381	2899	2905	2914	rVB4	3146	4263	1.44%	0.177%
18	11.249	3164	3175	3202	rBV	178714	282621	95.68%	11.745%
19	11.625	3280	3292	3308	rBV	127876	203785	68.99%	8.469%
20	12.249	3477	3486	3495	rVB3	2407	3758	1.27%	0.156%




Sum of corrected areas: 2406343

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
Data File : VV023975.D
Acq On : 14 Dec 2021 17:48
Operator : SY/MD
Sample : M5005-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

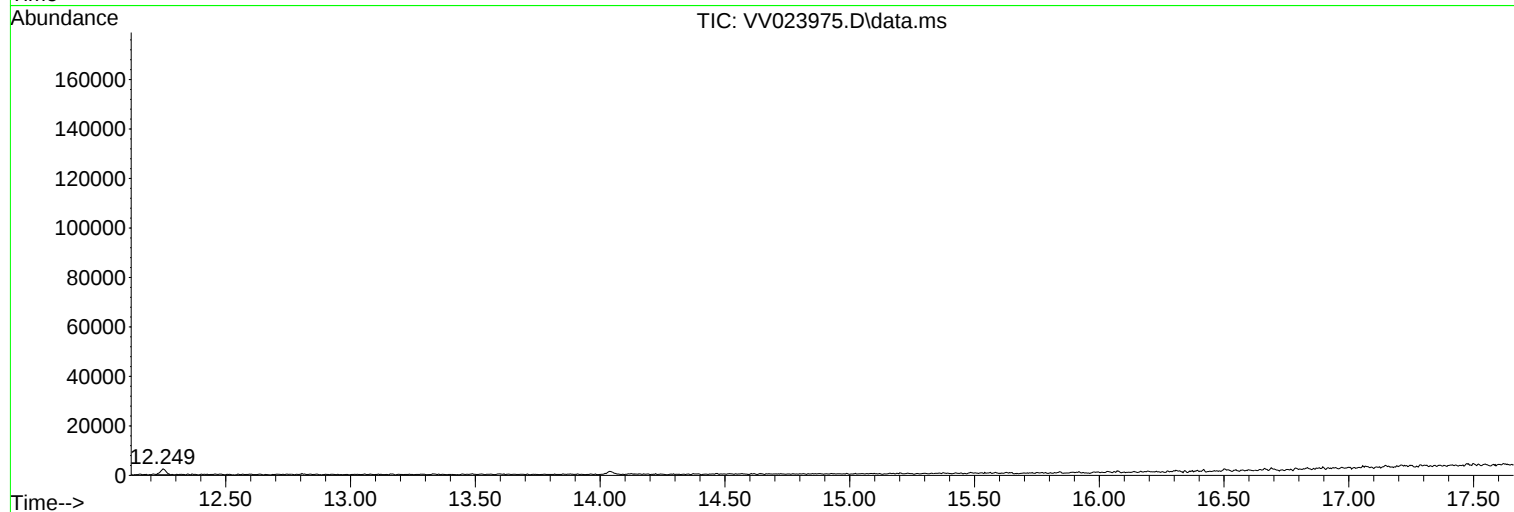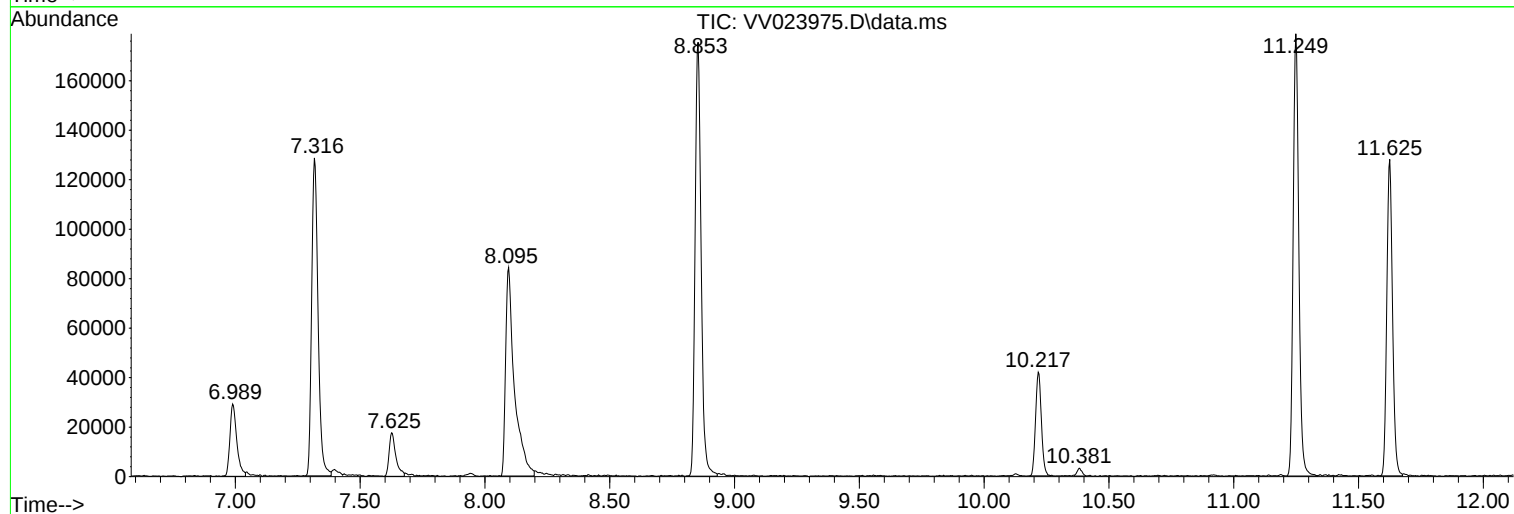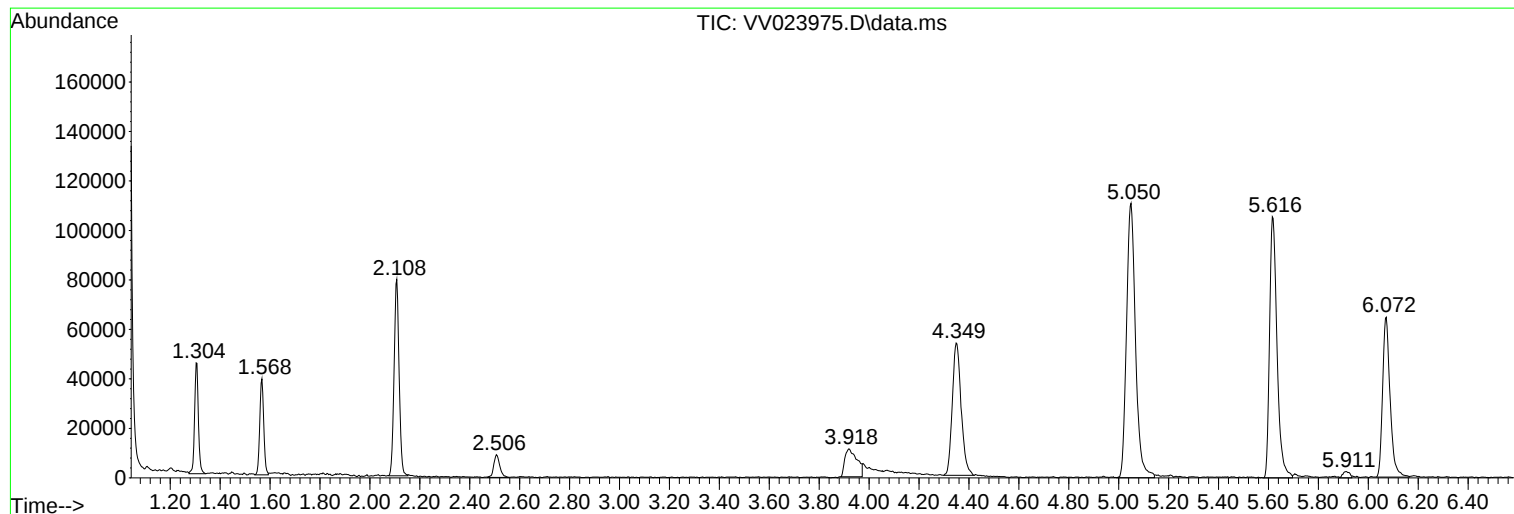

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
Data File : VV023975.D
Acq On : 14 Dec 2021 17:48
Operator : SY/MD
Sample : M5005-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
Data File : VV023975.D
Acq On : 14 Dec 2021 17:48
Operator : SY/MD
Sample : M5005-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc