

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
 Data File : VV023976.D
 Acq On : 14 Dec 2021 18:12
 Operator : SY/MD
 Sample : M5006-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	48156	48421	16.10%	1.960%
2	1.568	155	164	175	rBV	39269	45332	15.07%	1.835%
3	2.108	321	332	350	rVB	83571	120535	40.08%	4.878%
4	2.510	446	457	468	rBV3	7454	13129	4.37%	0.531%
5	3.915	881	894	897	rBV	11506	18600	6.18%	0.753%
6	4.349	1015	1029	1055	rBV	56420	135912	45.19%	5.501%
7	5.050	1232	1247	1276	rBV2	119148	300761	100.00%	12.172%
8	5.619	1411	1424	1452	rBV	103741	215833	71.76%	8.735%
9	5.918	1505	1517	1521	rBV5	2505	4108	1.37%	0.166%
10	6.072	1550	1565	1588	rBV2	66622	141286	46.98%	5.718%
11	6.989	1839	1850	1866	rBV	30564	59051	19.63%	2.390%
12	7.317	1936	1952	1974	rBV	140824	251168	83.51%	10.165%
13	7.394	1974	1976	1991	rVB3	2324	3360	1.12%	0.136%
14	7.625	2040	2048	2073	rBV2	16878	32308	10.74%	1.308%
15	8.095	2183	2194	2235	rBV	91342	222706	74.05%	9.013%
16	8.854	2418	2430	2448	rBV	174684	290010	96.43%	11.737%
17	10.217	2844	2854	2865	rBV	45768	71707	23.84%	2.902%
18	11.249	3164	3175	3192	rBV	175519	274848	91.38%	11.124%
19	11.625	3280	3292	3307	rBV	136512	217703	72.38%	8.811%
20	12.252	3471	3487	3497	rVB3	2240	4051	1.35%	0.164%




Sum of corrected areas: 2470829

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
Data File : VV023976.D
Acq On : 14 Dec 2021 18:12
Operator : SY/MD
Sample : M5006-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

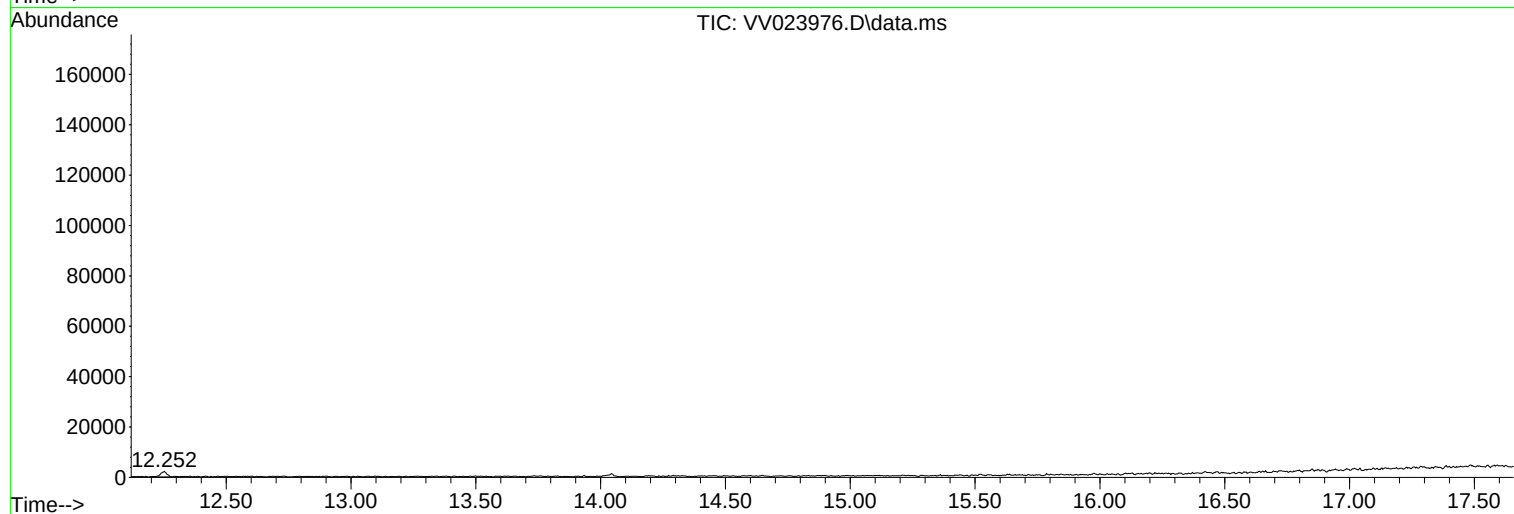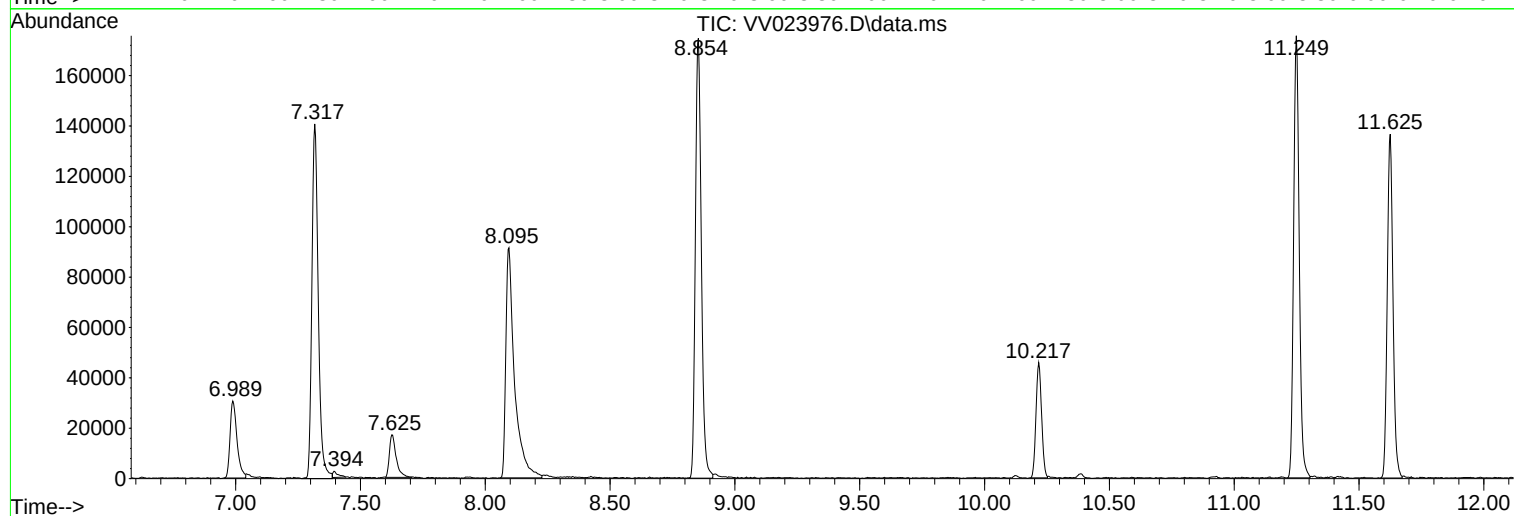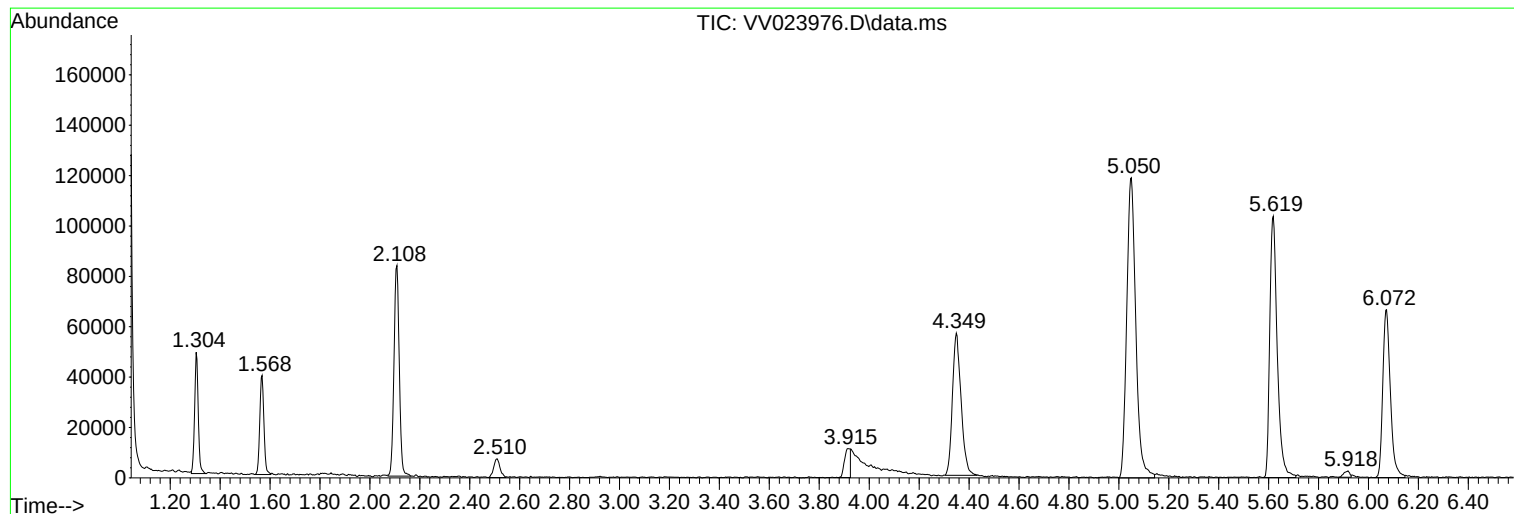

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
Data File : VV023976.D
Acq On : 14 Dec 2021 18:12
Operator : SY/MD
Sample : M5006-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121421\
Data File : VV023976.D
Acq On : 14 Dec 2021 18:12
Operator : SY/MD
Sample : M5006-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121021WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
