

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121422\
 Data File : VV029688.D
 Acq On : 14 Dec 2022 14:19
 Operator : SY/MD
 Sample : N5981-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	212348	211776	14.28%	1.722%
2	1.561	155	162	176	rVB	176738	198564	13.39%	1.615%
3	2.105	320	331	360	rBV	347515	504151	34.00%	4.100%
4	2.291	380	389	398	rVB	3128	4926	0.33%	0.040%
5	2.362	408	411	413	rBV2	213	122	0.01%	0.001%
6	2.507	447	456	466	rVB	4948	7716	0.52%	0.063%
7	2.580	476	479	481	rVB2	210	113	0.01%	0.001%
8	2.593	481	483	486	rBV	156	113	0.01%	0.001%
9	2.764	526	536	549	rBV4	5182	9286	0.63%	0.076%
10	2.880	568	572	577	rBV2	227	230	0.02%	0.002%
11	2.902	577	579	582	rBV3	185	110	0.01%	0.001%
12	3.079	629	634	636	rBV2	187	179	0.01%	0.001%
13	3.185	658	667	679	rVB2	1152	2583	0.17%	0.021%
14	3.307	702	705	709	rVB	160	126	0.01%	0.001%
15	3.343	709	716	718	rBV2	189	195	0.01%	0.002%
16	3.429	739	743	746	rVV4	305	233	0.02%	0.002%
17	3.539	775	777	784	rVB2	234	187	0.01%	0.002%
18	3.584	784	791	798	rBV2	204	256	0.02%	0.002%
19	3.696	822	826	830	rBV2	271	299	0.02%	0.002%
20	3.793	853	856	863	rBV2	262	245	0.02%	0.002%
21	3.825	863	866	870	rBV	133	109	0.01%	0.001%
22	3.870	871	880	920	rBV	122621	351478	23.70%	2.858%
23	4.339	1010	1026	1057	rBV	228730	571789	38.56%	4.650%
24	4.596	1098	1106	1107	rBV2	1552	1342	0.09%	0.011%
25	4.738	1146	1150	1152	rBV2	165	136	0.01%	0.001%
26	4.883	1192	1195	1199	rVB2	242	154	0.01%	0.001%
27	4.928	1205	1209	1213	rBV2	176	155	0.01%	0.001%
28	5.040	1223	1244	1287	rBV2	560613	1482960	100.00%	12.059%
29	5.391	1350	1353	1359	rBV4	380	444	0.03%	0.004%
30	5.452	1369	1372	1374	rBV2	159	124	0.01%	0.001%
31	5.468	1374	1377	1379	rVV2	282	167	0.01%	0.001%
32	5.519	1389	1393	1396	rVB2	178	118	0.01%	0.001%
33	5.548	1399	1402	1403	rBV	220	138	0.01%	0.001%
34	5.609	1407	1421	1451	rBV	522202	1063951	71.75%	8.652%
35	5.905	1502	1513	1528	rBV6	8036	18325	1.24%	0.149%
36	6.063	1547	1562	1591	rBV	319693	668199	45.06%	5.434%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121422\
 Data File : VW029688.D
 Acq On : 14 Dec 2022 14:19
 Operator : SY/MD
 Sample : N5981-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.259	1621	1623	1629	rVB2	476	247	0.02%	0.002%
38	6.288	1629	1632	1635	rBV2	354	191	0.01%	0.002%
39	6.323	1640	1643	1647	rBV	224	141	0.01%	0.001%
40	6.510	1693	1701	1711	rVV2	1418	2412	0.16%	0.020%
41	6.625	1733	1737	1741	rVV3	628	656	0.04%	0.005%
42	6.847	1804	1806	1810	rVB2	195	109	0.01%	0.001%
43	6.876	1810	1815	1816	rBV2	322	170	0.01%	0.001%
44	6.915	1824	1827	1830	rBV	171	114	0.01%	0.001%
45	6.979	1836	1847	1885	rBV	160046	301009	20.30%	2.448%
46	7.153	1899	1901	1903	rBB2	411	135	0.01%	0.001%
47	7.178	1907	1909	1911	rVB2	506	177	0.01%	0.001%
48	7.236	1920	1927	1936	rBV5	3340	5048	0.34%	0.041%
49	7.307	1937	1949	1970	rBV	671461	1184932	79.90%	9.635%
50	7.612	2034	2044	2075	rBV	114560	206003	13.89%	1.675%
51	7.902	2130	2134	2135	rBV2	264	188	0.01%	0.002%
52	8.082	2180	2190	2232	rBV	417038	768539	51.82%	6.249%
53	8.416	2286	2294	2298	rBV5	1222	1764	0.12%	0.014%
54	8.481	2310	2314	2317	rBV3	497	353	0.02%	0.003%
55	8.590	2345	2348	2349	rBV	481	229	0.02%	0.002%
56	8.628	2357	2360	2361	rBV2	242	148	0.01%	0.001%
57	8.667	2370	2372	2374	rBV2	245	121	0.01%	0.001%
58	8.722	2384	2389	2392	rBV2	277	286	0.02%	0.002%
59	8.741	2392	2395	2400	rVB2	282	270	0.02%	0.002%
60	8.792	2410	2411	2415	rBV2	196	123	0.01%	0.001%
61	8.844	2415	2427	2455	rBV	767356	1267277	85.46%	10.305%
62	9.008	2471	2478	2488	rVB2	5689	8419	0.57%	0.068%
63	9.133	2510	2517	2529	rVB4	5402	8566	0.58%	0.070%
64	9.288	2559	2565	2567	rBV	233	261	0.02%	0.002%
65	9.423	2603	2607	2608	rBV2	296	182	0.01%	0.001%
66	9.535	2634	2642	2644	rBV2	5558	5637	0.38%	0.046%
67	9.718	2693	2699	2709	rVB5	1294	2184	0.15%	0.018%
68	9.783	2715	2719	2724	rBV3	378	378	0.03%	0.003%
69	9.847	2735	2739	2741	rVB	188	119	0.01%	0.001%
70	9.879	2745	2749	2751	rVV2	265	154	0.01%	0.001%
71	9.921	2754	2762	2774	rBV2	6037	9095	0.61%	0.074%
72	10.008	2786	2789	2792	rVB2	190	121	0.01%	0.001%
73	10.069	2803	2808	2809	rBV	171	155	0.01%	0.001%
74	10.108	2815	2820	2821	rBV	229	154	0.01%	0.001%
75	10.162	2825	2837	2841	rBV	18492	26869	1.81%	0.218%
76	10.207	2842	2851	2877	rVB	491978	779416	52.56%	6.338%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121422\
 Data File : VV029688.D
 Acq On : 14 Dec 2022 14:19
 Operator : SY/MD
 Sample : N5981-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.320	2885	2886	2889	rVB2	360	136	0.01%	0.001%
78	10.374	2893	2903	2907	rBV4	992	1523	0.10%	0.012%
79	10.432	2919	2921	2929	rVB2	261	199	0.01%	0.002%
80	10.468	2929	2932	2940	rBV3	393	361	0.02%	0.003%
81	10.529	2942	2951	2957	rBV2	6077	8728	0.59%	0.071%
82	10.654	2985	2990	2993	rBV	246	255	0.02%	0.002%
83	10.722	3008	3011	3014	rBV2	248	157	0.01%	0.001%
84	10.792	3030	3033	3035	rBV2	161	143	0.01%	0.001%
85	10.905	3060	3068	3080	rBV2	7150	9217	0.62%	0.075%
86	11.101	3125	3129	3131	rBV	196	156	0.01%	0.001%
87	11.175	3144	3152	3160	rBV4	5548	8405	0.57%	0.068%
88	11.239	3160	3172	3201	rBV	858661	1346683	90.81%	10.951%
89	11.612	3276	3288	3314	rBV	748787	1184590	79.88%	9.633%
90	11.831	3353	3356	3361	rBV2	400	263	0.02%	0.002%
91	11.879	3367	3371	3373	rBV3	391	276	0.02%	0.002%
92	11.969	3396	3399	3400	rBV2	230	112	0.01%	0.001%
93	12.107	3439	3442	3445	rBV2	239	174	0.01%	0.001%
94	12.451	3546	3549	3550	rBV	405	206	0.01%	0.002%
95	12.635	3599	3606	3620	rVB3	6621	10038	0.68%	0.082%
96	12.805	3657	3659	3662	rBV2	256	118	0.01%	0.001%
97	13.185	3774	3777	3779	rBV2	370	244	0.02%	0.002%
98	13.252	3790	3798	3807	rBV3	6845	10307	0.70%	0.084%
99	13.496	3865	3874	3885	rBV2	13324	20909	1.41%	0.170%
100	13.731	3940	3947	3957	rVB2	7559	11088	0.75%	0.090%




Sum of corrected areas: 12297639

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121422\
Data File : VV029688.D
Acq On : 14 Dec 2022 14:19
Operator : SY/MD
Sample : N5981-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

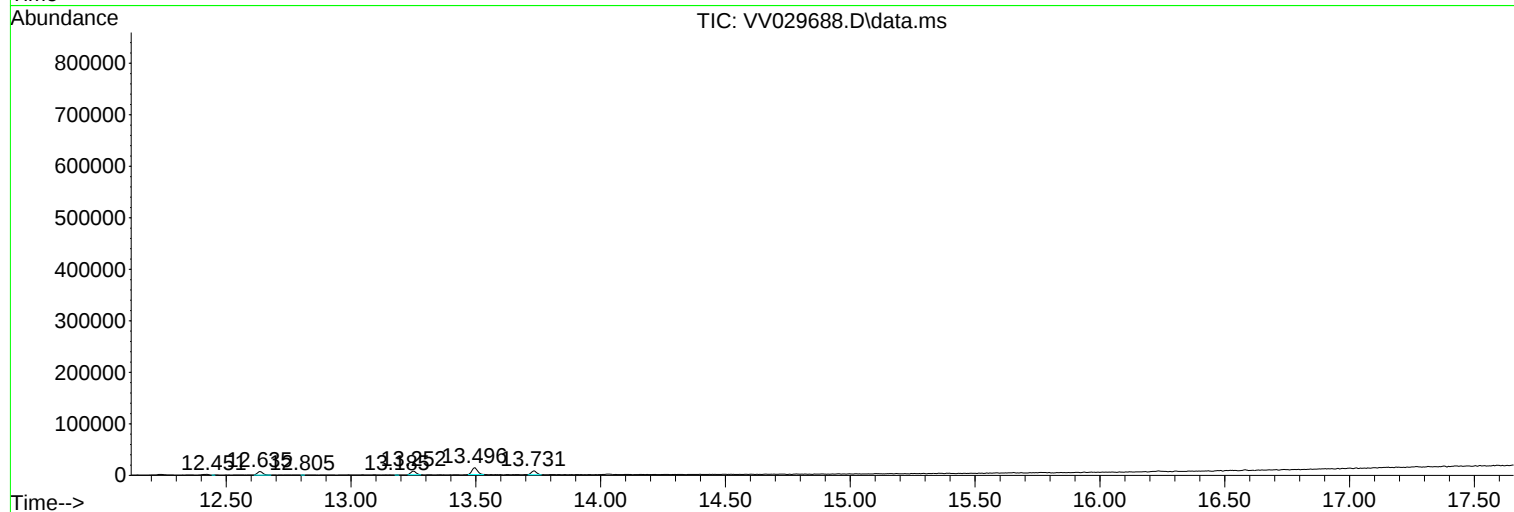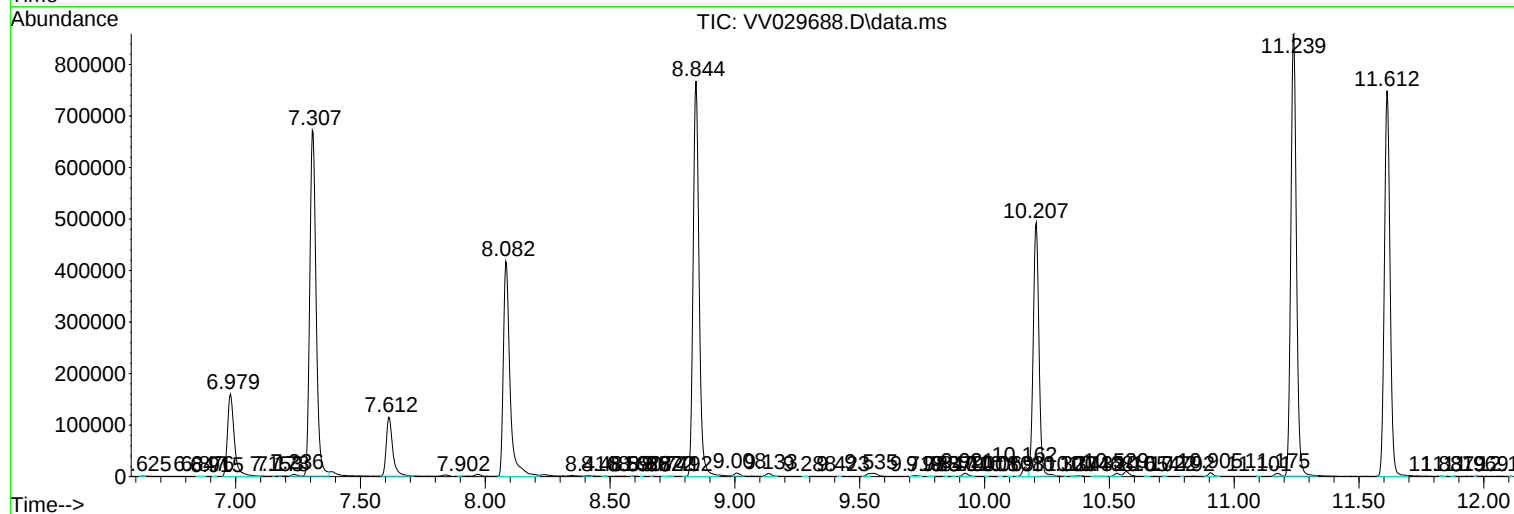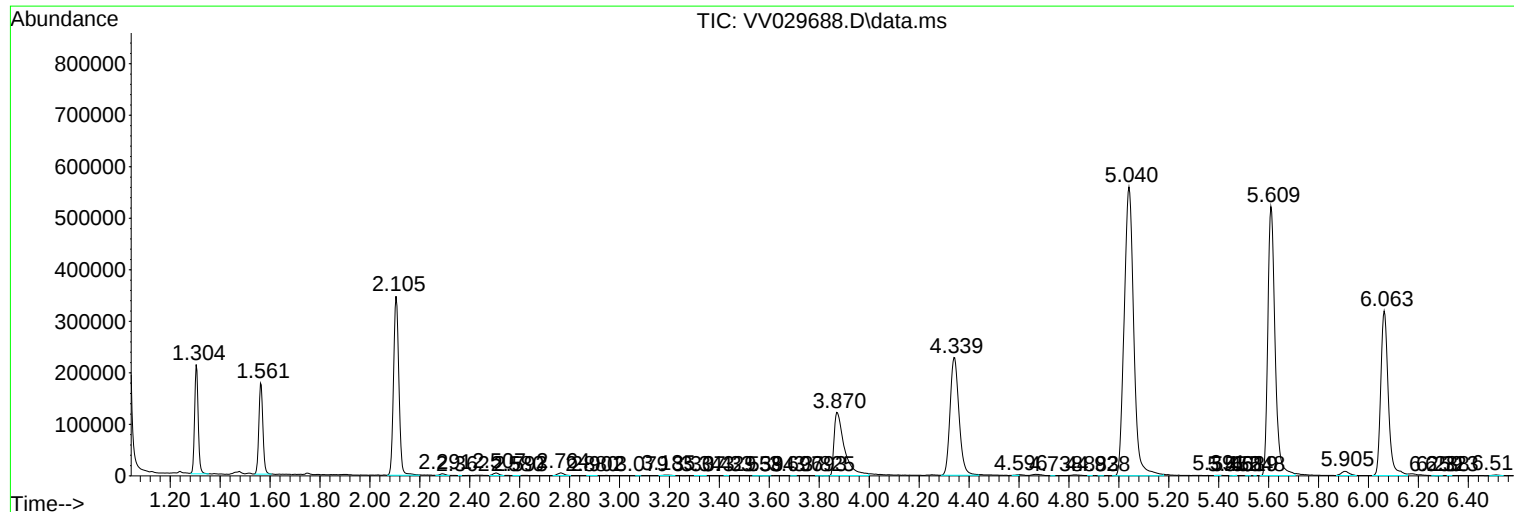

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121422\
Data File : VV029688.D
Acq On : 14 Dec 2022 14:19
Operator : SY/MD
Sample : N5981-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121422\
Data File : VV029688.D
Acq On : 14 Dec 2022 14:19
Operator : SY/MD
Sample : N5981-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc