

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121422\
 Data File : VV029689.D
 Acq On : 14 Dec 2022 14:43
 Operator : SY/MD
 Sample : N5980-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	185293	187002	13.48%	1.637%
2	1.561	155	162	173	rVB	160992	179473	12.94%	1.571%
3	2.105	320	331	343	rBV	309304	443165	31.94%	3.880%
4	2.375	413	415	418	rBV	234	145	0.01%	0.001%
5	2.503	447	455	465	rVB2	5480	8747	0.63%	0.077%
6	2.610	482	488	491	rBV3	569	622	0.04%	0.005%
7	2.764	527	536	550	rVB5	4866	8941	0.64%	0.078%
8	2.873	565	570	572	rBV2	333	262	0.02%	0.002%
9	2.947	590	593	601	rVB3	199	176	0.01%	0.002%
10	3.127	646	649	651	rBV3	213	124	0.01%	0.001%
11	3.172	659	663	664	rBV2	737	449	0.03%	0.004%
12	3.301	698	703	705	rBV	206	202	0.01%	0.002%
13	3.381	724	728	731	rVB2	178	133	0.01%	0.001%
14	3.420	735	740	742	rBV	153	130	0.01%	0.001%
15	3.478	750	758	759	rBV2	241	215	0.02%	0.002%
16	3.487	759	761	766	rVB	195	142	0.01%	0.001%
17	3.536	773	776	778	rBV	264	163	0.01%	0.001%
18	3.590	791	793	795	rVB	305	92	0.01%	0.001%
19	3.613	795	800	801	rBV2	233	174	0.01%	0.002%
20	3.873	871	881	922	rBV	123751	369322	26.62%	3.233%
21	4.339	1010	1026	1061	rBV	214714	535392	38.59%	4.687%
22	4.606	1098	1109	1118	rVV7	1612	3712	0.27%	0.032%
23	4.664	1118	1127	1142	rVB8	2171	5438	0.39%	0.048%
24	4.719	1142	1144	1147	rBV2	294	170	0.01%	0.001%
25	4.818	1167	1175	1178	rBV5	1281	1901	0.14%	0.017%
26	4.867	1188	1190	1192	rVB	310	113	0.01%	0.001%
27	4.883	1192	1195	1198	rBV2	156	100	0.01%	0.001%
28	4.902	1198	1201	1203	rBV	187	94	0.01%	0.001%
29	5.037	1225	1243	1287	rBV2	514983	1387315	100.00%	12.145%
30	5.394	1352	1354	1358	rBV3	293	224	0.02%	0.002%
31	5.445	1367	1370	1373	rBV2	227	162	0.01%	0.001%
32	5.561	1403	1406	1408	rBV2	239	118	0.01%	0.001%
33	5.609	1408	1421	1464	rBV	469666	975080	70.29%	8.536%
34	5.905	1502	1513	1529	rBV8	7179	17249	1.24%	0.151%
35	6.063	1548	1562	1589	rBV	305481	632495	45.59%	5.537%
36	6.256	1619	1622	1627	rVB2	305	225	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121422\
 Data File : VW029689.D
 Acq On : 14 Dec 2022 14:43
 Operator : SY/MD
 Sample : N5980-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.442	1677	1680	1683	rBV2	221	155	0.01%	0.001%
38	6.513	1693	1702	1711	rVB5	1384	2495	0.18%	0.022%
39	6.561	1715	1717	1721	rVB	268	124	0.01%	0.001%
40	6.632	1734	1739	1741	rBV2	697	629	0.05%	0.006%
41	6.719	1763	1766	1769	rVB2	205	139	0.01%	0.001%
42	6.757	1776	1778	1783	rVB2	230	124	0.01%	0.001%
43	6.796	1788	1790	1793	rVB	292	101	0.01%	0.001%
44	6.867	1808	1812	1814	rBV	276	175	0.01%	0.002%
45	6.924	1826	1830	1833	rVB	358	293	0.02%	0.003%
46	6.979	1835	1847	1885	rBV	150652	288620	20.80%	2.527%
47	7.108	1885	1887	1889	rBV	370	146	0.01%	0.001%
48	7.233	1921	1926	1937	rVB6	3377	4867	0.35%	0.043%
49	7.307	1937	1949	1970	rBV	613371	1077638	77.68%	9.434%
50	7.613	2034	2044	2069	rBV	107914	197654	14.25%	1.730%
51	7.969	2148	2155	2164	rVB6	3531	5626	0.41%	0.049%
52	8.082	2180	2190	2230	rBV	415317	755166	54.43%	6.611%
53	8.416	2286	2294	2301	rBV5	2057	3091	0.22%	0.027%
54	8.490	2313	2317	2321	rBV3	585	503	0.04%	0.004%
55	8.513	2321	2324	2328	rVB	533	348	0.03%	0.003%
56	8.535	2328	2331	2333	rBV2	480	303	0.02%	0.003%
57	8.564	2336	2340	2343	rBV	306	203	0.01%	0.002%
58	8.658	2367	2369	2371	rBV	219	140	0.01%	0.001%
59	8.680	2371	2376	2381	rVB2	461	576	0.04%	0.005%
60	8.786	2405	2409	2411	rBV	351	246	0.02%	0.002%
61	8.844	2413	2427	2453	rBV	694391	1163868	83.89%	10.189%
62	9.008	2473	2478	2489	rVB3	5149	7397	0.53%	0.065%
63	9.137	2509	2518	2532	rVB	4869	8453	0.61%	0.074%
64	9.191	2532	2535	2538	rBV	292	173	0.01%	0.002%
65	9.297	2566	2568	2569	rBV	182	88	0.01%	0.001%
66	9.333	2575	2579	2580	rBV	238	159	0.01%	0.001%
67	9.381	2592	2594	2597	rBV	216	109	0.01%	0.001%
68	9.474	2619	2623	2624	rBV	236	168	0.01%	0.001%
69	9.542	2634	2644	2647	rBV2	5572	8168	0.59%	0.072%
70	9.725	2694	2701	2709	rVB5	1376	1923	0.14%	0.017%
71	9.760	2709	2712	2714	rBV2	244	158	0.01%	0.001%
72	9.789	2718	2721	2725	rBV2	184	122	0.01%	0.001%
73	9.866	2742	2745	2748	rBV	327	235	0.02%	0.002%
74	9.924	2755	2763	2774	rVB2	5241	7524	0.54%	0.066%
75	10.002	2783	2787	2789	rBV2	149	115	0.01%	0.001%
76	10.050	2800	2802	2806	rBV3	176	98	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121422\
 Data File : VV029689.D
 Acq On : 14 Dec 2022 14:43
 Operator : SY/MD
 Sample : N5980-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.162	2828	2837	2840	rBV2	17000	22494	1.62%	0.197%
78	10.204	2841	2850	2878	rVB	479845	756524	54.53%	6.623%
79	10.371	2895	2902	2910	rBV4	1258	1505	0.11%	0.013%
80	10.529	2945	2951	2956	rBV3	5296	6707	0.48%	0.059%
81	10.664	2990	2993	2998	rVB2	191	145	0.01%	0.001%
82	10.693	3000	3002	3004	rVV2	236	95	0.01%	0.001%
83	10.776	3024	3028	3031	rBV3	238	240	0.02%	0.002%
84	10.844	3047	3049	3050	rBV	212	91	0.01%	0.001%
85	10.905	3059	3068	3081	rBV	5380	7921	0.57%	0.069%
86	11.005	3096	3099	3105	rVB3	246	222	0.02%	0.002%
87	11.075	3117	3121	3122	rBV2	348	205	0.01%	0.002%
88	11.172	3145	3151	3160	rBV	4975	6890	0.50%	0.060%
89	11.236	3160	3171	3197	rBV	766858	1209921	87.21%	10.592%
90	11.403	3219	3223	3224	rBV	627	448	0.03%	0.004%
91	11.519	3257	3259	3263	rVB2	378	192	0.01%	0.002%
92	11.612	3274	3288	3323	rBV	670422	1080088	77.85%	9.456%
93	11.837	3356	3358	3361	rBV2	203	131	0.01%	0.001%
94	11.947	3390	3392	3396	rBV3	355	209	0.02%	0.002%
95	11.985	3402	3404	3406	rBV2	397	187	0.01%	0.002%
96	12.362	3519	3521	3523	rBV	335	167	0.01%	0.001%
97	12.635	3598	3606	3615	rVB3	5424	8067	0.58%	0.071%
98	12.718	3630	3632	3634	rBV	280	151	0.01%	0.001%
99	13.252	3791	3798	3809	rVB4	5802	8292	0.60%	0.073%
100	13.497	3866	3874	3883	rVB	8997	14077	1.01%	0.123%




Sum of corrected areas: 11422556

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121422\
Data File : VV029689.D
Acq On : 14 Dec 2022 14:43
Operator : SY/MD
Sample : N5980-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

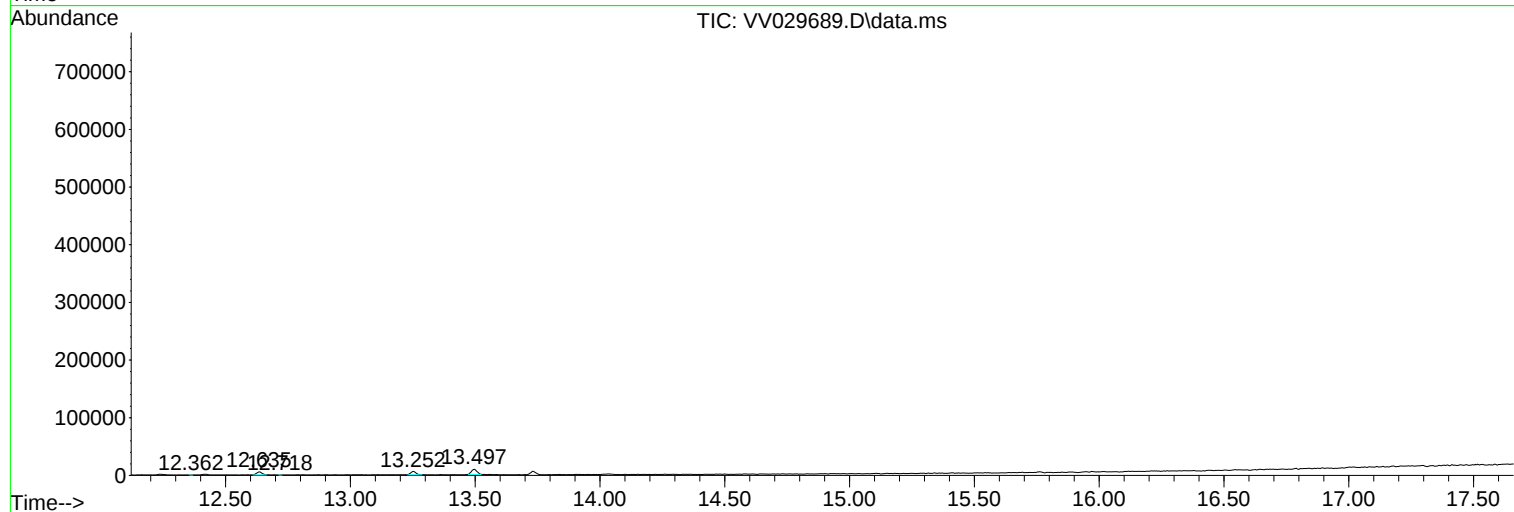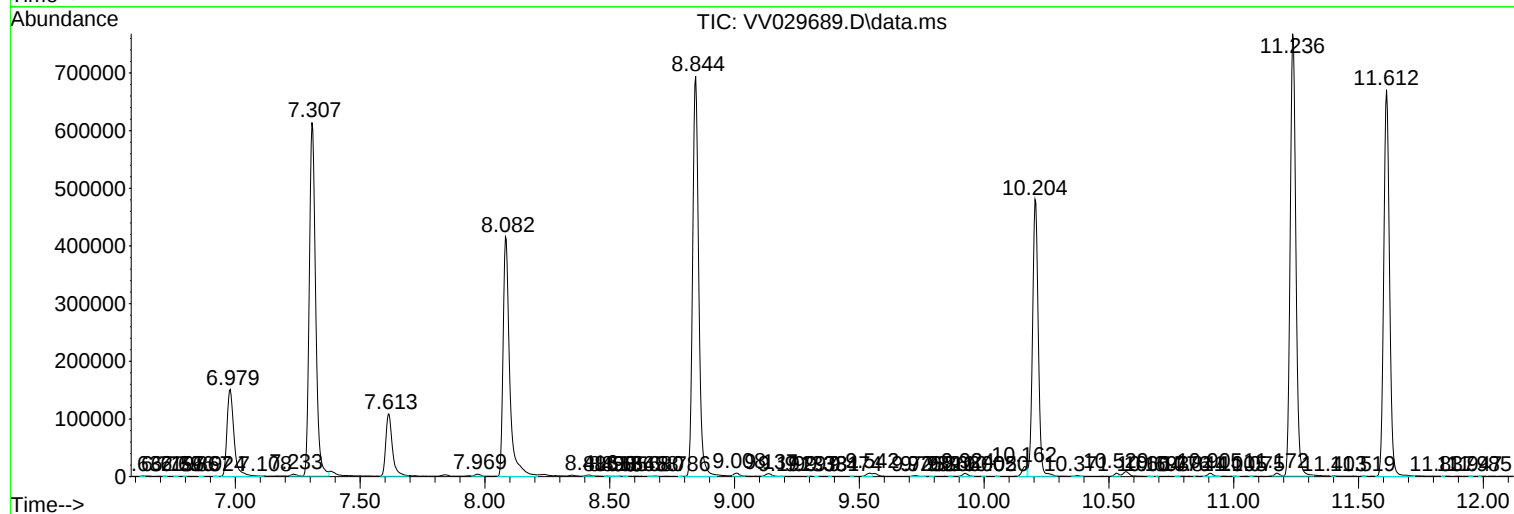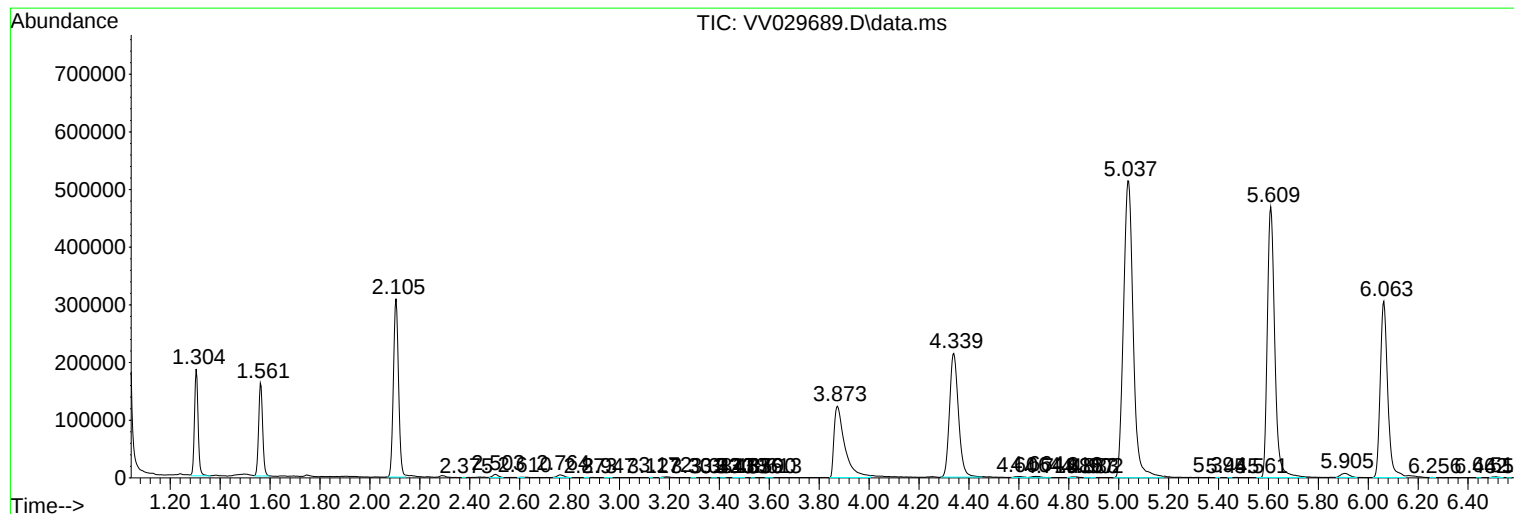

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121422\
Data File : VV029689.D
Acq On : 14 Dec 2022 14:43
Operator : SY/MD
Sample : N5980-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121422\
Data File : VV029689.D
Acq On : 14 Dec 2022 14:43
Operator : SY/MD
Sample : N5980-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc