
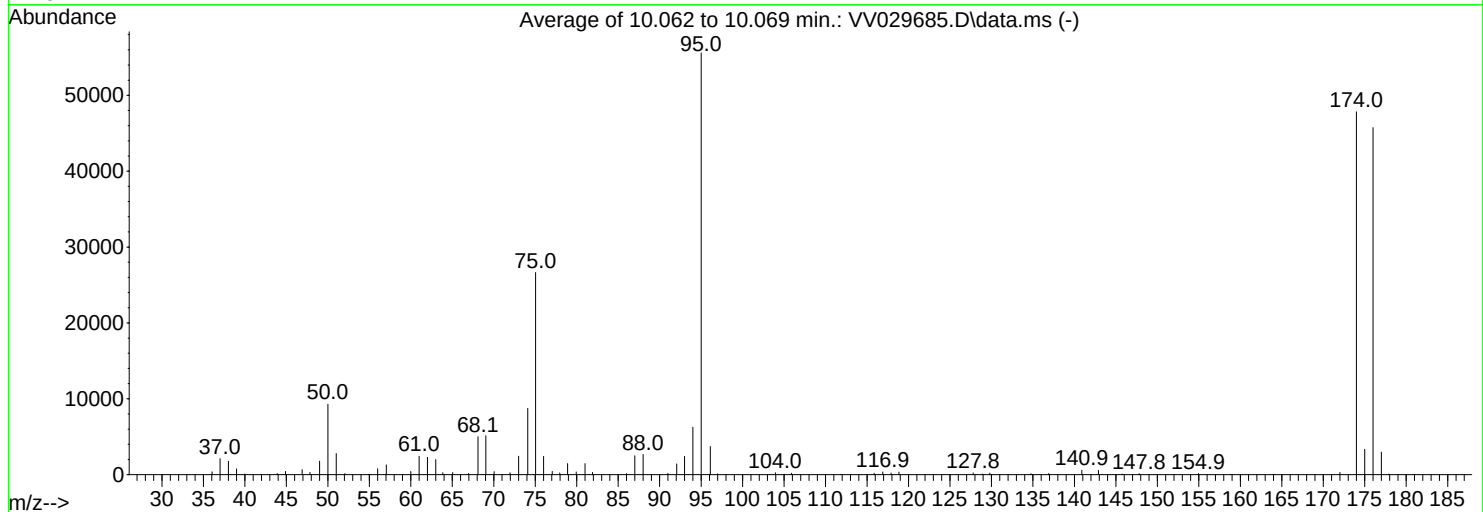


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121422\
 Data File : VV029685.D
 Acq On : 14 Dec 2022 12:39
 Operator : SY/MD
 Sample : BFB356
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB356

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 14 21:14:52 2022

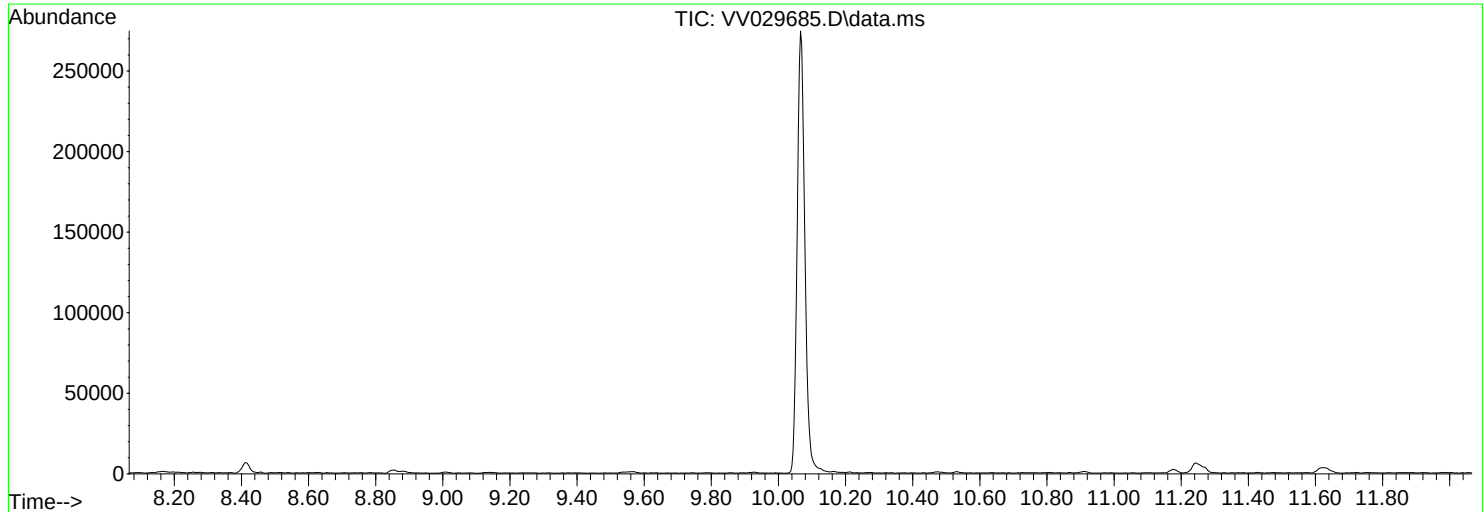

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	9285	PASS
75	95	30	80	47.9	26632	PASS
95	95	100	100	100.0	55600	PASS
96	95	5	9	6.7	3716	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.0	47827	PASS
175	174	5	9	7.0	3333	PASS
176	174	95	105	95.7	45752	PASS
177	176	5	10	6.5	2978	PASS

m/z	Abundance
39.90	184.0
43.90	363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356

m/z	Abundance
36.10	384.0
37.00	2000.0
38.00	1732.0
39.00	717.0
40.10	246.0
43.90	482.0
44.90	428.0
46.90	624.0
47.80	257.0
49.00	1811.0
50.00	8879.0
51.00	2688.0
52.10	128.0
54.90	119.0
56.00	683.0
57.10	1173.0
60.00	400.0
61.00	2416.0
62.00	2277.0
63.00	1989.0
63.80	232.0
65.00	268.0
67.00	130.0
68.10	4918.0
69.10	5019.0
70.10	417.0
71.90	242.0
73.00	2334.0
74.10	8511.0
75.10	26320.0
76.00	2381.0
77.00	453.0
77.90	211.0
78.90	1437.0
79.90	384.0
81.00	1386.0
81.90	294.0
86.00	228.0
87.00	2480.0
88.00	2738.0
90.90	179.0
92.00	1387.0
93.00	2318.0
94.00	5936.0
95.00	53936.0
96.10	3583.0
97.00	122.0
103.90	247.0
105.00	120.0
105.90	180.0
115.90	186.0
116.90	377.0
117.90	200.0
118.90	319.0
127.80	230.0
129.80	172.0
134.70	123.0
136.90	123.0
140.90	543.0
142.90	515.0
145.70	126.0
147.70	133.0
154.90	109.0
158.80	101.0
172.00	263.0
174.00	45080.0
175.00	3106.0
176.00	42616.0
177.00	2939.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356

m/z	Abundance
36.10	396.0
37.00	2203.0
38.00	1793.0
39.00	782.0
40.10	267.0
43.90	509.0
44.90	432.0
46.90	665.0
47.90	320.0
49.00	1835.0
50.00	9704.0
51.00	2883.0
52.10	139.0
56.00	805.0
57.00	1323.0
60.00	419.0
61.00	2493.0
62.00	2362.0
63.00	2052.0
63.80	257.0
65.10	288.0
66.90	150.0
68.10	5162.0
69.10	5250.0
70.00	406.0
72.00	269.0
73.00	2498.0
74.10	9099.0
75.10	27568.0
76.00	2485.0
77.00	425.0
78.00	223.0
78.90	1494.0
79.90	361.0
81.00	1483.0
81.90	311.0
86.00	176.0
87.00	2575.0
88.00	2722.0
91.00	190.0
92.00	1456.0
93.00	2463.0
94.00	6468.0
95.00	57632.0
96.10	3869.0
97.00	122.0
103.90	251.0
105.00	101.0
105.90	191.0
111.80	101.0
115.80	184.0
116.90	388.0
117.90	222.0
118.80	345.0
127.80	231.0
128.90	105.0
129.80	227.0
134.80	147.0
136.90	161.0
140.90	635.0
142.90	559.0
145.80	111.0
147.80	153.0
155.00	144.0
172.00	298.0
174.00	49488.0
175.00	3459.0
176.00	47376.0
177.00	3063.0
177.90	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356

m/z	Abundance
36.00	391.0
37.00	2100.0
38.00	1712.0
39.00	754.0
39.90	280.0
43.90	535.0
44.90	390.0
46.90	642.0
47.90	332.0
49.00	1702.0
50.00	9271.0
51.00	2815.0
52.00	163.0
56.00	860.0
57.00	1391.0
60.00	444.0
61.00	2377.0
62.00	2176.0
63.00	1932.0
63.90	255.0
65.10	284.0
66.90	170.0
68.10	4912.0
69.00	5104.0
70.00	395.0
72.00	261.0
73.00	2428.0
74.10	8602.0
75.00	26008.0
76.00	2342.0
77.10	386.0
78.00	242.0
78.90	1447.0
80.00	310.0
81.00	1524.0
81.90	294.0
87.00	2430.0
88.00	2511.0
91.10	165.0
92.10	1377.0
93.00	2437.0
94.00	6320.0
95.00	55232.0
96.10	3697.0
97.00	102.0
104.00	236.0
105.90	206.0
115.80	184.0
116.90	327.0
117.90	223.0
118.80	337.0
127.80	235.0
128.90	123.0
129.80	258.0
134.80	142.0
136.90	130.0
140.90	614.0
142.90	554.0
147.90	171.0
155.00	169.0
172.00	332.0
174.00	48912.0
175.00	3433.0
176.00	47264.0
177.00	2932.0
177.90	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB356