

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033332.D
 Acq On : 14 Dec 2023 14:03
 Operator : SY/MD
 Sample : 05773-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 15 01:04:56 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	237128	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	241841	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	131429	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	59648	42.078	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	84.160%		
7) Chloroethane-d5	1.532	69	47725	48.319	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.640%		
11) 1,1-Dichloroethene-d2	2.060	65	25248	46.819	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	93.640%		
21) 2-Butanone-d5	3.783	46	55770	79.211	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	79.210%		
24) Chloroform-d	4.249	84	151571	50.384	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.760%		
26) 1,2-Dichloroethane-d4	4.941	65	98625	52.731	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	105.460%		
32) Benzene-d6	4.960	84	279312	49.382	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.760%		
36) 1,2-Dichloropropane-d6	5.989	67	71079	46.738	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.480%		
41) Toluene-d8	7.243	98	264910	49.097	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.200%		
43) trans-1,3-Dichloroprop...	7.555	79	44216	45.978	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.960%		
47) 2-Hexanone-d5	8.024	63	52359	85.700	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.700%		
56) 1,1,2,2-Tetrachloroeth...	10.153	84	108637	50.251	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	100.500%		
66) 1,2-Dichlorobenzene-d4	11.561	152	131730	56.333	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	112.660%		
Target Compounds						Qvalue
15) Methyl Acetate	2.114	43	1815	1.620	ug/L	# 47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033332.D
Acq On : 14 Dec 2023 14:03
Operator : SY/MD
Sample : 05773-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Dec 15 01:04:56 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration

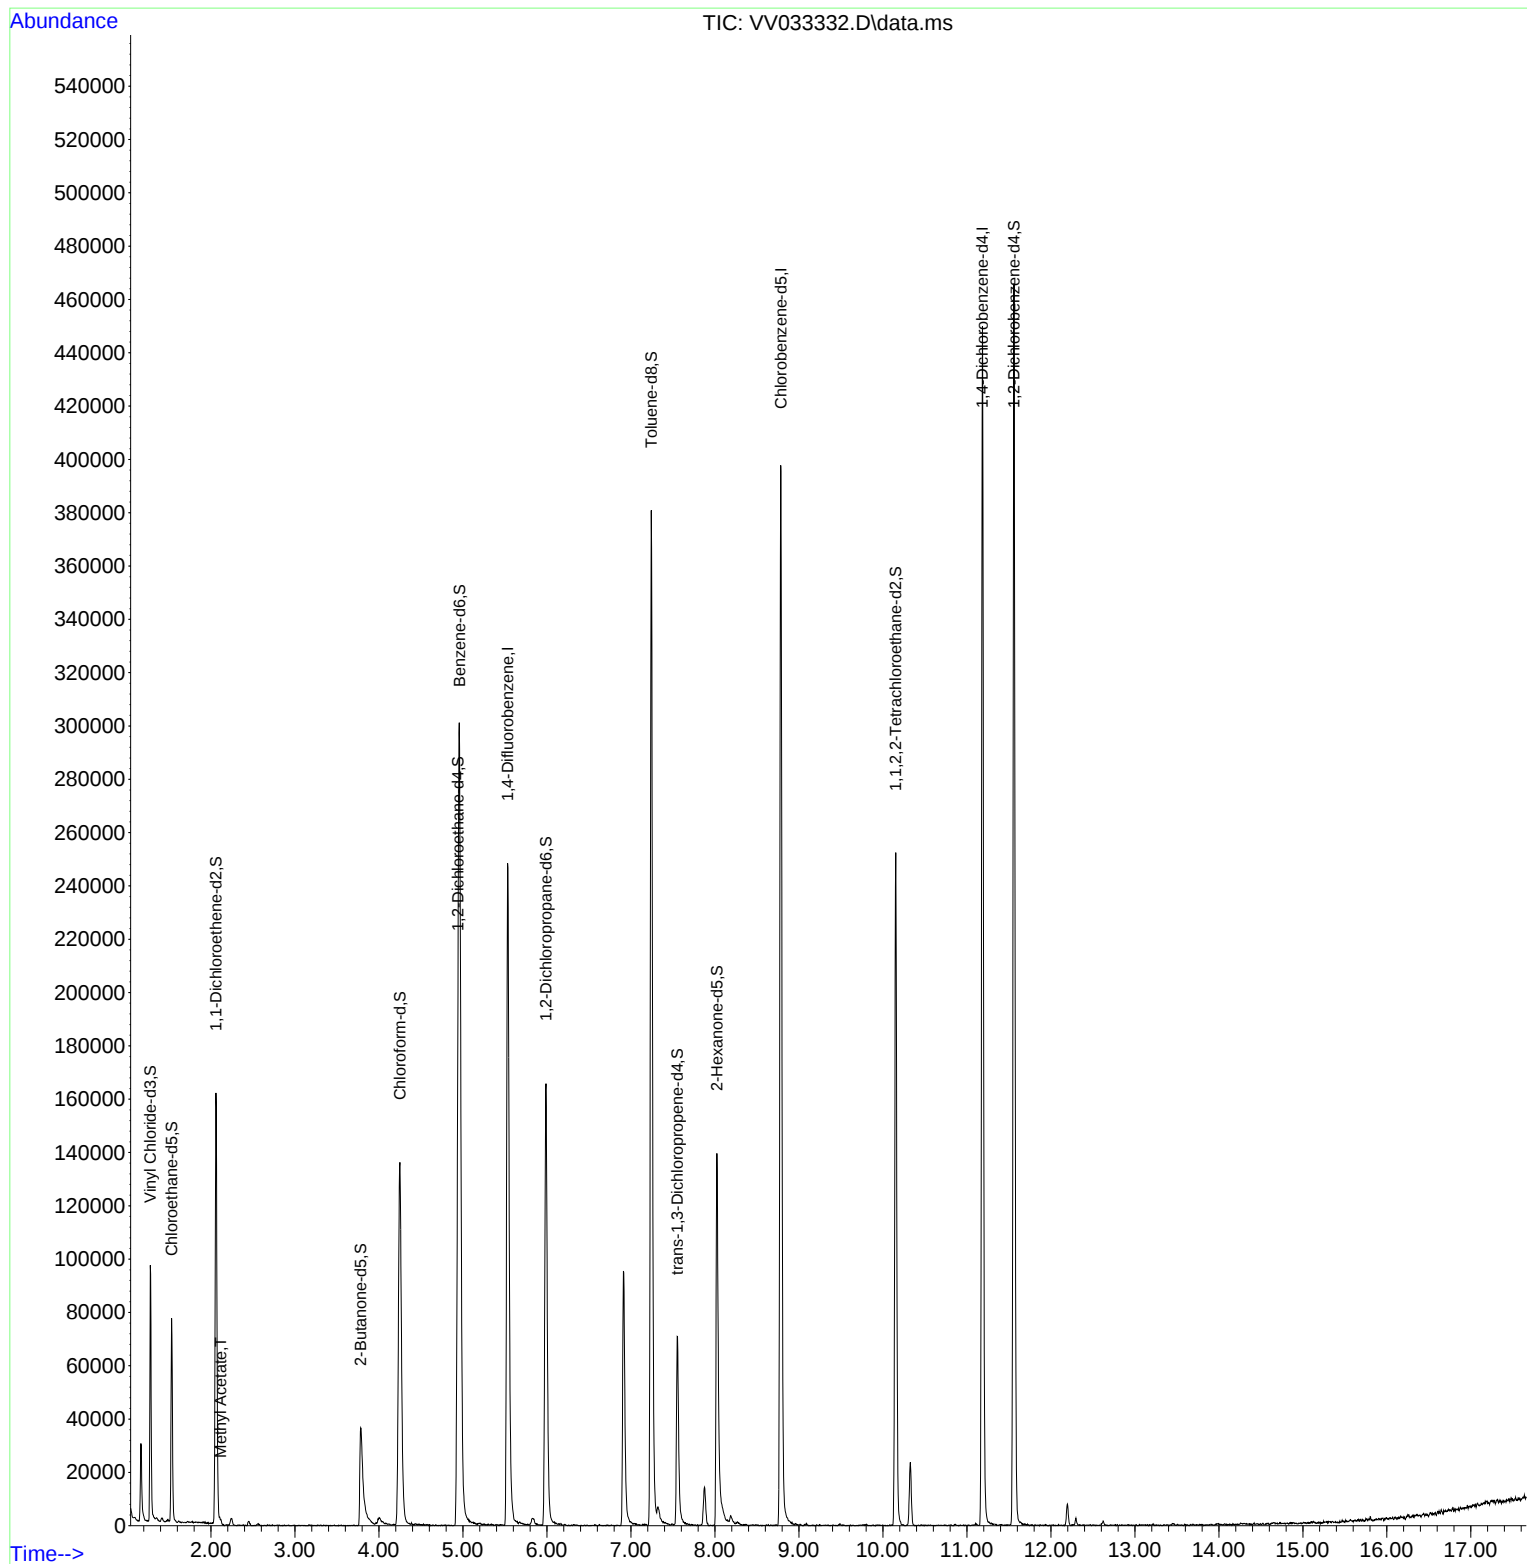

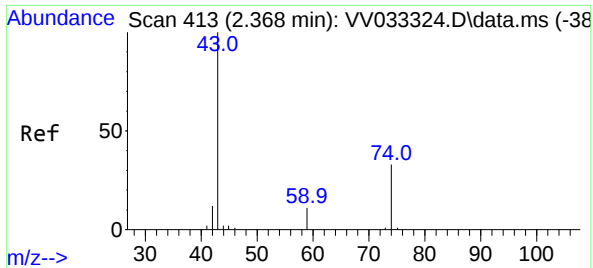

#15
Methyl Acetate
Concen: 1.620 ug/L
RT: 2.114 min Scan# 31
Delta R.T. -0.254 min
Lab File: VV033332.D
Acq: 14 Dec 2023 14:03

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 43 Resp: 1815
Ion Ratio Lower Upper
43 100
74 0.0 22.6 33.8#

