

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033334.D
 Acq On : 14 Dec 2023 14:50
 Operator : SY/MD
 Sample : 05799-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 15 01:05:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	237689	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	241233	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	133870	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	60176	42.351	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.700%
7) Chloroethane-d5	1.532	69	45900	46.362	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.720%
11) 1,1-Dichloroethene-d2	2.063	65	25201	46.621	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.240%
21) 2-Butanone-d5	3.783	46	55722	78.956	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	78.960%
24) Chloroform-d	4.249	84	149911	49.715	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.420%
26) 1,2-Dichloroethane-d4	4.940	65	100977	53.861	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.720%
32) Benzene-d6	4.960	84	281714	49.933	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.860%
36) 1,2-Dichloropropane-d6	5.989	67	70511	46.481	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	92.960%
41) Toluene-d8	7.243	98	272713	50.671	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.340%
43) trans-1,3-Dichloroprop...	7.551	79	43274	45.112	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.220%
47) 2-Hexanone-d5	8.024	63	51801	85.001	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.000%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	110113	51.063	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	102.120%
66) 1,2-Dichlorobenzene-d4	11.561	152	132969	55.826	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	111.660%
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.185	75	11583	6.939	ug/L	# 63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033334.D
Acq On : 14 Dec 2023 14:50
Operator : SY/MD
Sample : 05799-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Dec 15 01:05:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration

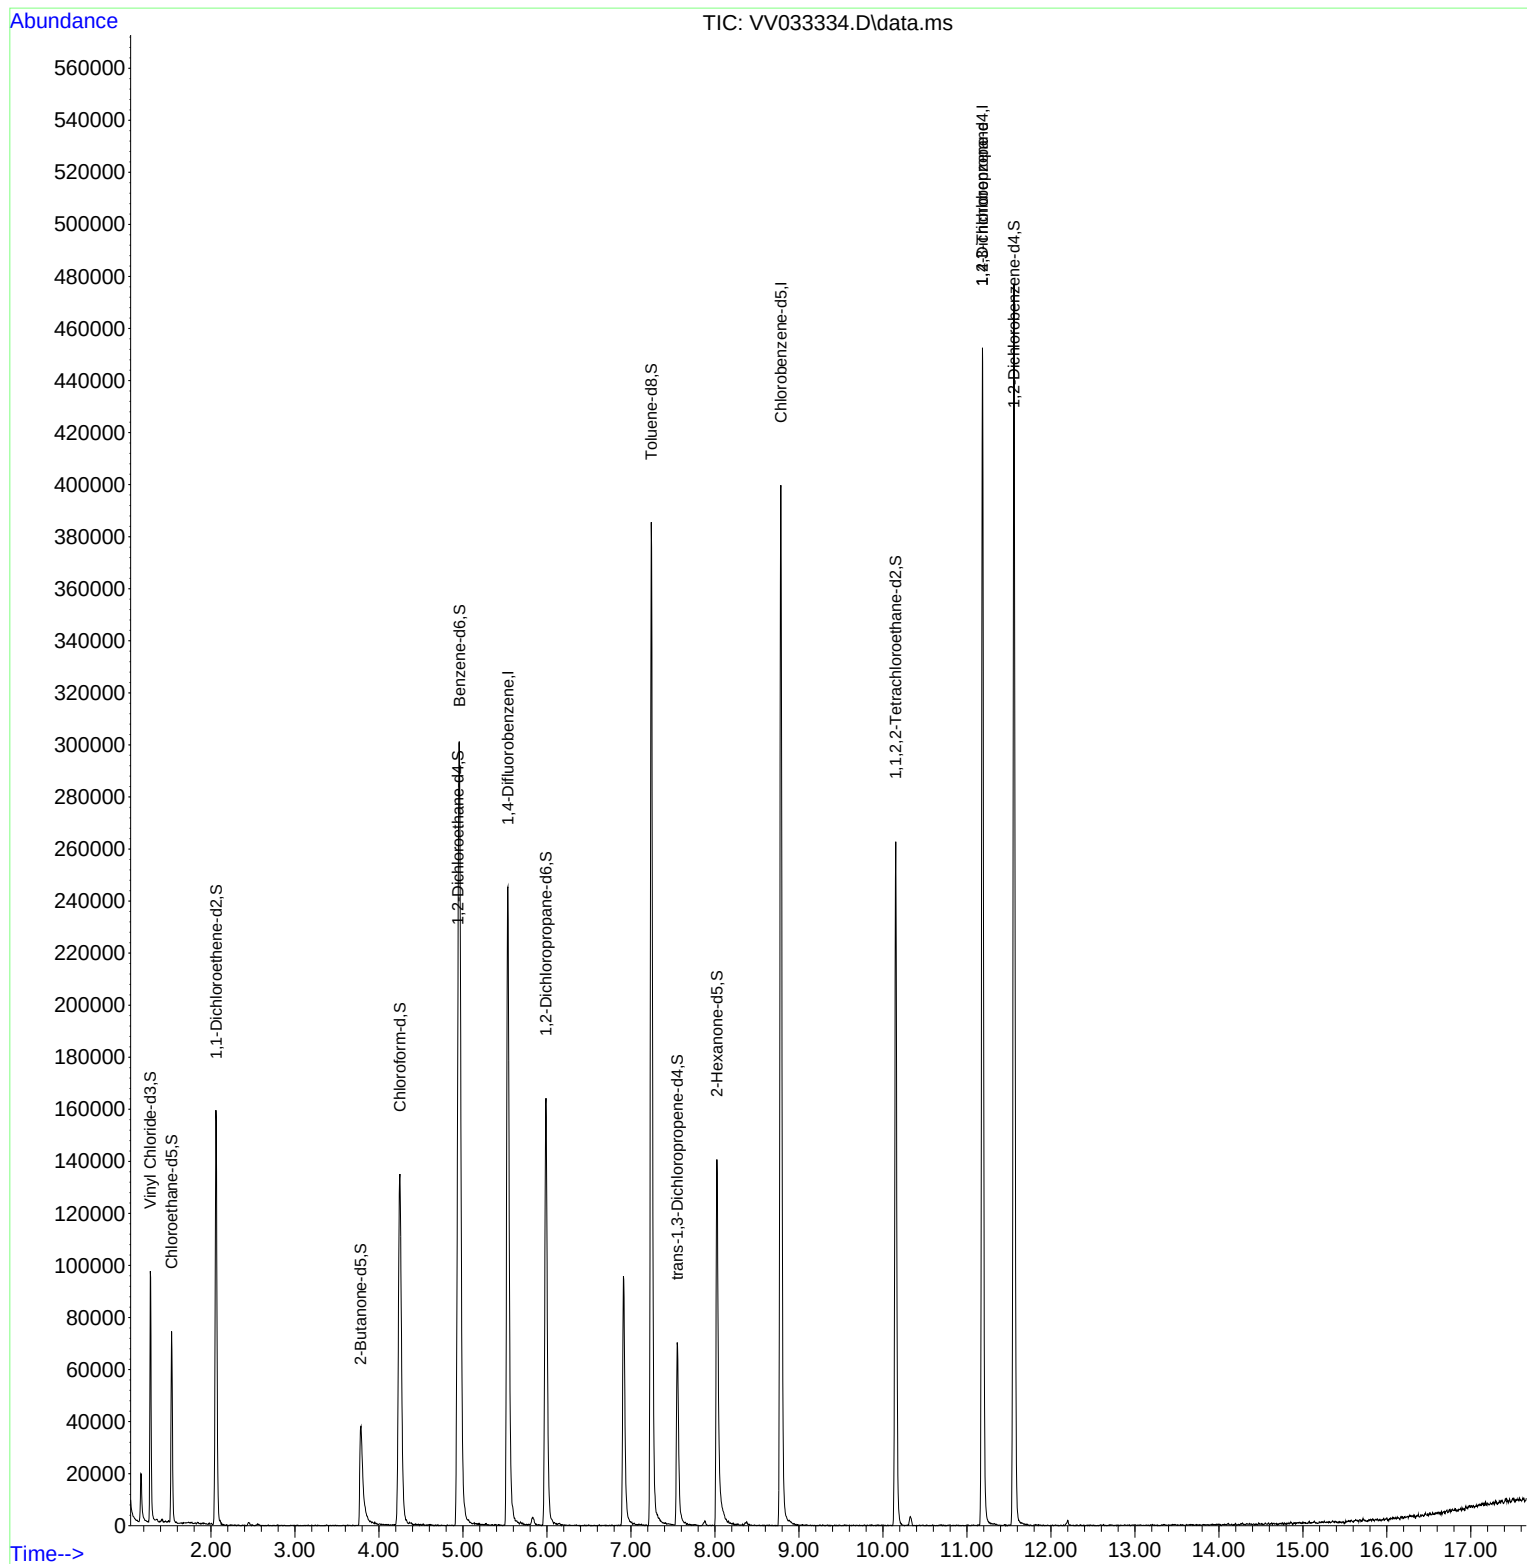

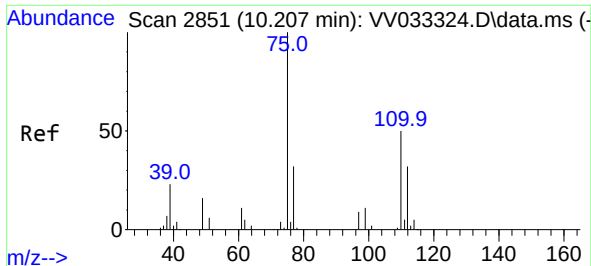

#61

1,2,3-Trichloropropane

Concen: 6.939 ug/L

RT: 11.185 min Scan# 31

Delta R.T. 0.977 min


Lab File: VV033334.D

Acq: 14 Dec 2023 14:50

Instrument :

MSVOA_V

ClientSampleId :

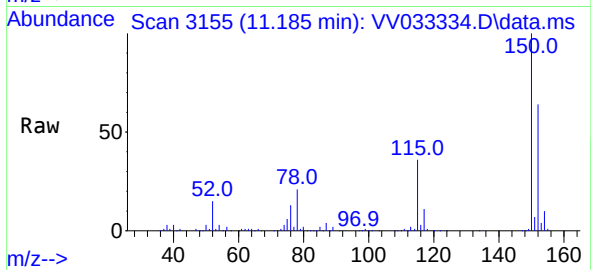

Tgt Ion: 75 Resp: 11583

Ion Ratio Lower Upper

75 100

77 33.7 27.0 40.6

110 4.9 38.1 57.1#

