

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033343.D
 Acq On : 14 Dec 2023 18:18
 Operator : SY/MD
 Sample : 05794-10
 Misc : 4.80g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 15 01:06:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	240079	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	241897	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	136101	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	61355	42.750	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 85.500%			
7) Chloroethane-d5	1.532	69	50409	50.409	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 100.820%			
11) 1,1-Dichloroethene-d2	2.060	65	27919	51.135	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 102.280%			
21) 2-Butanone-d5	3.780	46	64085	89.902	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 89.900%			
24) Chloroform-d	4.246	84	166239	54.581	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 109.160%			
26) 1,2-Dichloroethane-d4	4.941	65	109552	57.853	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 115.700%			
32) Benzene-d6	4.960	84	308792	54.582	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 109.160%			
36) 1,2-Dichloropropane-d6	5.989	67	77672	51.061	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 102.120%			
41) Toluene-d8	7.243	98	297646	55.152	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 110.300%			
43) trans-1,3-Dichloroprop...	7.551	79	46742	48.594	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 97.180%			
47) 2-Hexanone-d5	8.024	63	60023	98.222	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 98.220%			
56) 1,1,2,2-Tetrachloroeth...	10.153	84	119580	55.300	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 110.600%			
66) 1,2-Dichlorobenzene-d4	11.561	152	149155	61.595	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 123.180%#			
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.915	75	3210	1.247	ug/L	89
61) 1,2,3-Trichloropropane	11.185	75	10849	6.393	ug/L #	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033343.D
Acq On : 14 Dec 2023 18:18
Operator : SY/MD
Sample : 05794-10
Misc : 4.80g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Dec 15 01:06:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration




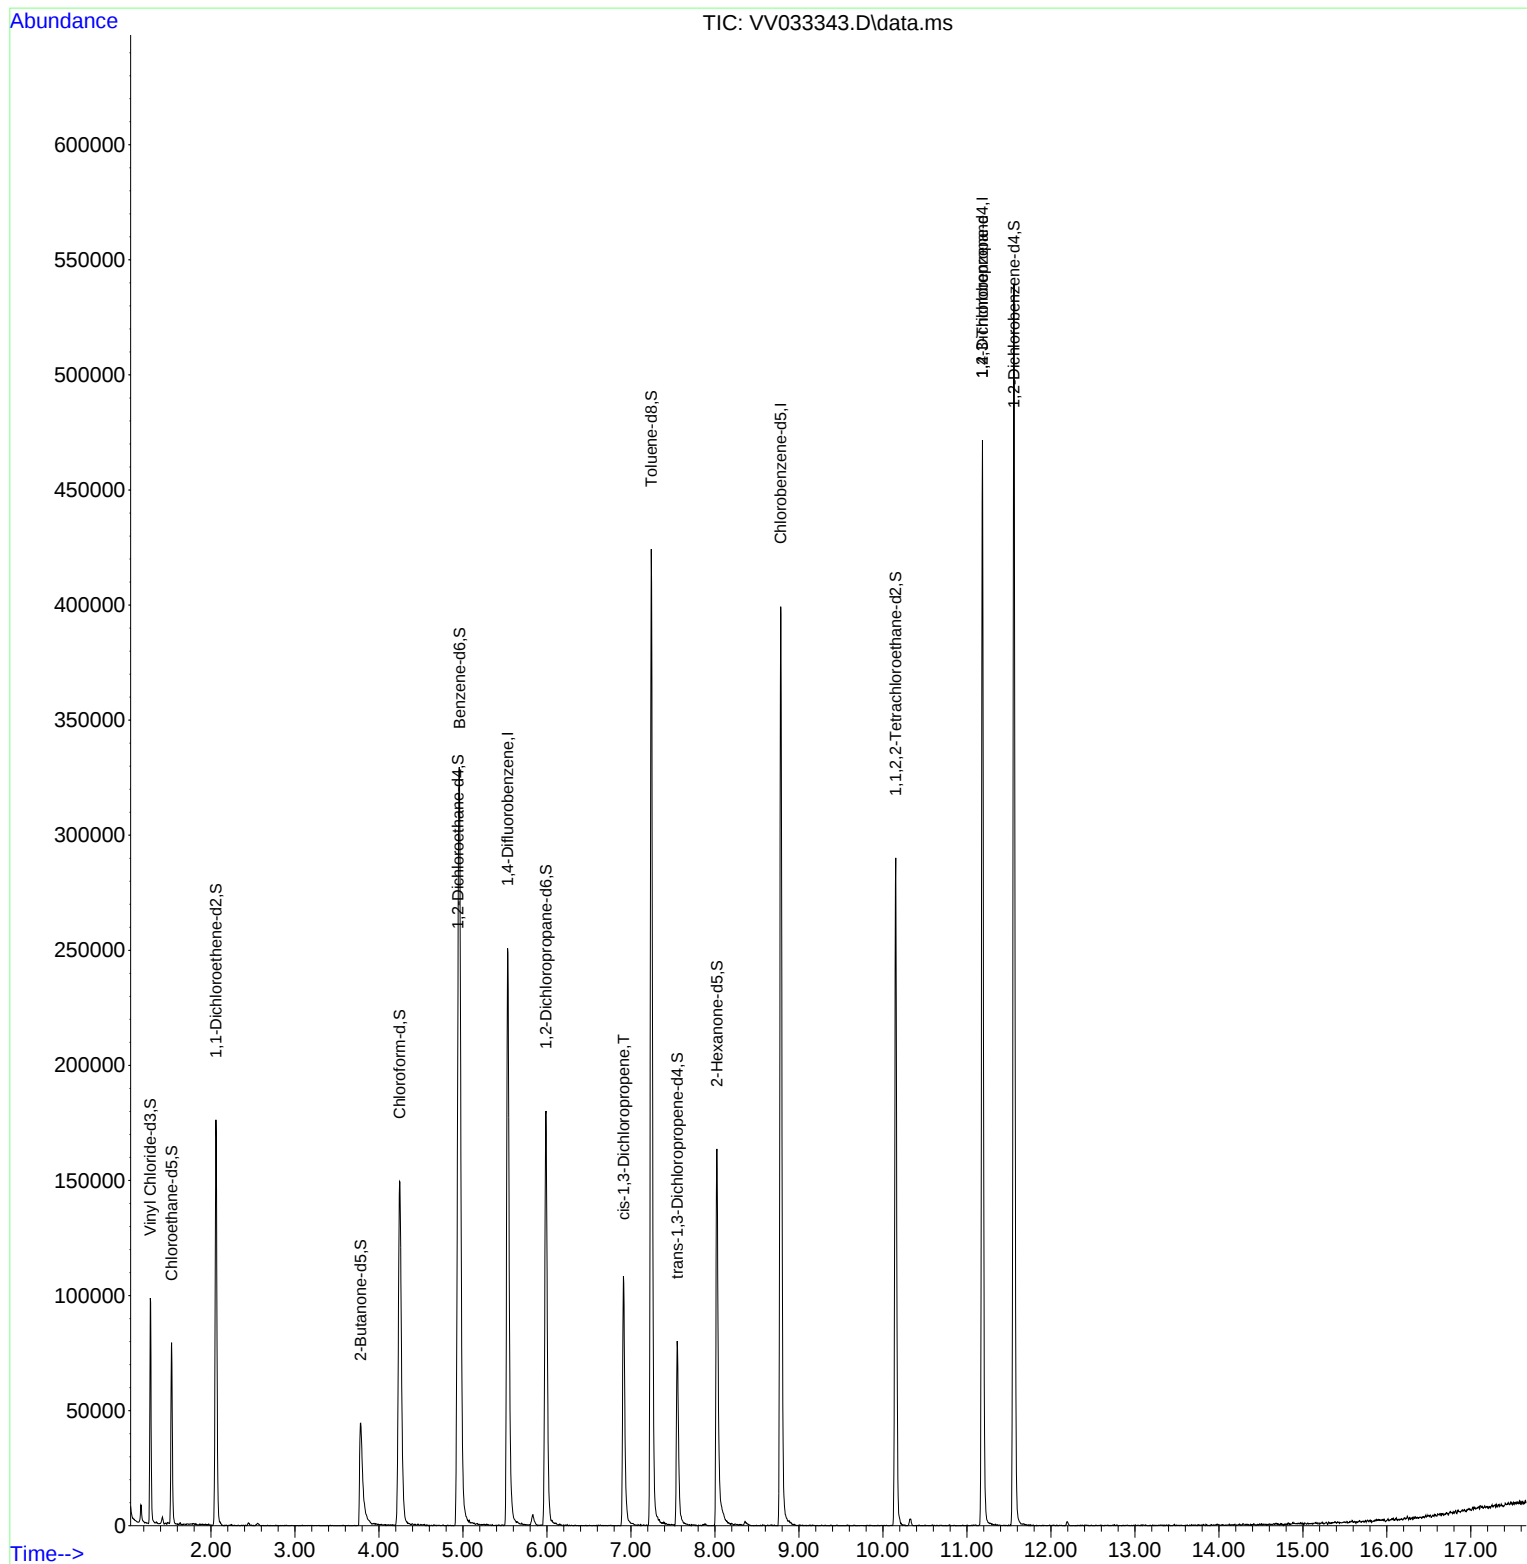


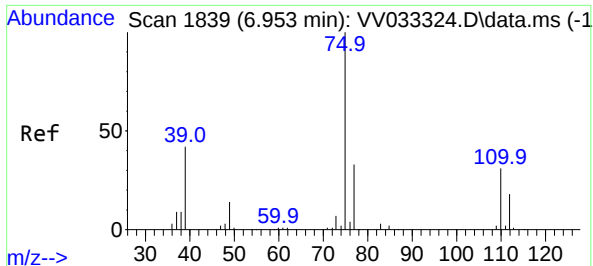

#39
cis-1,3-Dichloropropene
Concen: 1.247 ug/L
RT: 6.915 min Scan# 11
Delta R.T. -0.035 min
Lab File: VV033343.D
Acq: 14 Dec 2023 18:18

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 3210
Ion Ratio Lower Upper
75 100
77 37.9 22.4 41.6

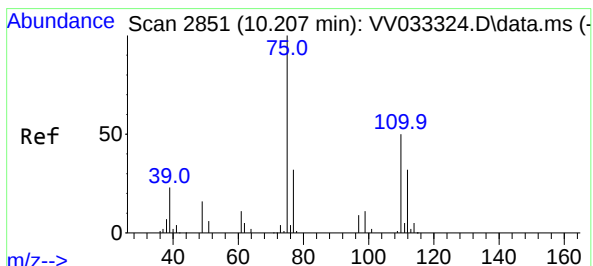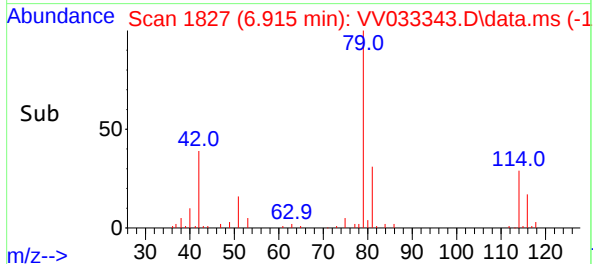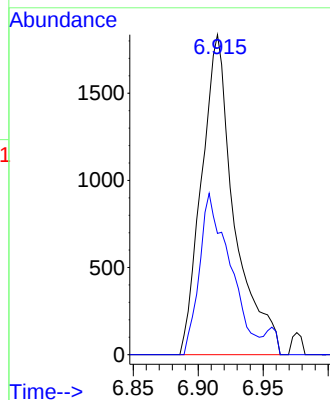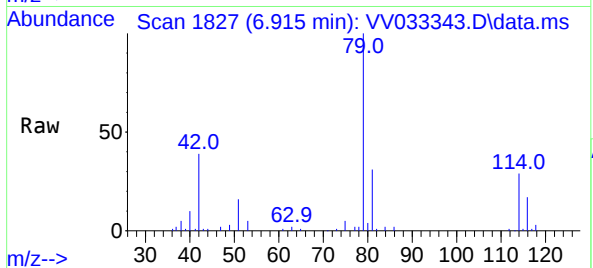

#61
1,2,3-Trichloropropane
Concen: 6.393 ug/L
RT: 11.185 min Scan# 3155
Delta R.T. 0.978 min
Lab File: VV033343.D
Acq: 14 Dec 2023 18:18

Tgt Ion: 75 Resp: 10849
Ion Ratio Lower Upper
75 100
77 37.3 27.0 40.6
110 4.0 38.1 57.1#

