

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033347.D
 Acq On : 14 Dec 2023 19:50
 Operator : SY/MD
 Sample : 05794-14
 Misc : 5.12g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 15 01:07:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	219207	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	224544	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	127398	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	51066	38.969	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	77.940%
7) Chloroethane-d5	1.532	69	42036	46.039	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.080%
11) 1,1-Dichloroethene-d2	2.060	65	23842	47.826	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.660%
21) 2-Butanone-d5	3.789	46	52126	80.088	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	80.090%
24) Chloroform-d	4.249	84	138339	49.745	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.500%
26) 1,2-Dichloroethane-d4	4.941	65	93504	54.080	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.160%
32) Benzene-d6	4.960	84	259851	49.481	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.960%
36) 1,2-Dichloropropane-d6	5.989	67	60905	43.133	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.260%
41) Toluene-d8	7.243	98	251193	50.141	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.280%
43) trans-1,3-Dichloroprop...	7.551	79	40032	44.834	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.660%
47) 2-Hexanone-d5	8.024	63	51210	90.276	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.280%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	99968	49.804	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.600%
66) 1,2-Dichlorobenzene-d4	11.561	152	128211	56.563	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.120%
Target Compounds						
44) trans-1,3-Dichloropropene	7.551	75	1841	0.762	ug/L #	78
61) 1,2,3-Trichloropropane	11.185	75	10313	6.492	ug/L #	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033347.D
Acq On : 14 Dec 2023 19:50
Operator : SY/MD
Sample : 05794-14
Misc : 5.12g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Dec 15 01:07:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration




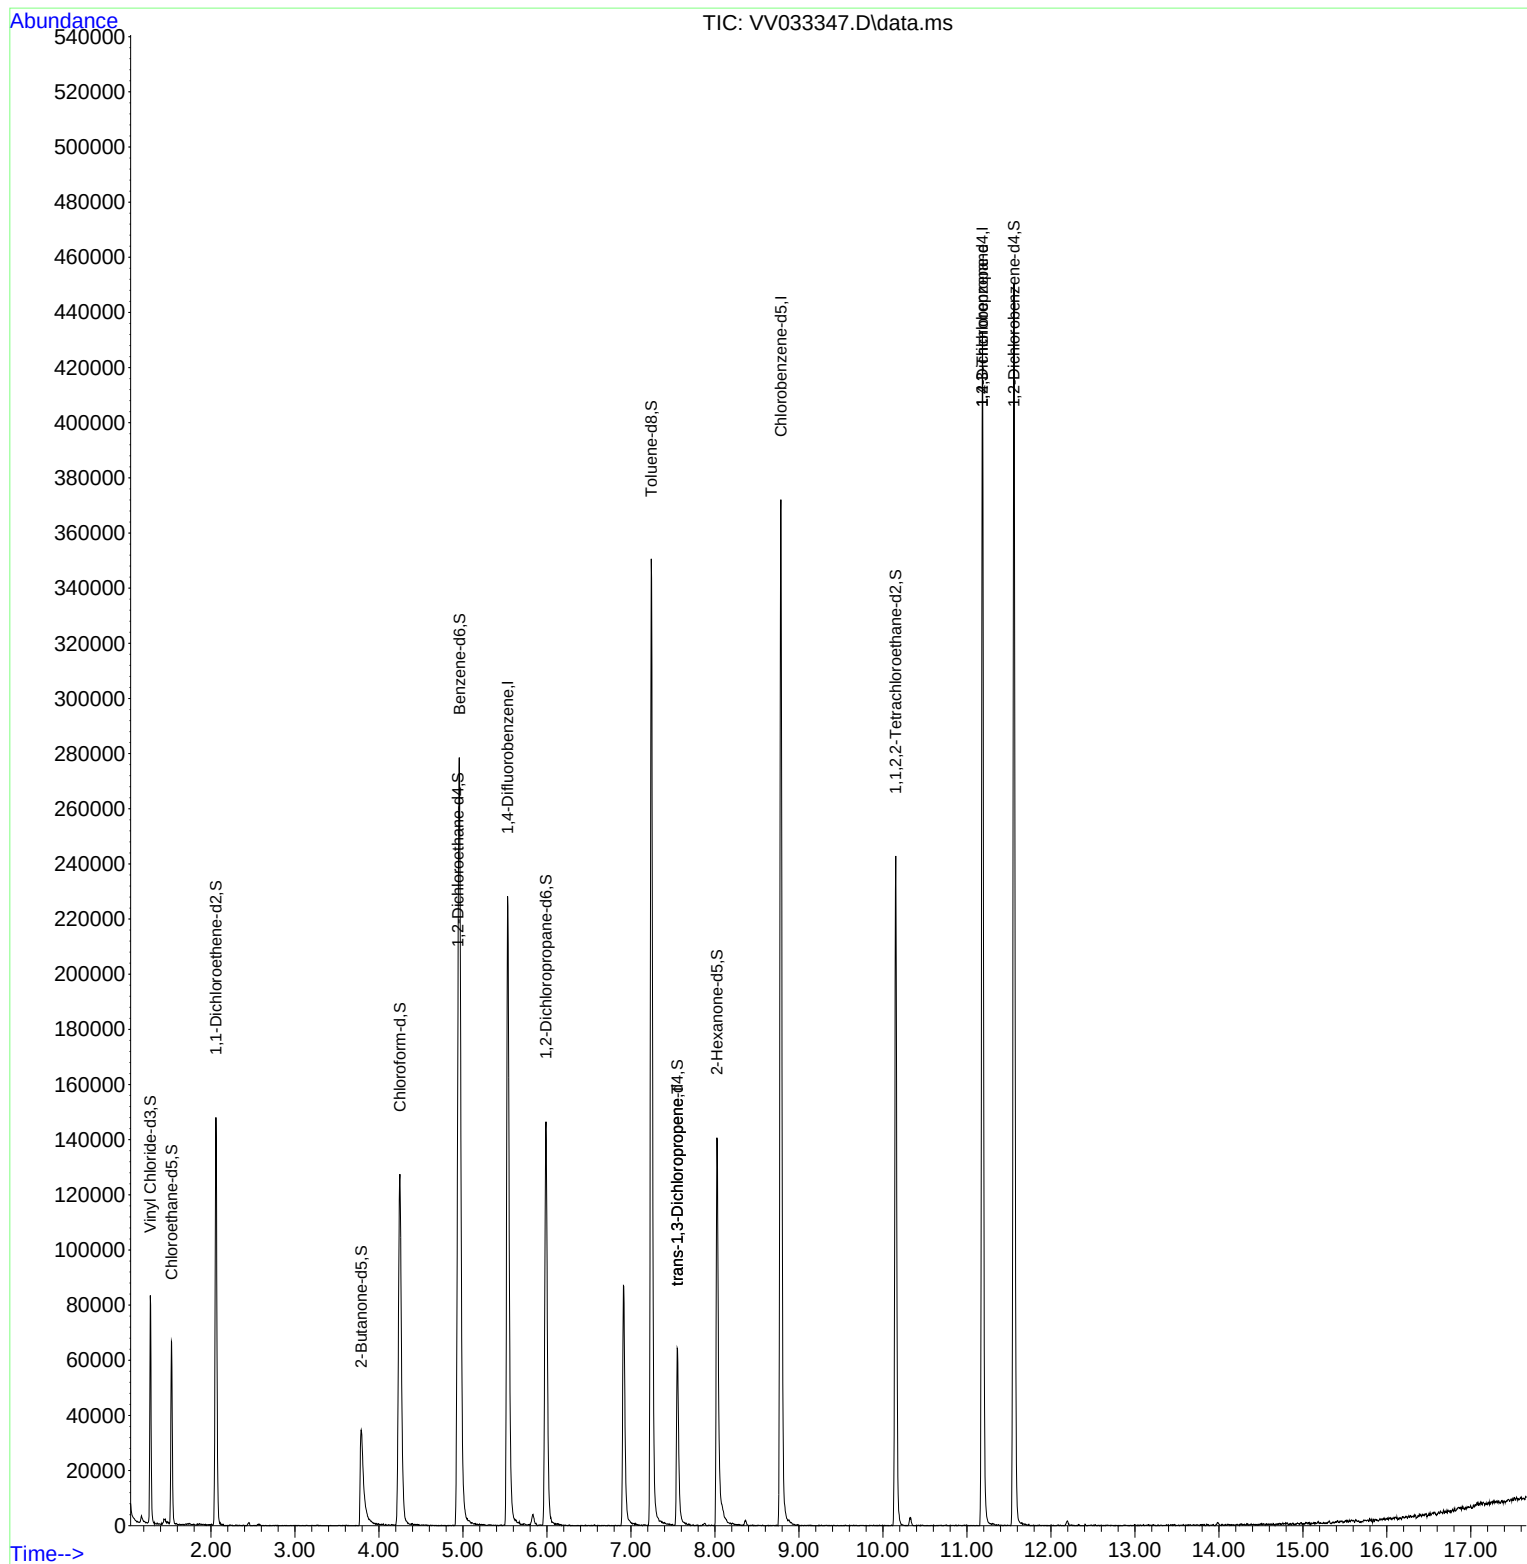


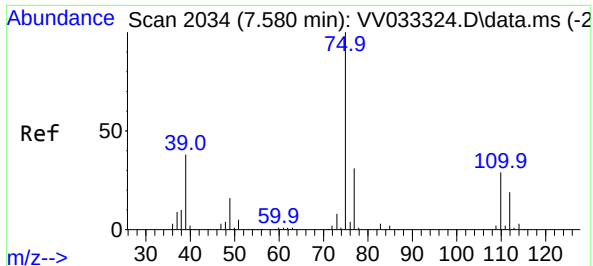

#44
trans-1,3-Dichloropropene
Concen: 0.762 ug/L
RT: 7.551 min Scan# 2034
Delta R.T. -0.029 min
Lab File: VV033347.D
Acq: 14 Dec 2023 19:50

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 1841
Ion Ratio Lower Upper
75 100
77 43.6 22.0 41.0#

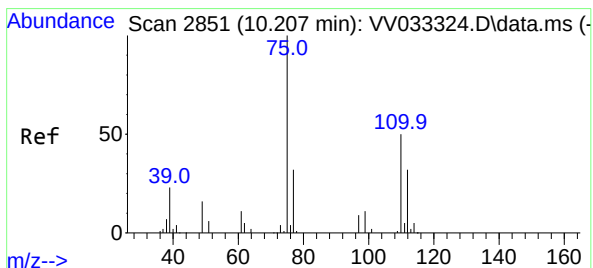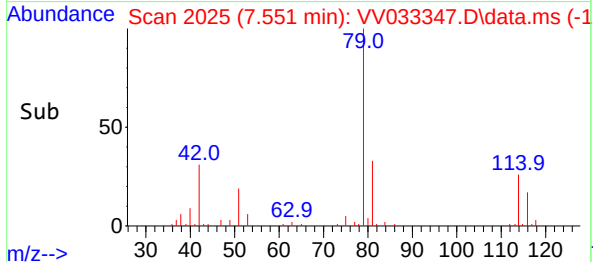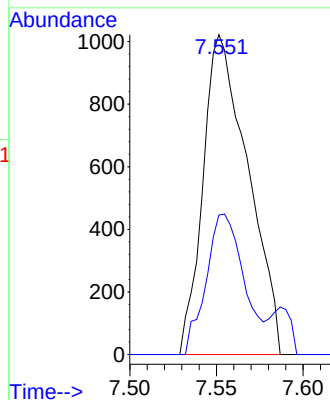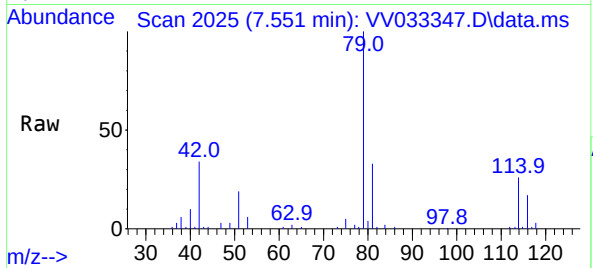

#61
1,2,3-Trichloropropane
Concen: 6.492 ug/L
RT: 11.185 min Scan# 3155
Delta R.T. 0.978 min
Lab File: VV033347.D
Acq: 14 Dec 2023 19:50

Tgt Ion: 75 Resp: 10313
Ion Ratio Lower Upper
75 100
77 33.9 27.0 40.6
110 1.5 38.1 57.1#

