

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033341.D
 Acq On : 14 Dec 2023 17:32
 Operator : SY/MD
 Sample : 05794-08
 Misc : 4.42g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3Q2

Quant Time: Dec 15 01:06:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	197597	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	200946	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	112267	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	64406	54.524	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 109.040%			
7) Chloroethane-d5	1.532	69	51428	62.485	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 124.980%			
11) 1,1-Dichloroethene-d2	2.060	65	27227	60.589	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 121.180%			
21) 2-Butanone-d5	3.780	46	67645	115.298	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 115.300%			
24) Chloroform-d	4.249	84	172168	68.680	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 137.360%#			
26) 1,2-Dichloroethane-d4	4.941	65	112533	72.203	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 144.400%#			
32) Benzene-d6	4.960	84	318301	67.728	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 135.460%#			
36) 1,2-Dichloropropane-d6	5.986	67	81312	64.348	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 128.700%#			
41) Toluene-d8	7.243	98	307397	68.566	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 137.140%#			
43) trans-1,3-Dichloroprop...	7.551	79	49568	62.034	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 124.060%			
47) 2-Hexanone-d5	8.021	63	61911	121.958	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 121.960%			
56) 1,1,2,2-Tetrachloroeth...	10.153	84	120786	67.242	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 134.480%#			
66) 1,2-Dichlorobenzene-d4	11.561	152	155699	77.947	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 155.900%#			
Target Compounds					Qvalue	
12) 1,1-Dichloroethene	2.056	96	895	0.903	ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033341.D
Acq On : 14 Dec 2023 17:32
Operator : SY/MD
Sample : 05794-08
Misc : 4.42g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3Q2

Quant Time: Dec 15 01:06:20 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration

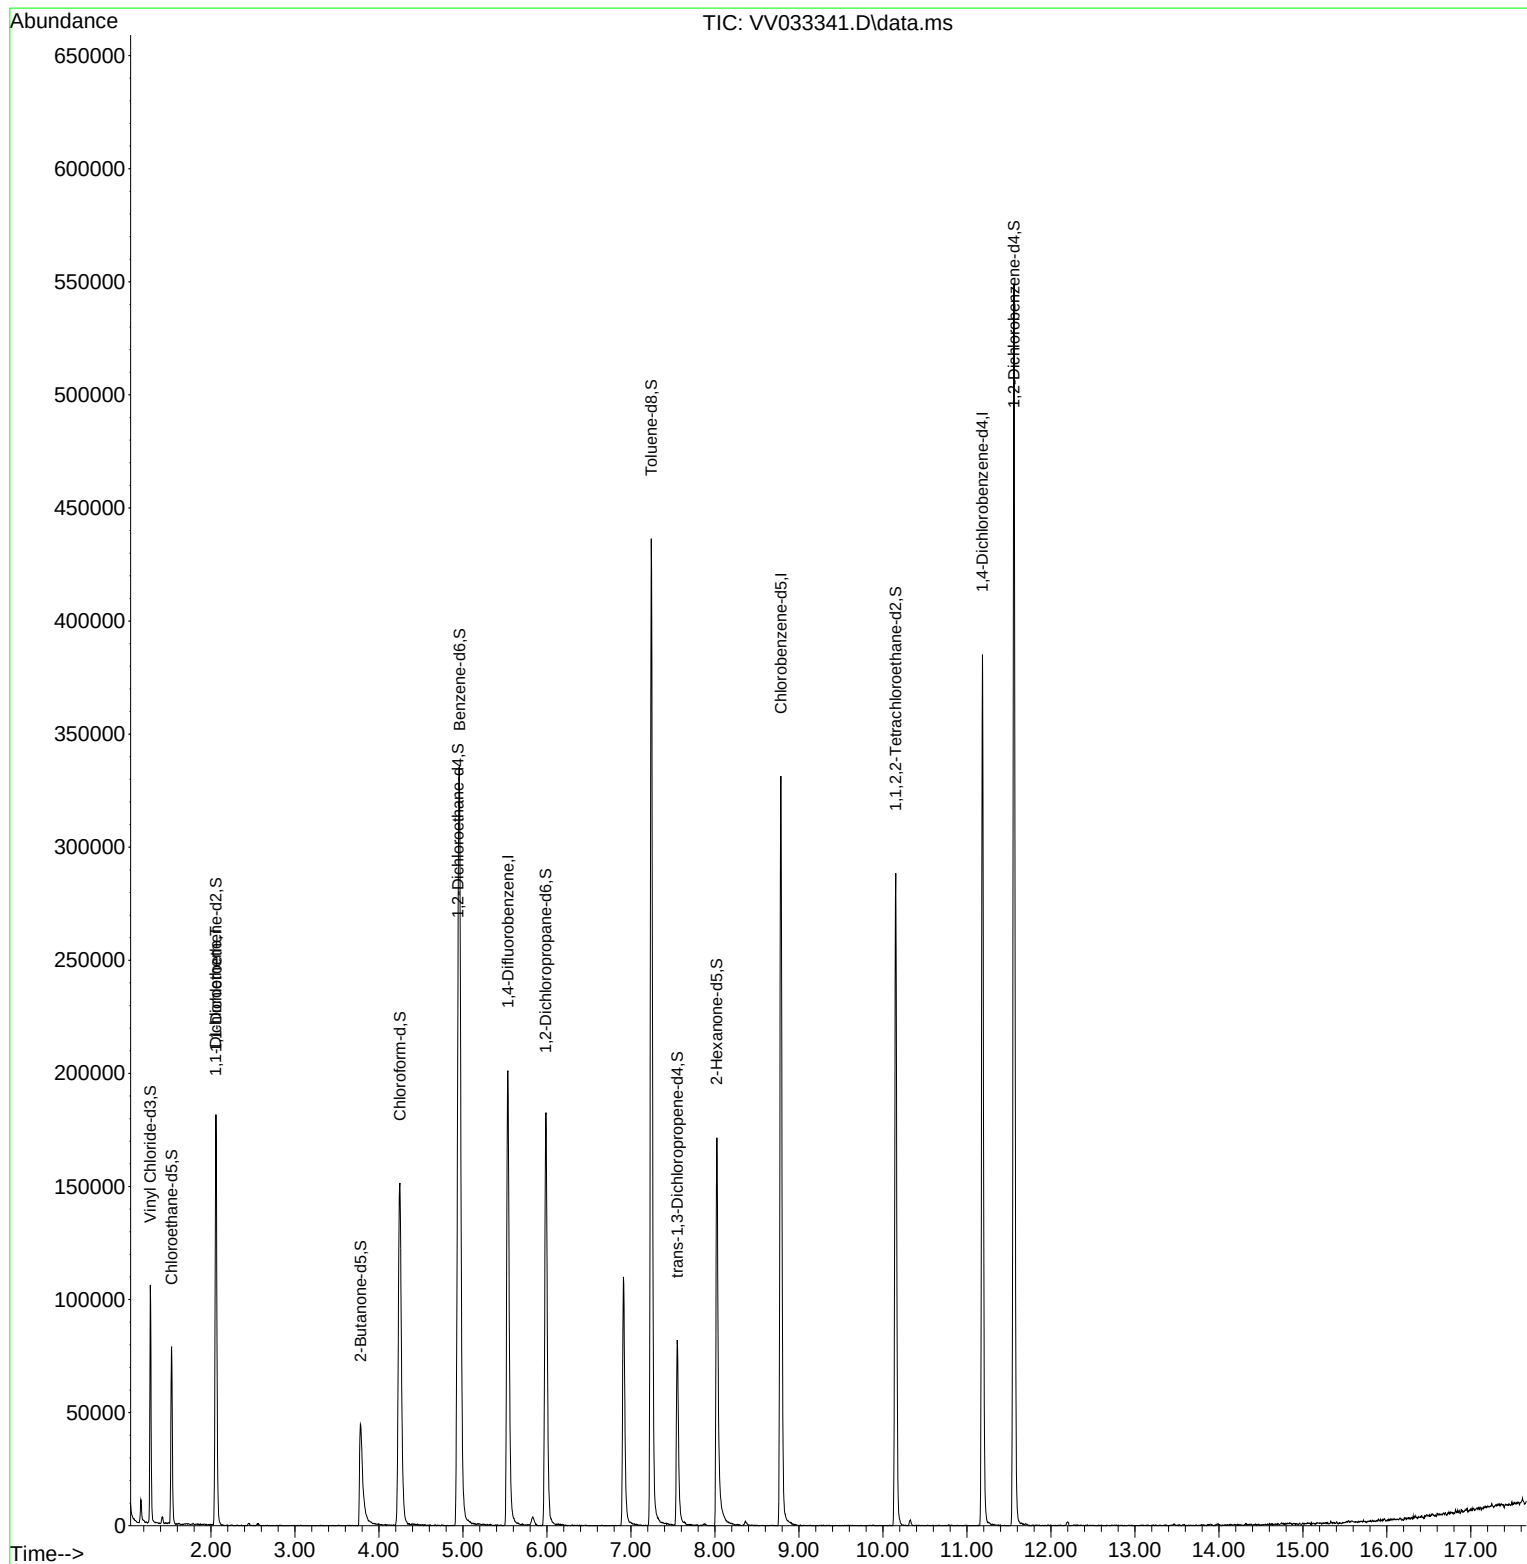

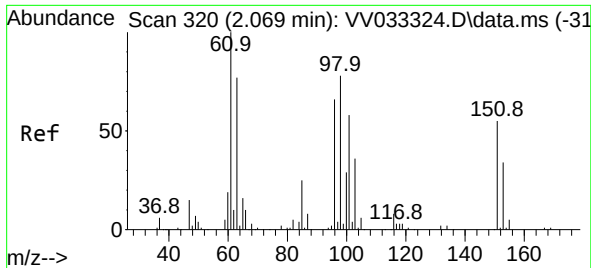

#12
 1,1-Dichloroethene
 Concen: 0.903 ug/L
 RT: 2.056 min Scan# 31
 Delta R.T. -0.013 min
 Lab File: VV033341.D
 Acq: 14 Dec 2023 17:32

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3Q2

Tgt Ion: 96 Resp: 895
 Ion Ratio Lower Upper
 96 100
 61 1462.4 109.1 202.7#
 63 10021.3 85.3 158.3#

