

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033353.D
 Acq On : 14 Dec 2023 22:33
 Operator : SY/MD
 Sample : 05807-10 100X
 Misc : 3.24g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ2

Quant Time: Dec 15 04:09:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	217867	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	219308	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	124268	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	48624	37.334	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.660%
7) Chloroethane-d5	1.532	69	39519	43.548	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	87.100%
11) 1,1-Dichloroethene-d2	2.060	65	21408	43.208	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.420%
21) 2-Butanone-d5	3.786	46	52109	80.554	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	80.550%
24) Chloroform-d	4.249	84	129958	47.019	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.040%
26) 1,2-Dichloroethane-d4	4.941	65	88733	51.636	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.280%
32) Benzene-d6	4.960	84	241615	47.107	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.220%
36) 1,2-Dichloropropane-d6	5.989	67	60086	43.569	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	87.140%
41) Toluene-d8	7.243	98	230652	47.140	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.280%
43) trans-1,3-Dichloroprop...	7.551	79	38310	43.930	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.860%
47) 2-Hexanone-d5	8.024	63	51195	92.405	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.400%
56) 1,1,2,2-Tetrachloroeth...	10.153	84	97682	49.827	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	99.660%
66) 1,2-Dichlorobenzene-d4	11.561	152	122278	55.304	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	110.600%
Target Compounds						
					Qvalue	
51) Chlorobenzene	8.821	112	2515	0.571	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033353.D
Acq On : 14 Dec 2023 22:33
Operator : SY/MD
Sample : 05807-10 100X
Misc : 3.24g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ2

Quant Time: Dec 15 04:09:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration

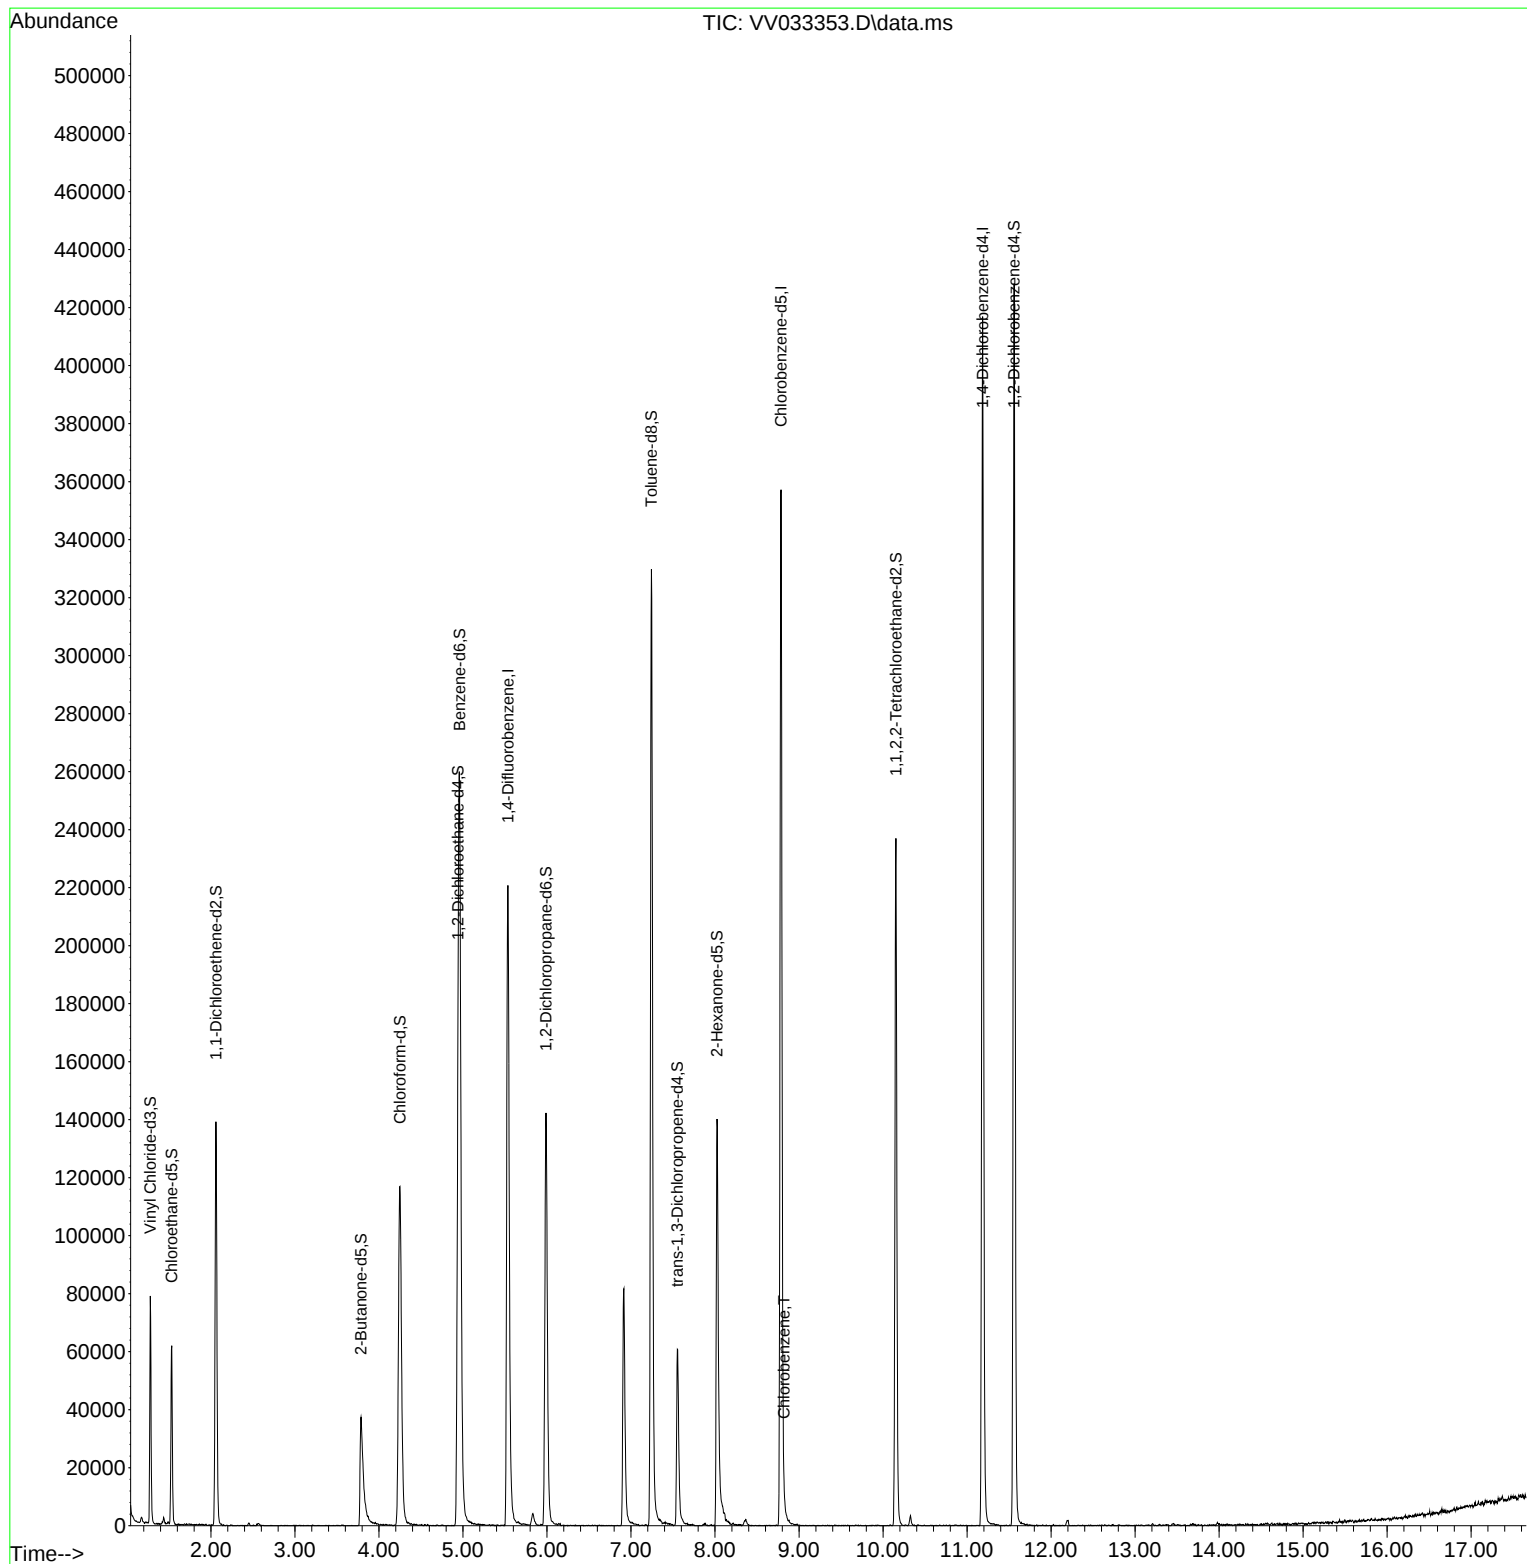

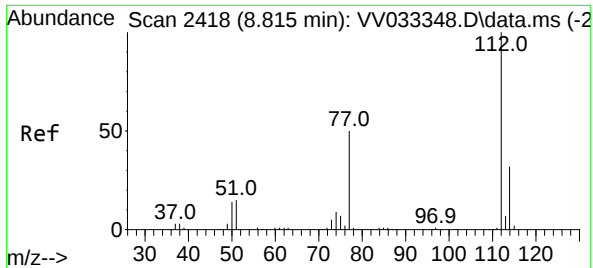

#51
 Chlorobenzene
 Concen: 0.571 ug/L
 RT: 8.821 min Scan# 24
 Delta R.T. 0.010 min
 Lab File: VV033353.D
 Acq: 14 Dec 2023 22:33

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ2

Tgt Ion:	112	Resp:	2515
Ion	Ratio	Lower	Upper
112	100		
114	30.5	22.9	42.5
77	54.9	42.6	64.0

