

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033362.D
 Acq On : 15 Dec 2023 02:01
 Operator : SY/MD
 Sample : 05802-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B03

Quant Time: Dec 15 04:10:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	204442	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	208433	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	116263	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	42994	35.179	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	70.360%	
7) Chloroethane-d5	1.532	69	32073	37.664	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	75.320%	
11) 1,1-Dichloroethene-d2	2.059	65	16873	36.291	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	72.580%	
21) 2-Butanone-d5	3.783	46	43435	71.555	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	71.550%	
24) Chloroform-d	4.246	84	125109	48.237	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.480%	
26) 1,2-Dichloroethane-d4	4.940	65	85640	53.109	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	106.220%	
32) Benzene-d6	4.960	84	230481	47.280	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	94.560%	
36) 1,2-Dichloropropane-d6	5.989	67	55920	42.664	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	85.320%	
41) Toluene-d8	7.243	98	222940	47.941	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.880%	
43) trans-1,3-Dichloroprop...	7.551	79	35788	43.179	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	86.360%	
47) 2-Hexanone-d5	8.024	63	43267	82.170	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	82.170%	
56) 1,1,2,2-Tetrachloroeth...	10.152	84	87802	47.124	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	94.240%	
66) 1,2-Dichlorobenzene-d4	11.561	152	115239	55.709	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	111.420%	
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.069	96	969	0.945	ug/L	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033362.D
Acq On : 15 Dec 2023 02:01
Operator : SY/MD
Sample : 05802-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B03

Quant Time: Dec 15 04:10:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration

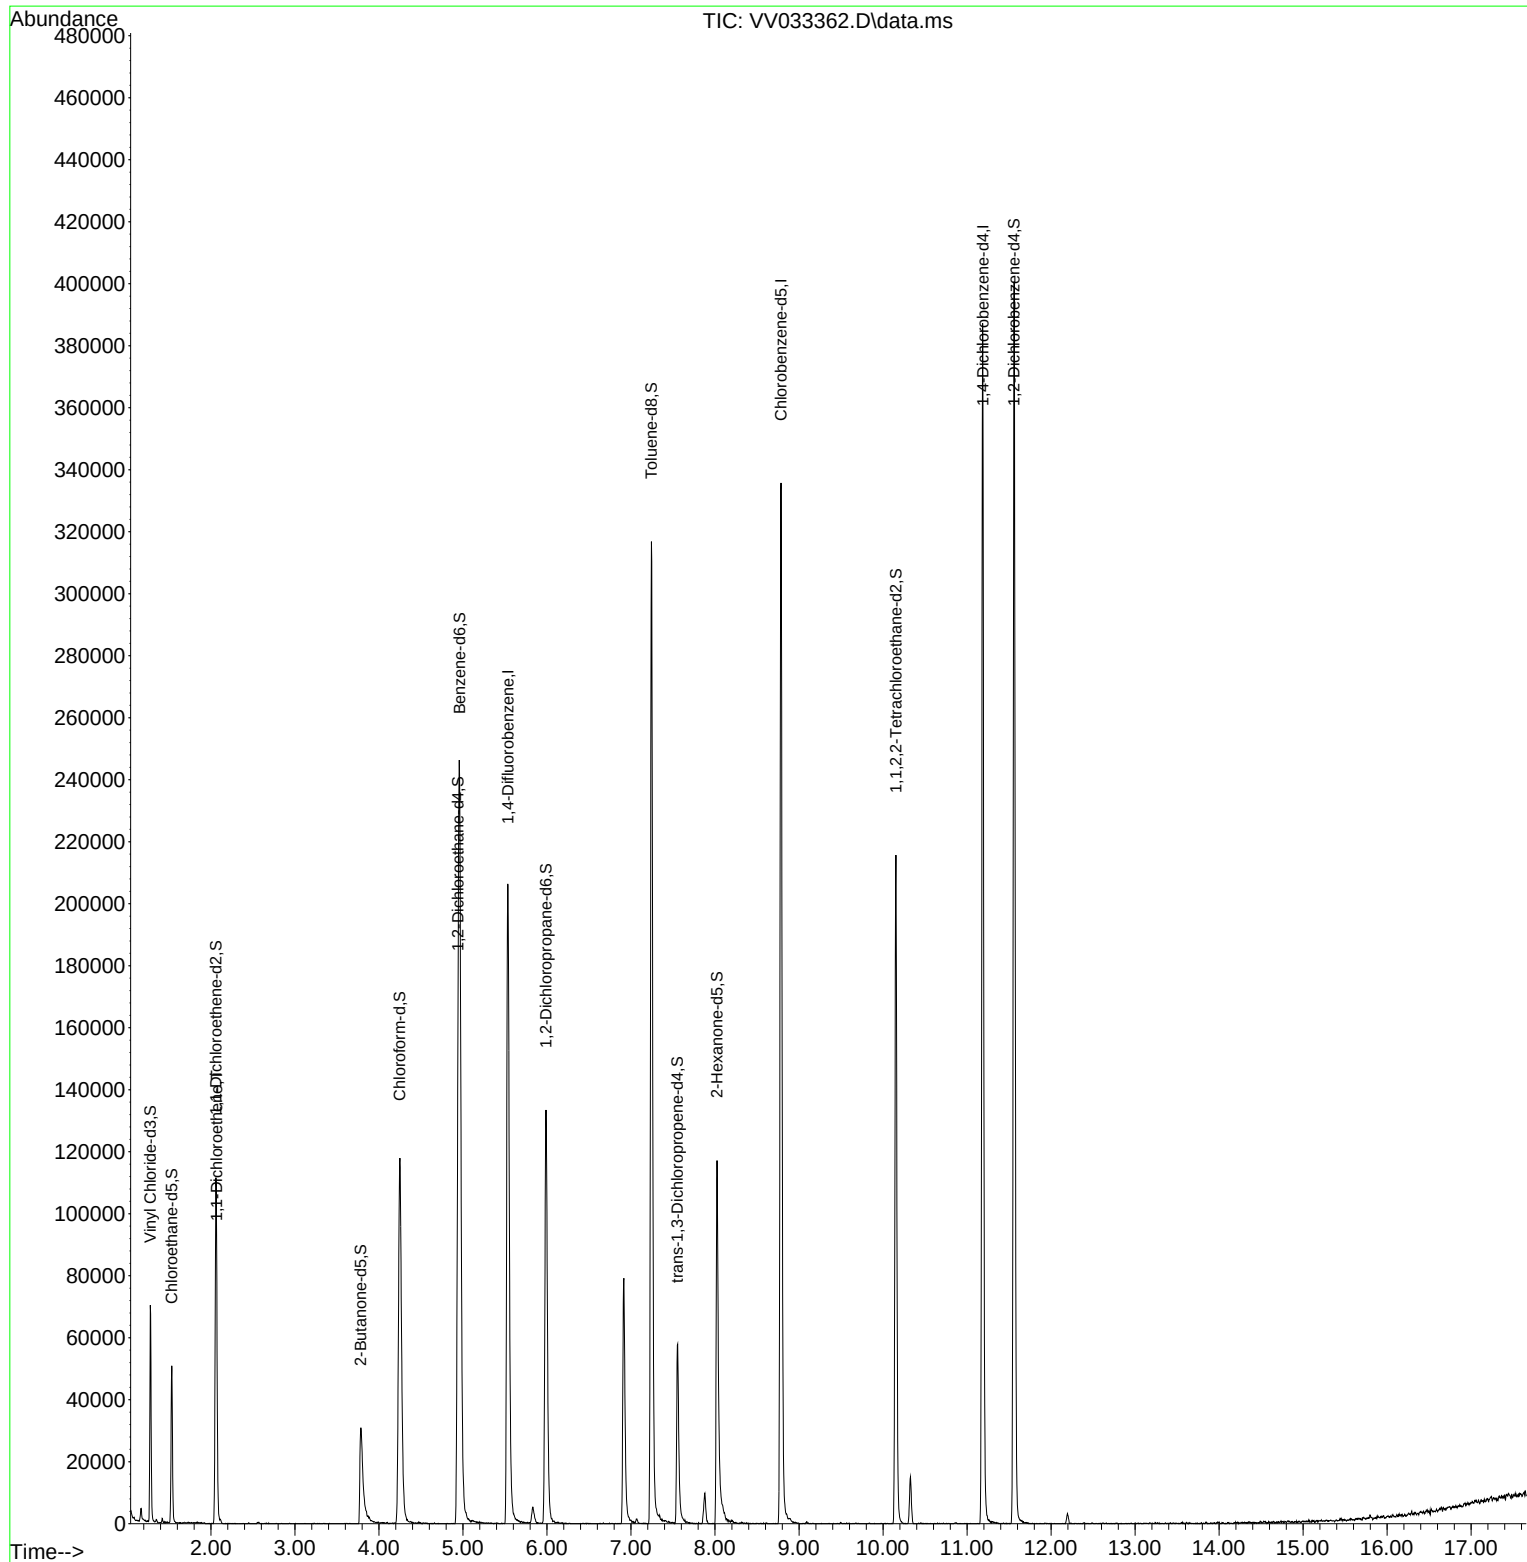

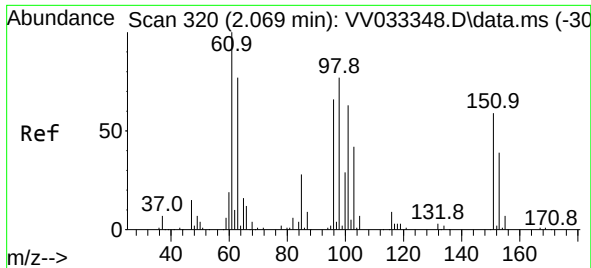

#12
 1,1-Dichloroethene
 Concen: 0.945 ug/L
 RT: 2.069 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV033362.D
 Acq: 15 Dec 2023 02:01

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B03

Tgt Ion: 96 Resp: 969
 Ion Ratio Lower Upper
 96 100
 61 668.7 109.1 202.7#
 63 4130.8 85.3 158.3#

