

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033326.D
 Acq On : 14 Dec 2023 11:42
 Operator : SY/MD
 Sample : VV1214WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK244

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rBV	114986	125988	14.18%	2.059%
2	2.506	452	456	458	rBV	274	209	0.02%	0.003%
3	2.625	487	493	498	rBV2	329	520	0.06%	0.008%
4	2.680	508	510	512	rBV	144	102	0.01%	0.002%
5	2.744	527	530	531	rBV	385	186	0.02%	0.003%
6	2.809	547	550	554	rBB	288	225	0.03%	0.004%
7	2.899	574	578	581	rBV2	303	240	0.03%	0.004%
8	3.015	612	614	615	rBV	243	113	0.01%	0.002%
9	3.043	620	623	625	rBV	279	227	0.03%	0.004%
10	3.082	633	635	637	rBB	234	91	0.01%	0.001%
11	3.095	637	639	641	rBB	226	108	0.01%	0.002%
12	3.117	642	646	647	rBV	226	114	0.01%	0.002%
13	3.175	661	664	668	rBV	274	231	0.03%	0.004%
14	3.281	694	697	701	rBV2	256	231	0.03%	0.004%
15	3.330	711	712	714	rBV2	207	98	0.01%	0.002%
16	3.371	722	725	731	rBV2	318	378	0.04%	0.006%
17	3.420	738	740	742	rBV2	213	122	0.01%	0.002%
18	3.510	765	768	771	rBV	209	188	0.02%	0.003%
19	3.587	791	792	794	rBB	244	91	0.01%	0.001%
20	3.651	808	812	814	rBV	130	112	0.01%	0.002%
21	3.783	844	853	887	rBV2	41661	115966	13.05%	1.895%
22	4.580	1098	1101	1104	rBV	340	229	0.03%	0.004%
23	4.709	1135	1141	1145	rBV2	401	423	0.05%	0.007%
24	4.728	1145	1147	1150	rVV2	355	189	0.02%	0.003%
25	4.770	1157	1160	1161	rBV2	361	199	0.02%	0.003%
26	4.828	1175	1178	1182	rBV2	397	325	0.04%	0.005%
27	4.957	1201	1218	1243	rBV2	332723	888603	100.00%	14.523%
28	5.410	1356	1359	1361	rBV2	299	158	0.02%	0.003%
29	5.532	1386	1397	1427	rBV	268296	553428	62.28%	9.045%
30	5.985	1525	1538	1569	rBV2	180981	381355	42.92%	6.233%
31	6.291	1630	1633	1635	rBB	256	125	0.01%	0.002%
32	6.304	1635	1637	1639	rBV	139	96	0.01%	0.002%
33	6.866	1809	1812	1814	rBB	271	163	0.02%	0.003%
34	6.911	1814	1826	1853	rBV	105146	199473	22.45%	3.260%
35	7.198	1912	1915	1917	rBV	291	166	0.02%	0.003%
36	7.243	1918	1929	1951	rBV	420321	733815	82.58%	11.993%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033326.D
 Acq On : 14 Dec 2023 11:42
 Operator : SY/MD
 Sample : VV1214WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK244

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	7.551	2016	2025	2056	rBV	75657	137379	15.46%	2.245%
38	7.931	2139	2143	2145	rBB2	335	232	0.03%	0.004%
39	7.953	2146	2150	2151	rBV2	269	156	0.02%	0.003%
40	7.985	2158	2160	2162	rBV	258	163	0.02%	0.003%
41	8.024	2163	2172	2201	rBV	151282	287524	32.36%	4.699%
42	8.535	2329	2331	2336	rBB	226	165	0.02%	0.003%
43	8.612	2352	2355	2356	rBV	142	99	0.01%	0.002%
44	8.680	2372	2376	2379	rBB2	311	275	0.03%	0.004%
45	8.709	2380	2385	2390	rBV	406	512	0.06%	0.008%
46	8.783	2397	2408	2434	rBV	428388	710918	80.00%	11.619%
47	9.085	2496	2502	2503	rBV3	598	430	0.05%	0.007%
48	9.169	2526	2528	2531	rBV2	412	229	0.03%	0.004%
49	9.342	2579	2582	2584	rBV	304	179	0.02%	0.003%
50	9.374	2590	2592	2596	rVB	339	256	0.03%	0.004%
51	9.403	2599	2601	2603	rBV	138	99	0.01%	0.002%
52	9.458	2615	2618	2621	rBV2	297	244	0.03%	0.004%
53	9.522	2637	2638	2641	rVB	272	127	0.01%	0.002%
54	9.583	2653	2657	2661	rBB2	341	277	0.03%	0.005%
55	9.606	2662	2664	2667	rBV	143	124	0.01%	0.002%
56	9.638	2671	2674	2676	rVV2	214	120	0.01%	0.002%
57	9.702	2691	2694	2697	rBV	376	251	0.03%	0.004%
58	9.741	2702	2706	2709	rBV2	275	279	0.03%	0.005%
59	9.799	2719	2724	2726	rBV2	281	264	0.03%	0.004%
60	9.847	2736	2739	2742	rBV	266	185	0.02%	0.003%
61	9.863	2742	2744	2746	rBV	481	270	0.03%	0.004%
62	9.898	2753	2755	2760	rBB	339	238	0.03%	0.004%
63	9.927	2760	2764	2768	rBB2	384	371	0.04%	0.006%
64	9.963	2771	2775	2778	rBV	275	260	0.03%	0.004%
65	10.085	2810	2813	2816	rBV	384	294	0.03%	0.005%
66	10.152	2823	2834	2854	rBV	278339	436612	49.13%	7.136%
67	10.326	2880	2888	2896	rBV3	2326	3668	0.41%	0.060%
68	10.403	2910	2912	2916	rVB	343	193	0.02%	0.003%
69	10.535	2947	2953	2959	rBV2	306	519	0.06%	0.008%
70	10.612	2974	2977	2978	rBV	151	103	0.01%	0.002%
71	10.651	2986	2989	2992	rBV	295	225	0.03%	0.004%
72	10.712	3005	3008	3009	rBV	416	220	0.02%	0.004%
73	10.747	3014	3019	3022	rBV	453	402	0.05%	0.007%
74	10.770	3023	3026	3030	rVB2	334	206	0.02%	0.003%
75	10.850	3049	3051	3052	rBV	381	97	0.01%	0.002%
76	10.898	3064	3066	3069	rBB	320	185	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033326.D
 Acq On : 14 Dec 2023 11:42
 Operator : SY/MD
 Sample : VV1214WBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK244

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	10.960	3081	3085	3086	rBV	376	220	0.02%	0.004%
78	10.992	3093	3095	3097	rBV	308	183	0.02%	0.003%
79	11.098	3123	3128	3131	rBV2	405	437	0.05%	0.007%
80	11.185	3144	3155	3184	rBV	469839	731248	82.29%	11.951%
81	11.423	3226	3229	3231	rBV	178	139	0.02%	0.002%
82	11.490	3247	3250	3253	rBV2	334	316	0.04%	0.005%
83	11.561	3260	3272	3292	rBV	491689	776341	87.37%	12.688%
84	11.914	3379	3382	3383	rBV2	362	194	0.02%	0.003%
85	11.956	3393	3395	3397	rBV2	264	127	0.01%	0.002%
86	12.053	3422	3425	3426	rBV2	243	144	0.02%	0.002%
87	12.156	3455	3457	3459	rBV	249	151	0.02%	0.002%
88	12.226	3477	3479	3480	rBV	227	92	0.01%	0.002%
89	12.419	3537	3539	3543	rBV	276	214	0.02%	0.003%
90	12.541	3575	3577	3583	rVB2	441	266	0.03%	0.004%
91	12.628	3602	3604	3605	rBV	272	145	0.02%	0.002%
92	12.676	3617	3619	3621	rBV3	312	178	0.02%	0.003%
93	12.767	3643	3647	3650	rBB2	297	241	0.03%	0.004%
94	12.783	3650	3652	3654	rBB	165	86	0.01%	0.001%
95	12.795	3654	3656	3658	rBV	141	92	0.01%	0.002%
96	12.808	3658	3660	3661	rBV	364	131	0.01%	0.002%
97	13.210	3777	3785	3792	rBV4	2438	3684	0.41%	0.060%
98	13.451	3850	3860	3873	rBV3	8184	14692	1.65%	0.240%
99	13.902	3998	4000	4002	rBV	259	86	0.01%	0.001%
100	13.918	4002	4005	4007	rBV3	733	466	0.05%	0.008%



Sum of corrected areas: 6118510

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033326.D
Acq On : 14 Dec 2023 11:42
Operator : SY/MD
Sample : VV1214WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

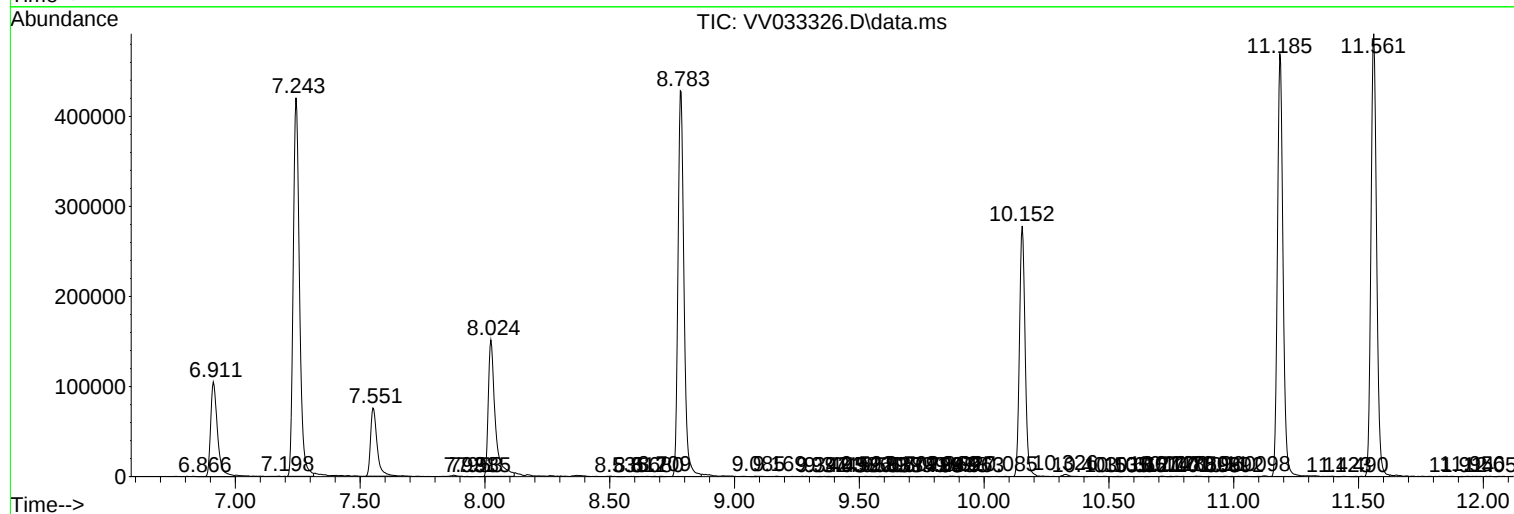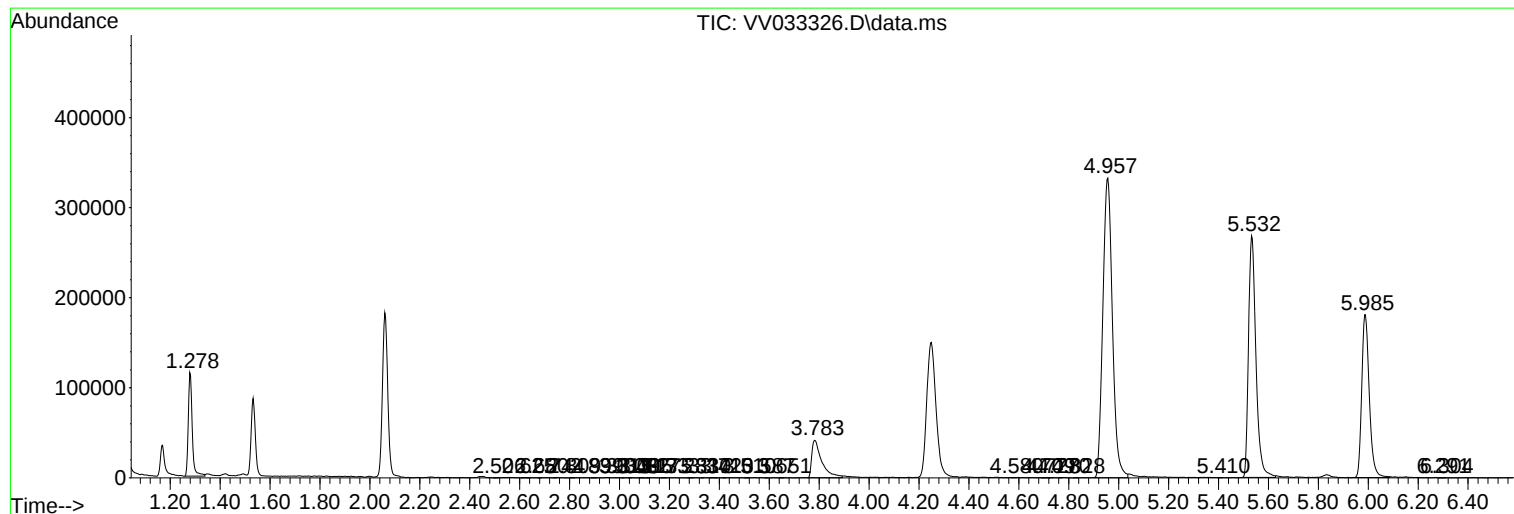

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033326.D
Acq On : 14 Dec 2023 11:42
Operator : SY/MD
Sample : VV1214WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033326.D
Acq On : 14 Dec 2023 11:42
Operator : SY/MD
Sample : VV1214WBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------