

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033330.D
 Acq On : 14 Dec 2023 13:17
 Operator : SY/MD
 Sample : 05799-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033330.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rBV	105210	115688	13.78%	1.830%
2	1.532	147	153	164	rVB	78763	90147	10.74%	1.426%
3	2.060	309	317	330	rVB	170044	243829	29.05%	3.856%
4	2.214	361	365	366	rBV2	571	447	0.05%	0.007%
5	2.310	391	395	398	rBV2	276	269	0.03%	0.004%
6	2.343	403	405	408	rVB	315	179	0.02%	0.003%
7	2.420	426	429	432	rBV	255	185	0.02%	0.003%
8	2.452	432	439	443	rBV5	1848	2223	0.26%	0.035%
9	2.609	483	488	490	rBV	287	248	0.03%	0.004%
10	2.706	515	518	523	rBB	197	177	0.02%	0.003%
11	2.760	530	535	537	rBB	265	204	0.02%	0.003%
12	2.867	564	568	571	rBV2	231	219	0.03%	0.003%
13	2.950	590	594	597	rBB2	282	273	0.03%	0.004%
14	3.114	642	645	646	rBV2	278	156	0.02%	0.002%
15	3.185	665	667	671	rBV	313	255	0.03%	0.004%
16	3.243	681	685	689	rBV	154	194	0.02%	0.003%
17	3.339	712	715	719	rBV	250	219	0.03%	0.003%
18	3.410	732	737	740	rBB	360	294	0.04%	0.005%
19	3.445	743	748	750	rBB	241	185	0.02%	0.003%
20	3.535	773	776	778	rBV	158	125	0.01%	0.002%
21	3.690	822	824	826	rBV2	276	149	0.02%	0.002%
22	3.783	844	853	876	rBV	39397	104377	12.43%	1.651%
23	4.555	1091	1093	1095	rBV2	509	214	0.03%	0.003%
24	4.603	1106	1108	1110	rBV2	255	142	0.02%	0.002%
25	4.793	1160	1167	1170	rBB	236	243	0.03%	0.004%
26	4.844	1181	1183	1184	rBV	353	122	0.01%	0.002%
27	4.886	1194	1196	1199	rBV	250	181	0.02%	0.003%
28	4.957	1201	1218	1247	rBV2	312883	839452	100.00%	13.276%
29	5.535	1384	1398	1433	rBV	268408	555902	66.22%	8.792%
30	5.989	1525	1539	1569	rBV	170983	357063	42.54%	5.647%
31	6.236	1612	1616	1620	rBV	302	273	0.03%	0.004%
32	6.288	1628	1632	1636	rBV	220	256	0.03%	0.004%
33	6.465	1685	1687	1690	rBV	162	128	0.02%	0.002%
34	6.538	1704	1710	1711	rBV	227	182	0.02%	0.003%
35	6.600	1726	1729	1731	rBV	279	212	0.03%	0.003%
36	6.706	1760	1762	1765	rBB	218	137	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033330.D
 Acq On : 14 Dec 2023 13:17
 Operator : SY/MD
 Sample : 05799-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.728	1766	1769	1772	rBV	257	146	0.02%	0.002%
38	6.863	1809	1811	1816	rBB	255	209	0.02%	0.003%
39	6.911	1816	1826	1854	rBV	104076	193526	23.05%	3.061%
40	7.111	1886	1888	1890	rBV	256	184	0.02%	0.003%
41	7.243	1917	1929	1949	rBV	402548	708411	84.39%	11.203%
42	7.551	2015	2025	2047	rBV	73040	133586	15.91%	2.113%
43	7.757	2085	2089	2090	rBV2	244	201	0.02%	0.003%
44	7.876	2113	2126	2142	rBV2	11610	20313	2.42%	0.321%
45	7.976	2155	2157	2161	rBB2	405	284	0.03%	0.004%
46	8.024	2163	2172	2206	rBV	145041	279943	33.35%	4.427%
47	8.381	2281	2283	2285	rBV	330	168	0.02%	0.003%
48	8.481	2310	2314	2316	rBV	339	258	0.03%	0.004%
49	8.632	2358	2361	2364	rBV3	538	418	0.05%	0.007%
50	8.654	2367	2368	2371	rBV	263	150	0.02%	0.002%
51	8.783	2397	2408	2434	rBV	426586	711338	84.74%	11.250%
52	9.085	2498	2502	2509	rBV2	547	739	0.09%	0.012%
53	9.198	2534	2537	2540	rBV	260	207	0.02%	0.003%
54	9.342	2578	2582	2585	rBB	174	163	0.02%	0.003%
55	9.371	2586	2591	2593	rBV	277	222	0.03%	0.004%
56	9.410	2600	2603	2604	rBV	223	123	0.01%	0.002%
57	9.522	2636	2638	2639	rBV	398	175	0.02%	0.003%
58	9.558	2646	2649	2651	rBB	378	227	0.03%	0.004%
59	9.571	2651	2653	2657	rBV	215	171	0.02%	0.003%
60	9.648	2674	2677	2679	rBV2	229	141	0.02%	0.002%
61	9.863	2742	2744	2746	rBB	262	135	0.02%	0.002%
62	9.882	2747	2750	2751	rBV	243	125	0.01%	0.002%
63	9.963	2772	2775	2778	rBB	144	122	0.01%	0.002%
64	9.979	2778	2780	2782	rBV	241	141	0.02%	0.002%
65	10.152	2823	2834	2852	rBV	259622	413605	49.27%	6.541%
66	10.326	2877	2888	2899	rBB3	14045	22033	2.62%	0.348%
67	10.371	2899	2902	2906	rBV2	287	323	0.04%	0.005%
68	10.423	2916	2918	2921	rBV	142	125	0.01%	0.002%
69	10.477	2932	2935	2937	rBB	416	241	0.03%	0.004%
70	10.551	2955	2958	2961	rBV2	273	190	0.02%	0.003%
71	10.754	3017	3021	3023	rBV	184	163	0.02%	0.003%
72	10.779	3026	3029	3031	rBV	284	171	0.02%	0.003%
73	10.808	3035	3038	3042	rVV2	294	185	0.02%	0.003%
74	10.918	3070	3072	3076	rBV	303	250	0.03%	0.004%
75	11.011	3097	3101	3104	rBV	207	221	0.03%	0.003%
76	11.069	3117	3119	3125	rBV2	342	347	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033330.D
 Acq On : 14 Dec 2023 13:17
 Operator : SY/MD
 Sample : 05799-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.185	3144	3155	3183	rBV	481103	753149	89.72%	11.911%
78	11.378	3209	3215	3217	rBV3	633	593	0.07%	0.009%
79	11.471	3242	3244	3246	rBV	401	241	0.03%	0.004%
80	11.561	3260	3272	3291	rBV	479485	756025	90.06%	11.956%
81	11.741	3325	3328	3330	rBV	376	168	0.02%	0.003%
82	11.776	3335	3339	3342	rBV	415	299	0.04%	0.005%
83	11.796	3342	3345	3348	rBV	294	268	0.03%	0.004%
84	11.889	3370	3374	3375	rBV	293	166	0.02%	0.003%
85	12.275	3492	3494	3497	rBV2	373	254	0.03%	0.004%
86	12.413	3534	3537	3539	rBV	263	207	0.02%	0.003%
87	12.493	3559	3562	3566	rBV3	493	451	0.05%	0.007%
88	12.586	3588	3591	3594	rBV2	398	283	0.03%	0.004%
89	12.615	3594	3600	3608	rVB5	1628	2512	0.30%	0.040%
90	12.763	3642	3646	3649	rBV2	445	379	0.05%	0.006%
91	13.117	3753	3756	3757	rBV	339	208	0.02%	0.003%
92	13.313	3815	3817	3820	rBB	536	250	0.03%	0.004%
93	13.332	3820	3823	3826	rBV2	276	236	0.03%	0.004%
94	13.348	3826	3828	3829	rBV	323	149	0.02%	0.002%
95	13.387	3835	3840	3842	rBV2	305	284	0.03%	0.004%
96	13.570	3894	3897	3901	rVB3	326	248	0.03%	0.004%
97	13.747	3948	3952	3956	rBV3	658	613	0.07%	0.010%
98	13.860	3983	3987	3989	rBV	464	371	0.04%	0.006%
99	13.905	3996	4001	4002	rBV	509	429	0.05%	0.007%
100	14.037	4036	4042	4047	rBV5	818	1128	0.13%	0.018%




Sum of corrected areas: 6323140

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033330.D
Acq On : 14 Dec 2023 13:17
Operator : SY/MD
Sample : 05799-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

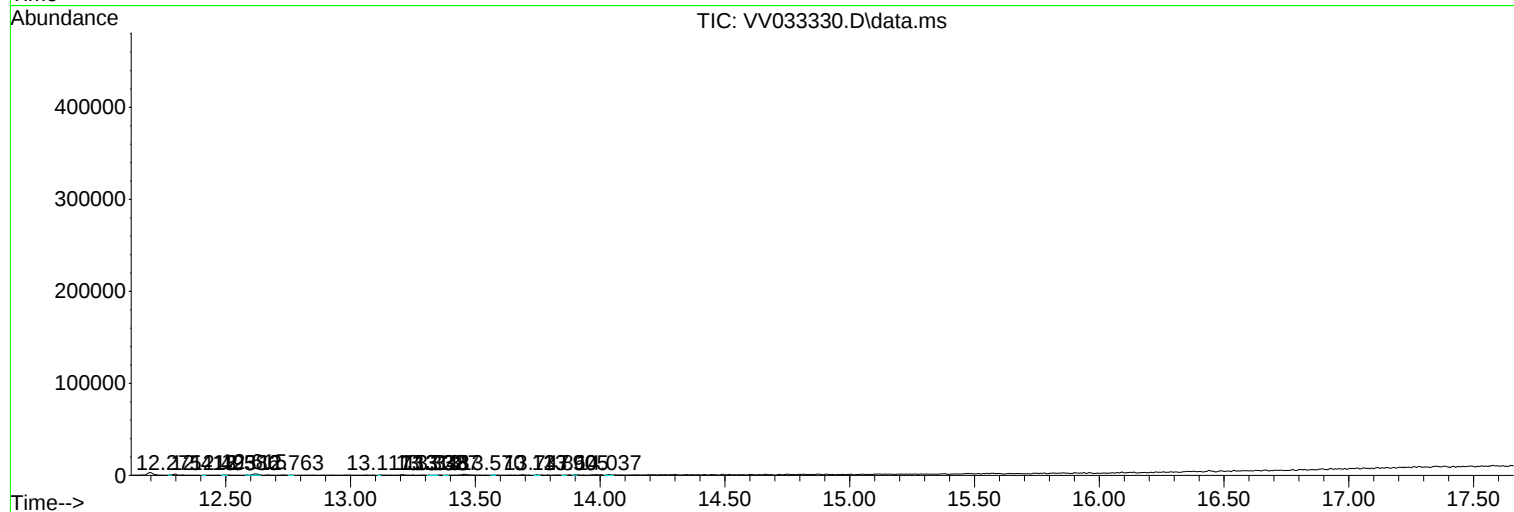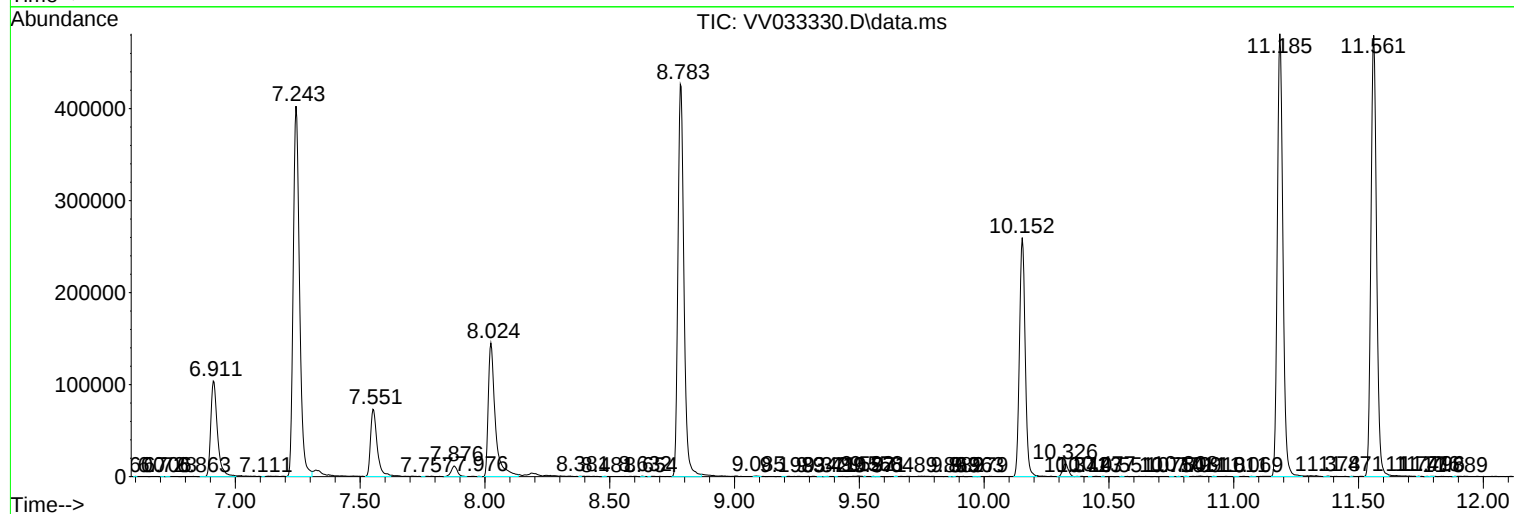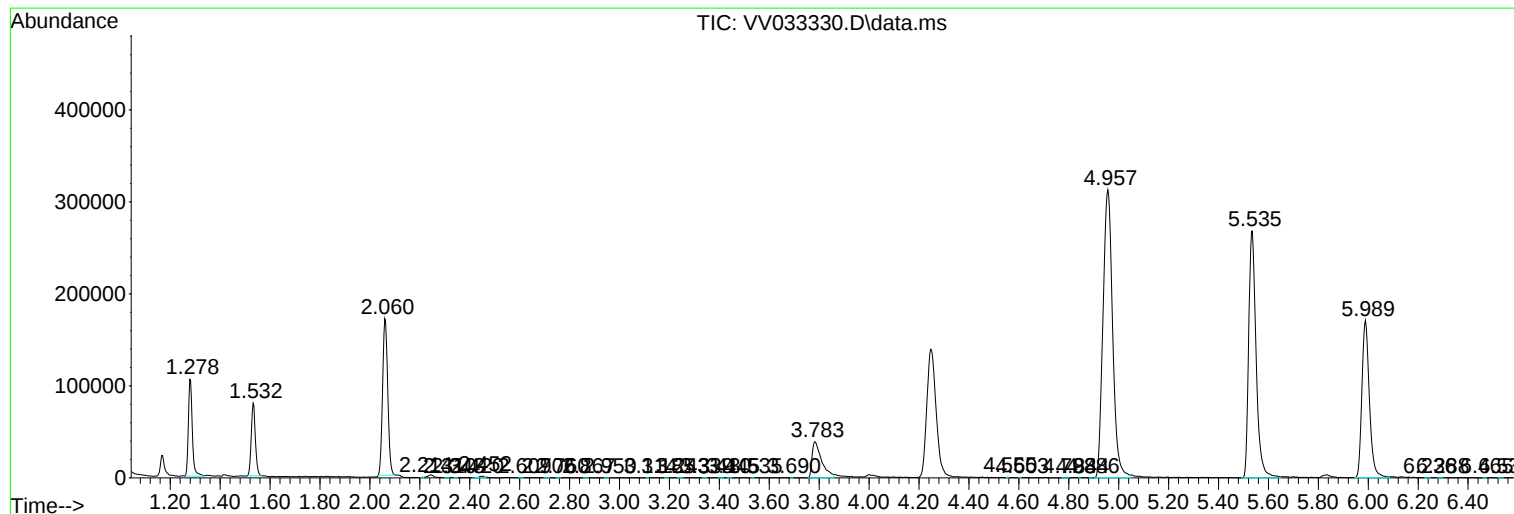

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033330.D
Acq On : 14 Dec 2023 13:17
Operator : SY/MD
Sample : 05799-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033330.D
Acq On : 14 Dec 2023 13:17
Operator : SY/MD
Sample : 05799-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------