

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033333.D
 Acq On : 14 Dec 2023 14:26
 Operator : SY/MD
 Sample : 05682-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033333.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rBV	100579	105921	12.77%	1.701%
2	1.532	147	153	170	rVB	79008	92880	11.20%	1.492%
3	2.060	307	317	340	rVB	167117	247669	29.86%	3.978%
4	2.211	361	364	366	rBV	182	157	0.02%	0.003%
5	2.330	397	401	402	rBV	154	142	0.02%	0.002%
6	2.375	413	415	419	rBV	301	256	0.03%	0.004%
7	2.449	432	438	447	rVB4	1417	2214	0.27%	0.036%
8	2.619	489	491	495	rBB	154	127	0.02%	0.002%
9	2.709	515	519	523	rBV	518	494	0.06%	0.008%
10	2.937	586	590	594	rBV2	274	256	0.03%	0.004%
11	3.031	615	619	623	rBV2	270	227	0.03%	0.004%
12	3.111	640	644	649	rBB2	300	347	0.04%	0.006%
13	3.140	649	653	656	rBB2	247	208	0.03%	0.003%
14	3.285	696	698	701	rBB	254	147	0.02%	0.002%
15	3.384	726	729	731	rBV	155	129	0.02%	0.002%
16	3.651	809	812	815	rVB2	312	194	0.02%	0.003%
17	3.783	843	853	886	rBV	37998	105667	12.74%	1.697%
18	4.597	1103	1106	1108	rBV2	262	187	0.02%	0.003%
19	4.661	1119	1126	1128	rBB2	371	376	0.05%	0.006%
20	4.683	1129	1133	1137	rBB3	474	388	0.05%	0.006%
21	4.738	1146	1150	1151	rBV	321	193	0.02%	0.003%
22	4.957	1201	1218	1248	rBV2	310469	829361	100.00%	13.322%
23	5.410	1354	1359	1362	rBV2	295	349	0.04%	0.006%
24	5.532	1385	1397	1425	rBV	261343	538389	64.92%	8.648%
25	5.989	1526	1539	1567	rBV	168349	350968	42.32%	5.637%
26	6.359	1651	1654	1660	rBV	128	209	0.03%	0.003%
27	6.494	1693	1696	1699	rBB	252	161	0.02%	0.003%
28	6.728	1766	1769	1772	rBB	301	225	0.03%	0.004%
29	6.912	1816	1826	1842	rBV2	98863	182763	22.04%	2.936%
30	7.059	1870	1872	1873	rBV	540	262	0.03%	0.004%
31	7.243	1918	1929	1953	rBV	401122	708978	85.48%	11.388%
32	7.551	2016	2025	2047	rBV	73370	129157	15.57%	2.075%
33	7.822	2106	2109	2111	rBV	135	123	0.01%	0.002%
34	7.950	2146	2149	2151	rBV	296	213	0.03%	0.003%
35	8.024	2163	2172	2205	rBV	141328	276562	33.35%	4.442%
36	8.461	2305	2308	2313	rBV2	474	412	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033333.D
 Acq On : 14 Dec 2023 14:26
 Operator : SY/MD
 Sample : 05682-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	8.558	2337	2338	2342	rBB	225	130	0.02%	0.002%
38	8.606	2350	2353	2355	rBV	156	128	0.02%	0.002%
39	8.648	2364	2366	2368	rBV	408	206	0.02%	0.003%
40	8.680	2373	2376	2377	rBV	238	131	0.02%	0.002%
41	8.783	2397	2408	2432	rBV	416891	694657	83.76%	11.158%
42	9.005	2474	2477	2483	rBV3	505	416	0.05%	0.007%
43	9.075	2497	2499	2503	rVB	346	247	0.03%	0.004%
44	9.137	2514	2518	2521	rBB	274	205	0.02%	0.003%
45	9.477	2622	2624	2625	rBV	260	124	0.01%	0.002%
46	9.519	2635	2637	2639	rBV	237	136	0.02%	0.002%
47	9.577	2652	2655	2656	rBV	252	166	0.02%	0.003%
48	9.619	2666	2668	2672	rBV2	545	364	0.04%	0.006%
49	9.754	2707	2710	2713	rBV	181	174	0.02%	0.003%
50	9.889	2749	2752	2754	rBV	271	128	0.02%	0.002%
51	10.005	2786	2788	2791	rBB	249	125	0.02%	0.002%
52	10.153	2820	2834	2852	rBV	263056	415651	50.12%	6.676%
53	10.288	2873	2876	2878	rBB	304	189	0.02%	0.003%
54	10.329	2879	2889	2898	rBV2	6506	10307	1.24%	0.166%
55	10.378	2903	2904	2908	rBV	223	139	0.02%	0.002%
56	10.452	2925	2927	2931	rBB	231	128	0.02%	0.002%
57	10.477	2932	2935	2937	rBV	174	143	0.02%	0.002%
58	10.600	2969	2973	2977	rBB2	416	309	0.04%	0.005%
59	10.661	2988	2992	2997	rBB	302	255	0.03%	0.004%
60	10.690	2998	3001	3005	rBB2	287	240	0.03%	0.004%
61	10.780	3026	3029	3031	rBB2	226	142	0.02%	0.002%
62	10.799	3032	3035	3037	rBB	277	156	0.02%	0.003%
63	10.828	3042	3044	3048	rBV	272	216	0.03%	0.003%
64	10.870	3053	3057	3058	rBV2	330	275	0.03%	0.004%
65	10.934	3072	3077	3081	rBB	311	365	0.04%	0.006%
66	11.133	3137	3139	3142	rBB	300	164	0.02%	0.003%
67	11.185	3143	3155	3178	rBV	480855	746200	89.97%	11.986%
68	11.416	3224	3227	3228	rBV	373	245	0.03%	0.004%
69	11.468	3238	3243	3244	rBV2	276	217	0.03%	0.003%
70	11.500	3250	3253	3256	rVB2	346	239	0.03%	0.004%
71	11.561	3260	3272	3294	rBV	488740	768270	92.63%	12.340%
72	11.735	3324	3326	3328	rBV	240	137	0.02%	0.002%
73	11.821	3349	3353	3354	rBV	315	234	0.03%	0.004%
74	11.876	3366	3370	3374	rBV2	401	428	0.05%	0.007%
75	11.937	3386	3389	3391	rBV	257	159	0.02%	0.003%
76	12.053	3423	3425	3430	rBB	247	205	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033333.D
 Acq On : 14 Dec 2023 14:26
 Operator : SY/MD
 Sample : 05682-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.108	3441	3442	3445	rBV	335	181	0.02%	0.003%
78	12.162	3457	3459	3461	rBV	201	133	0.02%	0.002%
79	12.268	3490	3492	3494	rBV	232	132	0.02%	0.002%
80	12.345	3512	3516	3518	rBV2	368	315	0.04%	0.005%
81	12.435	3540	3544	3545	rBV	203	161	0.02%	0.003%
82	12.686	3618	3622	3625	rBV2	346	330	0.04%	0.005%
83	12.757	3640	3644	3645	rBV	344	211	0.03%	0.003%
84	12.789	3651	3654	3655	rBV	329	204	0.02%	0.003%
85	13.085	3742	3746	3751	rBB2	285	261	0.03%	0.004%
86	13.143	3756	3764	3766	rBV2	331	528	0.06%	0.008%
87	13.191	3777	3779	3781	rBV	258	171	0.02%	0.003%
88	13.278	3804	3806	3812	rBV2	323	260	0.03%	0.004%
89	13.336	3822	3824	3827	rBV2	279	238	0.03%	0.004%
90	13.577	3896	3899	3902	rBV2	386	270	0.03%	0.004%
91	13.632	3911	3916	3919	rBV2	515	397	0.05%	0.006%
92	13.664	3923	3926	3927	rBV2	376	227	0.03%	0.004%
93	13.702	3936	3938	3943	rBV	279	169	0.02%	0.003%
94	13.722	3943	3944	3947	rVB2	337	140	0.02%	0.002%
95	13.754	3948	3954	3956	rBV3	445	521	0.06%	0.008%
96	13.866	3986	3989	3991	rBV	153	124	0.01%	0.002%
97	14.043	4041	4044	4045	rBV2	494	262	0.03%	0.004%
98	14.146	4073	4076	4082	rBV4	560	604	0.07%	0.010%
99	14.487	4181	4182	4186	rBV	495	363	0.04%	0.006%
100	14.574	4204	4209	4210	rBV2	954	757	0.09%	0.012%




Sum of corrected areas: 6225620

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033333.D
Acq On : 14 Dec 2023 14:26
Operator : SY/MD
Sample : 05682-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

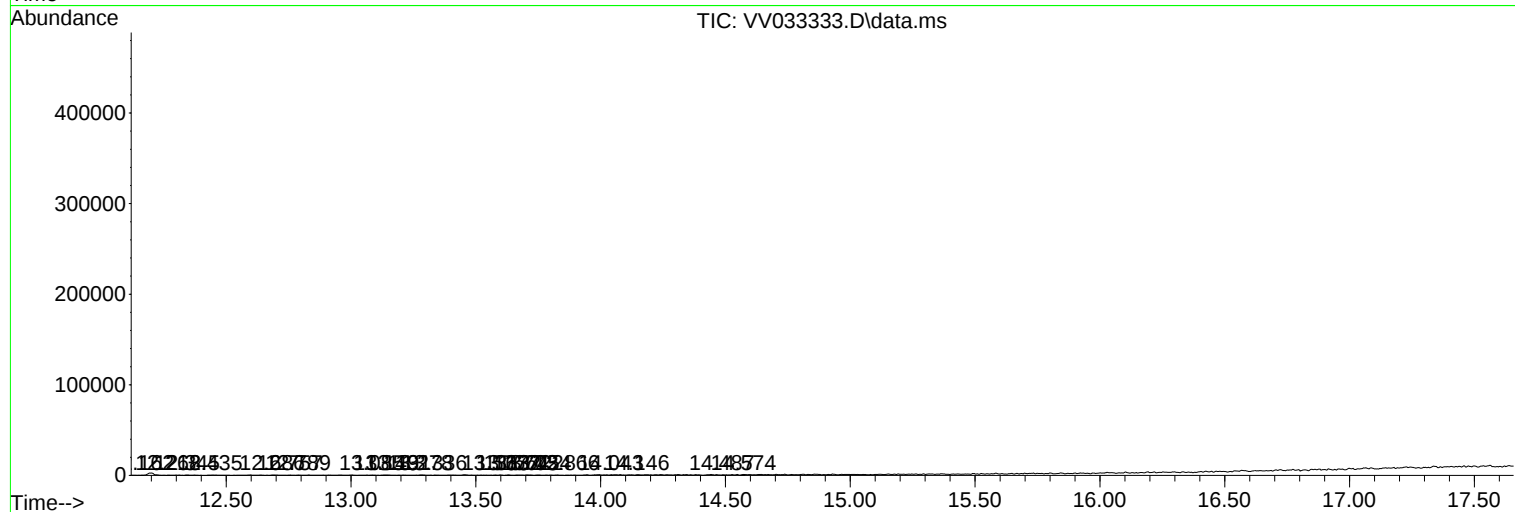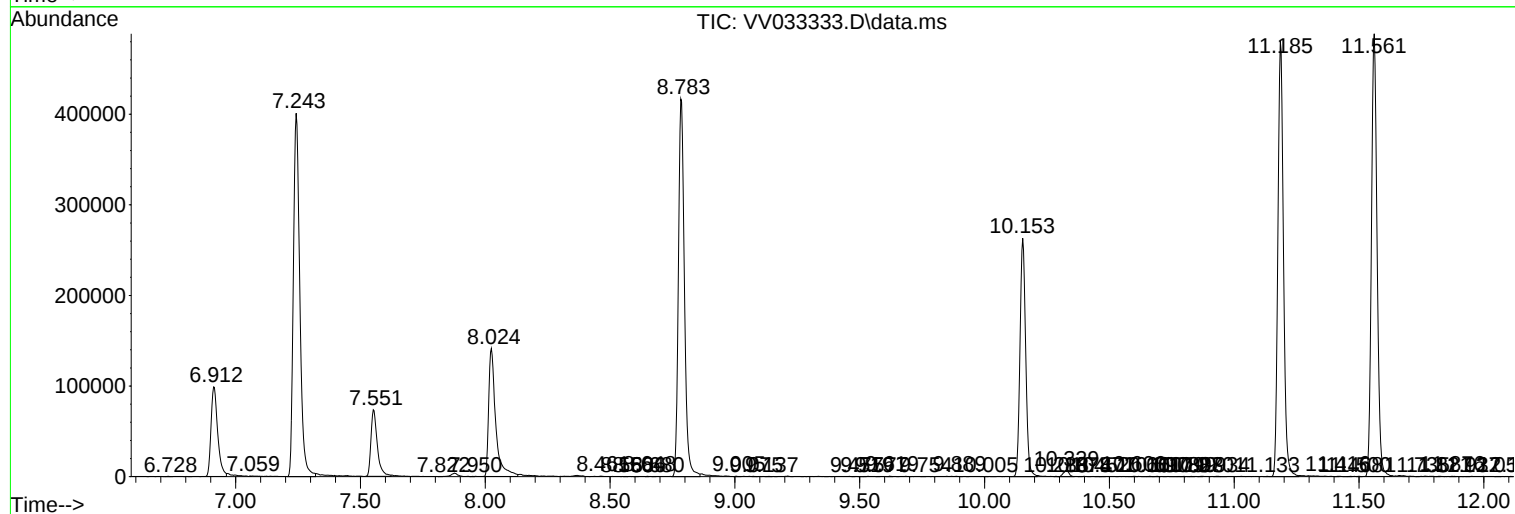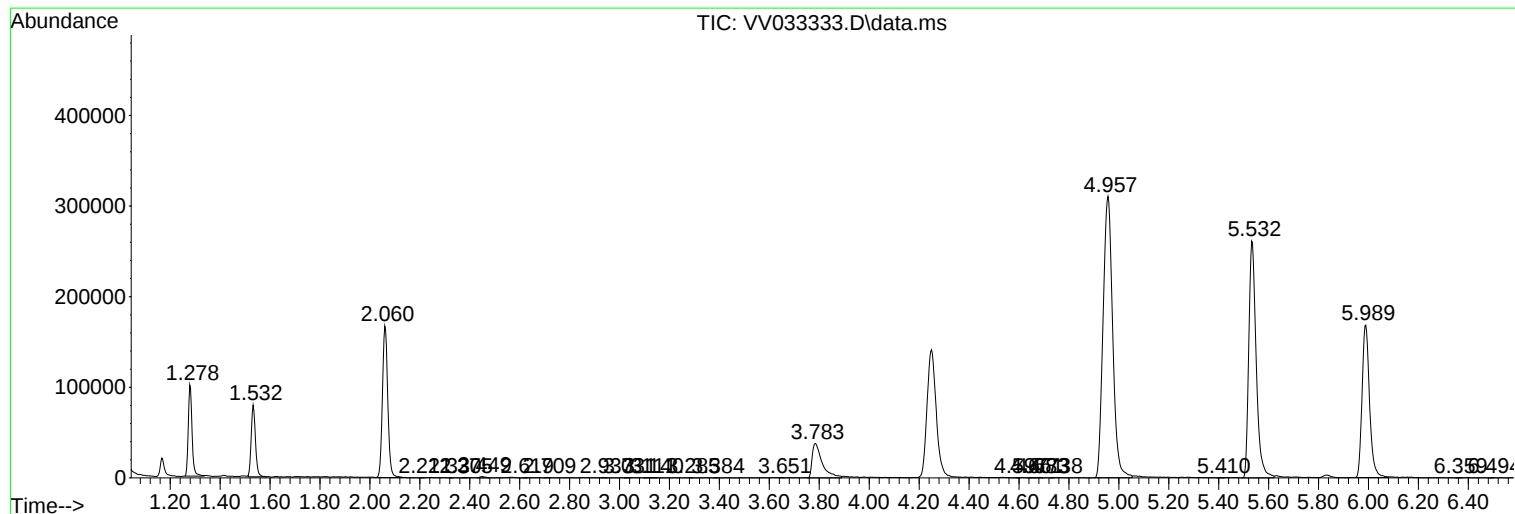

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033333.D
Acq On : 14 Dec 2023 14:26
Operator : SY/MD
Sample : 05682-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033333.D
Acq On : 14 Dec 2023 14:26
Operator : SY/MD
Sample : 05682-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------