

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033335.D
 Acq On : 14 Dec 2023 15:13
 Operator : SY/MD
 Sample : 05794-01
 Misc : 4.70g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033335.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rBV	99814	99204	12.41%	1.570%
2	1.532	146	153	168	rVB	72208	85947	10.75%	1.360%
3	2.060	309	317	337	rVB	161413	234324	29.31%	3.708%
4	2.217	364	366	369	rBB	260	143	0.02%	0.002%
5	2.365	409	412	415	rBV	192	170	0.02%	0.003%
6	2.417	426	428	432	rBB	274	179	0.02%	0.003%
7	2.446	432	437	444	rBV3	1156	1424	0.18%	0.023%
8	2.989	604	606	609	rBV2	373	234	0.03%	0.004%
9	3.230	678	681	684	rBB2	233	140	0.02%	0.002%
10	3.253	685	688	689	rBV	246	139	0.02%	0.002%
11	3.696	824	826	830	rBB	157	132	0.02%	0.002%
12	3.741	837	840	844	rBV	275	229	0.03%	0.004%
13	3.783	844	853	888	rBV	37733	105353	13.18%	1.667%
14	4.182	974	977	980	rBV	361	286	0.04%	0.005%
15	4.249	980	998	1023	rBV	134069	341693	42.74%	5.408%
16	4.735	1147	1149	1151	rBV	264	163	0.02%	0.003%
17	4.957	1199	1218	1250	rBV2	299181	799488	100.00%	12.653%
18	5.449	1369	1371	1374	rBV2	262	179	0.02%	0.003%
19	5.532	1386	1397	1433	rBV	246369	519195	64.94%	8.217%
20	5.989	1526	1539	1561	rBV	164535	335915	42.02%	5.316%
21	6.204	1601	1606	1610	rBV2	364	352	0.04%	0.006%
22	6.246	1616	1619	1621	rBV	269	169	0.02%	0.003%
23	6.285	1627	1631	1632	rBB	332	201	0.03%	0.003%
24	6.298	1632	1635	1637	rBB	270	143	0.02%	0.002%
25	6.362	1652	1655	1658	rBB	223	138	0.02%	0.002%
26	6.433	1674	1677	1679	rBV	253	166	0.02%	0.003%
27	6.484	1691	1693	1695	rBB	268	137	0.02%	0.002%
28	6.535	1706	1709	1711	rBB	273	195	0.02%	0.003%
29	6.552	1711	1714	1717	rBV	121	129	0.02%	0.002%
30	6.622	1730	1736	1738	rBV	491	398	0.05%	0.006%
31	6.703	1758	1761	1763	rBV	240	174	0.02%	0.003%
32	6.748	1772	1775	1778	rBV	181	163	0.02%	0.003%
33	6.831	1798	1801	1806	rBB	325	261	0.03%	0.004%
34	6.912	1814	1826	1850	rBV	95949	179469	22.45%	2.840%
35	7.243	1918	1929	1953	rBV	384240	673566	84.25%	10.660%
36	7.551	2016	2025	2055	rBV	68093	126385	15.81%	2.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033335.D
 Acq On : 14 Dec 2023 15:13
 Operator : SY/MD
 Sample : 05794-01
 Misc : 4.70g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	7.780	2095	2096	2098	rBV	328	142	0.02%	0.002%
38	7.873	2116	2125	2127	rBV4	1455	1835	0.23%	0.029%
39	7.937	2143	2145	2147	rBV	238	141	0.02%	0.002%
40	7.979	2156	2158	2161	rBV	227	158	0.02%	0.003%
41	8.024	2163	2172	2202	rBV	139041	260227	32.55%	4.118%
42	8.436	2296	2300	2302	rBB2	289	214	0.03%	0.003%
43	8.445	2302	2303	2308	rBB	225	176	0.02%	0.003%
44	8.539	2329	2332	2336	rBV2	279	262	0.03%	0.004%
45	8.587	2343	2347	2349	rBB	305	210	0.03%	0.003%
46	8.783	2395	2408	2446	rBV	406935	679534	85.00%	10.754%
47	9.059	2492	2494	2498	rBV	173	164	0.02%	0.003%
48	9.185	2530	2533	2536	rBB	295	201	0.03%	0.003%
49	9.262	2554	2557	2560	rBB2	250	160	0.02%	0.003%
50	9.526	2635	2639	2641	rBV	154	145	0.02%	0.002%
51	9.603	2661	2663	2665	rBB	307	138	0.02%	0.002%
52	9.625	2668	2670	2673	rBV	247	159	0.02%	0.003%
53	9.767	2711	2714	2718	rBB2	223	135	0.02%	0.002%
54	9.838	2734	2736	2741	rBB	150	157	0.02%	0.002%
55	9.902	2752	2756	2759	rBB	261	228	0.03%	0.004%
56	9.963	2771	2775	2777	rBV2	224	180	0.02%	0.003%
57	10.024	2790	2794	2796	rBB2	510	290	0.04%	0.005%
58	10.153	2823	2834	2862	rVB	258005	400407	50.08%	6.337%
59	10.268	2865	2870	2871	rBV	350	254	0.03%	0.004%
60	10.371	2898	2902	2905	rBB	212	187	0.02%	0.003%
61	10.423	2916	2918	2925	rBB	172	185	0.02%	0.003%
62	10.458	2926	2929	2934	rBB3	264	264	0.03%	0.004%
63	10.567	2961	2963	2968	rBB	252	187	0.02%	0.003%
64	10.638	2981	2985	2987	rBV	143	133	0.02%	0.002%
65	10.677	2994	2997	3000	rBV2	235	169	0.02%	0.003%
66	10.735	3013	3015	3018	rBV	171	137	0.02%	0.002%
67	10.796	3032	3034	3037	rBB	232	133	0.02%	0.002%
68	10.911	3064	3070	3072	rBB	166	192	0.02%	0.003%
69	10.956	3081	3084	3087	rBV	256	229	0.03%	0.004%
70	11.082	3119	3123	3125	rBB	247	164	0.02%	0.003%
71	11.137	3138	3140	3144	rVB	449	297	0.04%	0.005%
72	11.185	3144	3155	3183	rBV	457247	714084	89.32%	11.301%
73	11.410	3221	3225	3229	rBV2	479	364	0.05%	0.006%
74	11.448	3235	3237	3239	rVB	287	151	0.02%	0.002%
75	11.471	3240	3244	3246	rBB2	380	236	0.03%	0.004%
76	11.513	3254	3257	3259	rBV	238	141	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033335.D
 Acq On : 14 Dec 2023 15:13
 Operator : SY/MD
 Sample : 05794-01
 Misc : 4.70g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.561	3259	3272	3299	rVV	466630	742045	92.82%	11.744%
78	11.744	3326	3329	3331	rBV	278	145	0.02%	0.002%
79	11.834	3351	3357	3360	rBB3	421	486	0.06%	0.008%
80	11.870	3365	3368	3370	rBV	195	147	0.02%	0.002%
81	11.979	3400	3402	3408	rBB	150	151	0.02%	0.002%
82	12.194	3460	3469	3471	rBV3	1885	2228	0.28%	0.035%
83	12.255	3484	3488	3490	rBV	247	200	0.03%	0.003%
84	12.349	3515	3517	3519	rBV	272	173	0.02%	0.003%
85	12.362	3519	3521	3524	rVB	453	158	0.02%	0.003%
86	12.603	3594	3596	3599	rBV2	239	158	0.02%	0.003%
87	12.616	3599	3600	3604	rVV	267	152	0.02%	0.002%
88	12.670	3614	3617	3620	rBV	263	223	0.03%	0.004%
89	12.699	3623	3626	3627	rBV2	283	176	0.02%	0.003%
90	12.792	3649	3655	3656	rBV	345	202	0.03%	0.003%
91	12.821	3661	3664	3666	rBV	304	255	0.03%	0.004%
92	12.873	3677	3680	3682	rBV	294	225	0.03%	0.004%
93	13.072	3738	3742	3744	rBV2	259	190	0.02%	0.003%
94	13.124	3755	3758	3760	rBV	323	207	0.03%	0.003%
95	13.297	3807	3812	3814	rBV3	442	360	0.05%	0.006%
96	13.593	3902	3904	3908	rBV2	343	280	0.04%	0.004%
97	13.648	3919	3921	3923	rBV	245	163	0.02%	0.003%
98	13.918	4002	4005	4006	rBV2	571	309	0.04%	0.005%
99	14.066	4048	4051	4052	rBV	439	201	0.03%	0.003%
100	14.345	4136	4138	4142	rBV3	533	498	0.06%	0.008%




Sum of corrected areas: 6318685

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033335.D
Acq On : 14 Dec 2023 15:13
Operator : SY/MD
Sample : 05794-01
Misc : 4.70g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

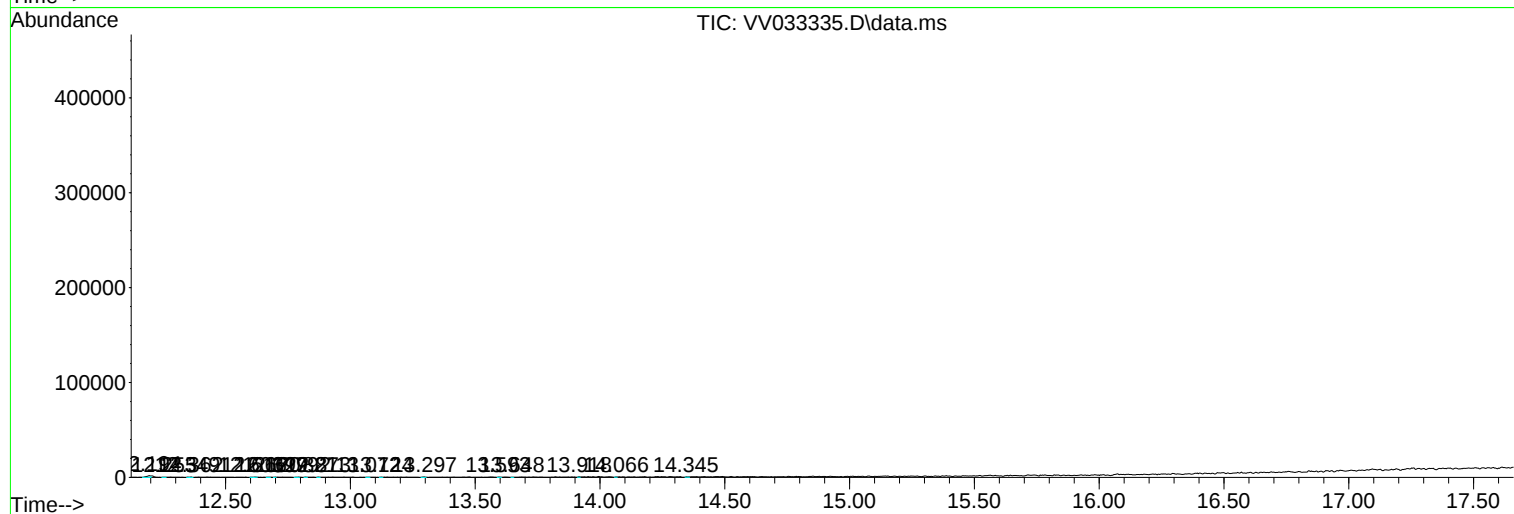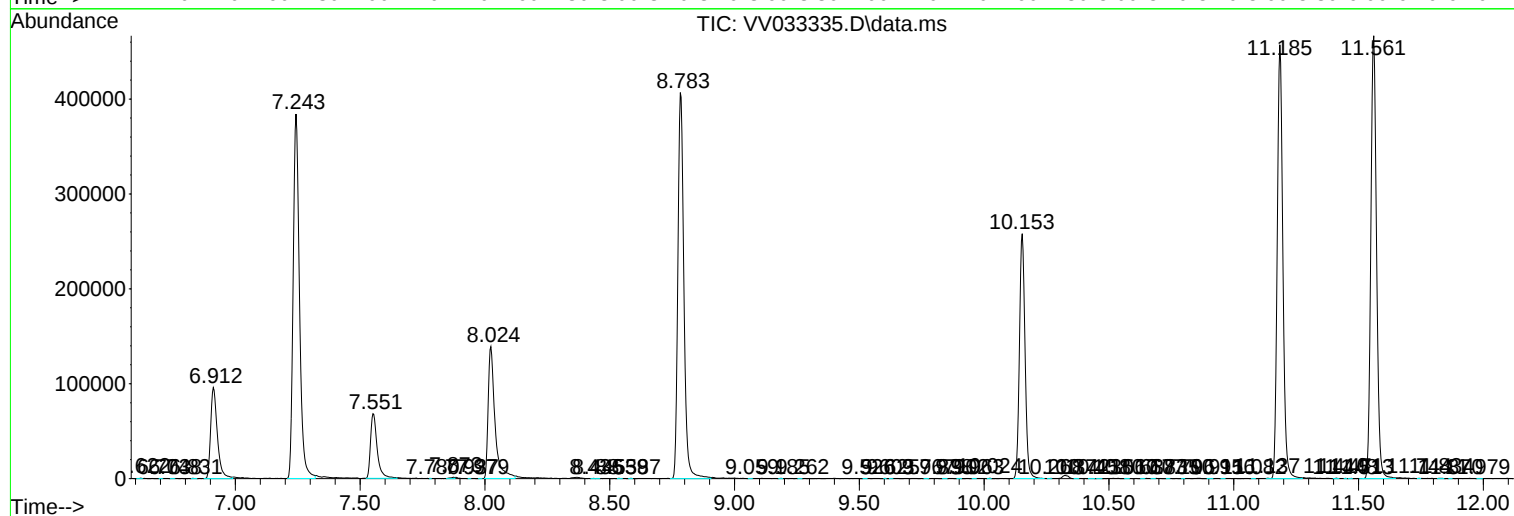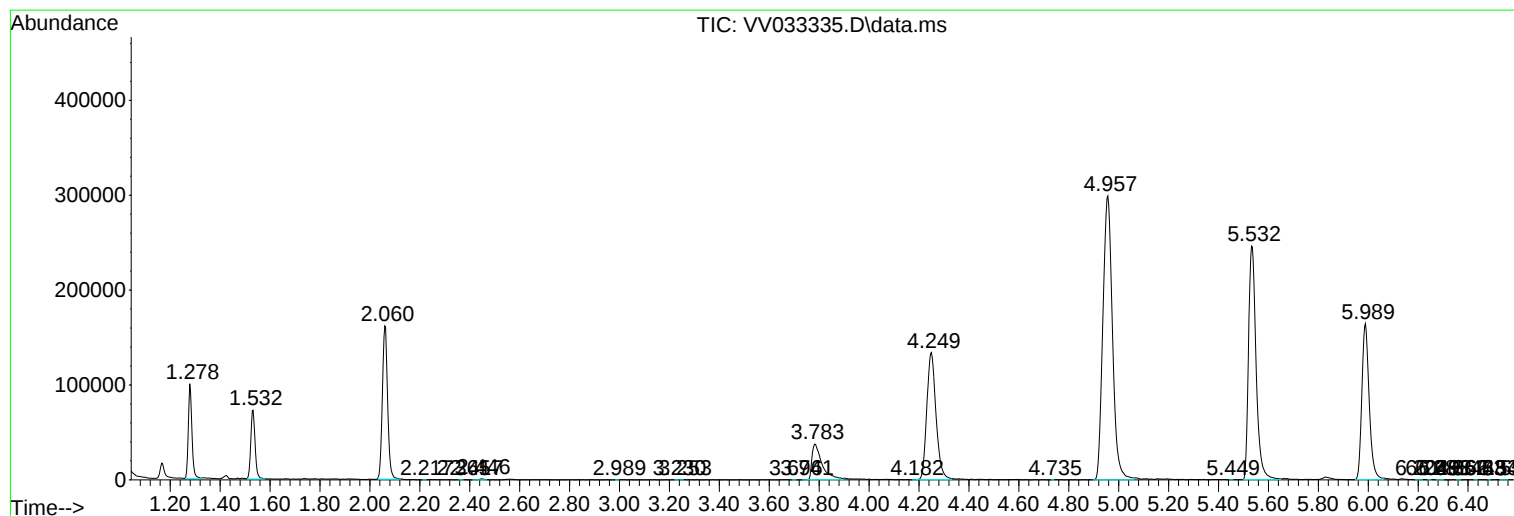

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033335.D
Acq On : 14 Dec 2023 15:13
Operator : SY/MD
Sample : 05794-01
Misc : 4.70g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033335.D
Acq On : 14 Dec 2023 15:13
Operator : SY/MD
Sample : 05794-01
Misc : 4.70g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------