

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033337.D
 Acq On : 14 Dec 2023 15:59
 Operator : SY/MD
 Sample : 05794-03
 Misc : 4.12g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rBV	101796	105027	11.98%	1.650%
2	1.532	146	153	170	rVB	79985	94286	10.76%	1.481%
3	2.059	307	317	335	rBV	179340	259753	29.63%	4.081%
4	2.301	388	392	393	rBV	392	234	0.03%	0.004%
5	2.410	424	426	430	rBB2	223	169	0.02%	0.003%
6	2.449	431	438	445	rBV4	1042	1550	0.18%	0.024%
7	2.551	465	470	472	rBV3	585	637	0.07%	0.010%
8	2.741	526	529	533	rBB	188	170	0.02%	0.003%
9	2.915	578	583	586	rBV	193	238	0.03%	0.004%
10	3.156	656	658	662	rBB	237	152	0.02%	0.002%
11	3.487	758	761	765	rBV	252	220	0.03%	0.003%
12	3.532	772	775	778	rBB	201	152	0.02%	0.002%
13	3.783	843	853	875	rBV	40603	106017	12.09%	1.666%
14	4.130	959	961	962	rBV	280	150	0.02%	0.002%
15	4.465	1061	1065	1068	rBV2	689	688	0.08%	0.011%
16	4.632	1115	1117	1121	rBV2	328	269	0.03%	0.004%
17	4.680	1128	1132	1135	rBB2	489	386	0.04%	0.006%
18	4.883	1193	1195	1198	rBV	270	142	0.02%	0.002%
19	4.956	1201	1218	1245	rBV2	328768	876573	100.00%	13.772%
20	5.445	1365	1370	1373	rBB	284	223	0.03%	0.004%
21	5.532	1383	1397	1427	rBV	246853	509157	58.08%	7.999%
22	5.831	1478	1490	1505	rBV5	3447	7603	0.87%	0.119%
23	5.989	1525	1539	1561	rBV	181166	370411	42.26%	5.819%
24	6.249	1618	1620	1622	rBV	343	174	0.02%	0.003%
25	6.471	1685	1689	1692	rBB	160	137	0.02%	0.002%
26	6.522	1701	1705	1707	rBV	132	133	0.02%	0.002%
27	6.587	1724	1725	1732	rBV	361	261	0.03%	0.004%
28	6.911	1816	1826	1857	rBV	104889	196710	22.44%	3.090%
29	7.156	1900	1902	1905	rVB	376	151	0.02%	0.002%
30	7.175	1905	1908	1913	rBB	199	176	0.02%	0.003%
31	7.243	1917	1929	1957	rBV	423689	748784	85.42%	11.764%
32	7.551	2016	2025	2051	rBV	77267	137630	15.70%	2.162%
33	7.735	2080	2082	2084	rVB2	375	167	0.02%	0.003%
34	7.757	2087	2089	2091	rBV	355	202	0.02%	0.003%
35	7.808	2103	2105	2107	rVB	239	130	0.01%	0.002%
36	7.821	2107	2109	2112	rBV	243	161	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033337.D
 Acq On : 14 Dec 2023 15:59
 Operator : SY/MD
 Sample : 05794-03
 Misc : 4.12g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	7.985	2155	2160	2162	rBV	255	216	0.02%	0.003%
38	8.024	2163	2172	2207	rBV	154348	290779	33.17%	4.568%
39	8.471	2308	2311	2313	rBV	257	166	0.02%	0.003%
40	8.699	2379	2382	2384	rBV	287	167	0.02%	0.003%
41	8.783	2398	2408	2437	rBV	400021	666820	76.07%	10.476%
42	9.027	2482	2484	2487	rBV	265	192	0.02%	0.003%
43	9.082	2497	2501	2502	rBV	273	166	0.02%	0.003%
44	9.107	2507	2509	2512	rBV	156	138	0.02%	0.002%
45	9.181	2529	2532	2537	rBV3	360	336	0.04%	0.005%
46	9.246	2546	2552	2556	rBB	201	271	0.03%	0.004%
47	9.275	2556	2561	2563	rBV	271	248	0.03%	0.004%
48	9.503	2629	2632	2636	rBV2	268	251	0.03%	0.004%
49	9.725	2698	2701	2703	rVB2	263	163	0.02%	0.003%
50	9.747	2704	2708	2710	rBV	164	140	0.02%	0.002%
51	9.783	2715	2719	2722	rBV2	302	264	0.03%	0.004%
52	9.947	2766	2770	2772	rBB2	247	172	0.02%	0.003%
53	10.152	2823	2834	2854	rBV	278356	437488	49.91%	6.873%
54	10.278	2871	2873	2877	rBB	382	229	0.03%	0.004%
55	10.326	2878	2888	2900	rBV2	3586	5274	0.60%	0.083%
56	10.413	2912	2915	2918	rBV	178	167	0.02%	0.003%
57	10.455	2925	2928	2930	rBV	153	133	0.02%	0.002%
58	10.493	2938	2940	2943	rBV	279	190	0.02%	0.003%
59	10.535	2949	2953	2955	rBV2	230	195	0.02%	0.003%
60	10.567	2959	2963	2966	rBB	194	145	0.02%	0.002%
61	10.844	3046	3049	3050	rBV	209	135	0.02%	0.002%
62	10.966	3084	3087	3090	rBB	257	167	0.02%	0.003%
63	11.021	3100	3104	3110	rBV2	306	366	0.04%	0.006%
64	11.185	3143	3155	3181	rBV	454463	713450	81.39%	11.209%
65	11.371	3210	3213	3216	rBV2	501	281	0.03%	0.004%
66	11.484	3244	3248	3252	rBB	173	160	0.02%	0.003%
67	11.561	3261	3272	3291	rBV	518179	818794	93.41%	12.864%
68	12.001	3406	3409	3410	rBV	267	142	0.02%	0.002%
69	12.030	3415	3418	3420	rBB2	344	178	0.02%	0.003%
70	12.059	3424	3427	3428	rBV2	230	130	0.01%	0.002%
71	12.371	3522	3524	3526	rBV	271	138	0.02%	0.002%
72	12.387	3526	3529	3531	rVV2	274	168	0.02%	0.003%
73	12.451	3546	3549	3551	rBV2	281	162	0.02%	0.003%
74	12.506	3563	3566	3567	rBV2	313	201	0.02%	0.003%
75	12.631	3603	3605	3609	rBB	286	168	0.02%	0.003%
76	12.699	3621	3626	3628	rBV	256	226	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033337.D
 Acq On : 14 Dec 2023 15:59
 Operator : SY/MD
 Sample : 05794-03
 Misc : 4.12g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.760	3641	3645	3648	rBV	171	162	0.02%	0.003%
78	12.799	3655	3657	3661	rVB2	428	199	0.02%	0.003%
79	12.856	3672	3675	3679	rBV	307	345	0.04%	0.005%
80	12.895	3685	3687	3692	rBB3	375	338	0.04%	0.005%
81	12.937	3695	3700	3703	rBB	368	272	0.03%	0.004%
82	12.972	3707	3711	3713	rBV	302	218	0.02%	0.003%
83	13.046	3731	3734	3736	rBV2	254	201	0.02%	0.003%
84	13.104	3746	3752	3755	rBB2	385	409	0.05%	0.006%
85	13.127	3756	3759	3760	rBV	267	156	0.02%	0.002%
86	13.316	3814	3818	3823	rBV2	388	436	0.05%	0.007%
87	13.339	3823	3825	3827	rVV	290	158	0.02%	0.002%
88	13.400	3842	3844	3846	rBV	347	171	0.02%	0.003%
89	13.461	3857	3863	3867	rBV3	680	817	0.09%	0.013%
90	13.602	3905	3907	3910	rBV2	393	275	0.03%	0.004%
91	13.728	3943	3946	3948	rBB	249	139	0.02%	0.002%
92	13.831	3976	3978	3980	rBV	332	170	0.02%	0.003%
93	13.847	3980	3983	3986	rBV	641	405	0.05%	0.006%
94	13.946	4011	4014	4017	rBV2	240	197	0.02%	0.003%
95	14.014	4032	4035	4036	rBV2	512	220	0.03%	0.003%
96	14.075	4051	4054	4061	rBV2	514	501	0.06%	0.008%
97	14.130	4068	4071	4073	rBV	392	336	0.04%	0.005%
98	14.178	4084	4086	4088	rBV	357	201	0.02%	0.003%
99	14.217	4095	4098	4100	rBV	611	353	0.04%	0.006%
100	14.271	4112	4115	4116	rBV3	484	186	0.02%	0.003%




Sum of corrected areas: 6365064

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033337.D
Acq On : 14 Dec 2023 15:59
Operator : SY/MD
Sample : 05794-03
Misc : 4.12g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

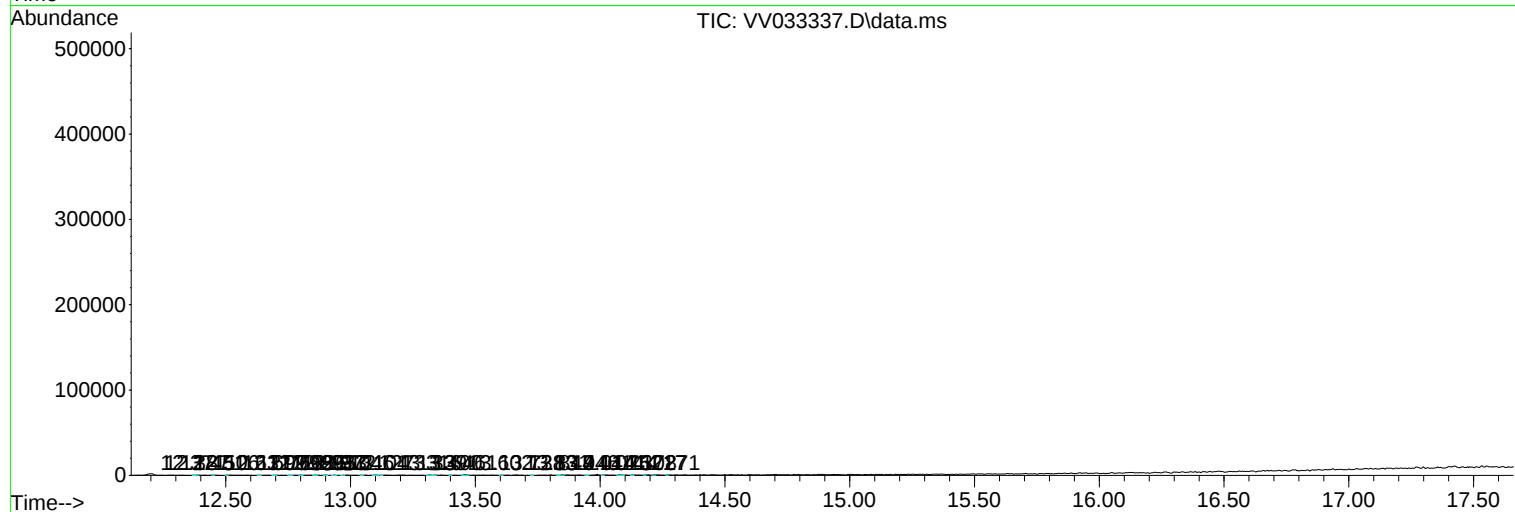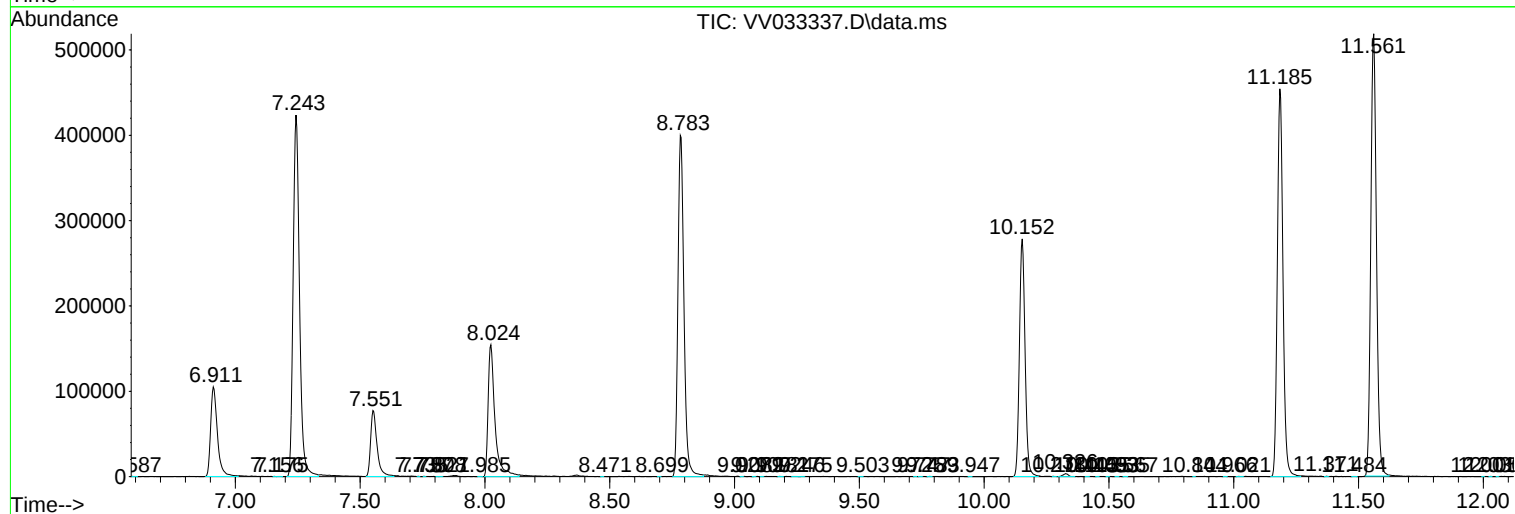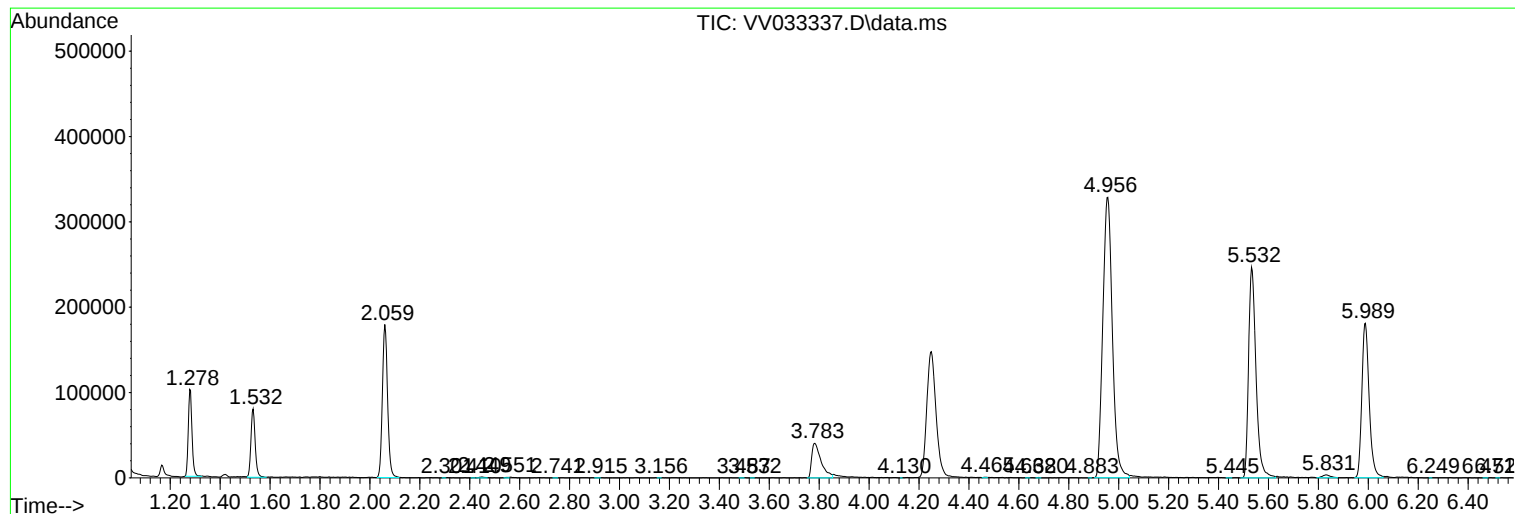

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033337.D
Acq On : 14 Dec 2023 15:59
Operator : SY/MD
Sample : 05794-03
Misc : 4.12g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033337.D
Acq On : 14 Dec 2023 15:59
Operator : SY/MD
Sample : 05794-03
Misc : 4.12g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRF9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------