

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033344.D
 Acq On : 14 Dec 2023 18:41
 Operator : SY/MD
 Sample : 05794-11
 Misc : 4.26g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3Q6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033344.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	92872	95316	11.74%	1.627%
2	1.529	146	152	167	rVB	72319	86367	10.64%	1.474%
3	2.005	299	300	303	rBV	233	144	0.02%	0.002%
4	2.021	303	305	306	rVV	515	176	0.02%	0.003%
5	2.060	308	317	333	rVB	162776	233653	28.78%	3.988%
6	2.146	340	344	346	rBV	197	137	0.02%	0.002%
7	2.301	389	392	395	rBV2	297	218	0.03%	0.004%
8	2.452	430	439	445	rBV3	1056	1762	0.22%	0.030%
9	2.555	465	471	472	rBV3	593	466	0.06%	0.008%
10	2.799	545	547	551	rBB	175	130	0.02%	0.002%
11	2.960	594	597	600	rBV2	228	153	0.02%	0.003%
12	3.146	653	655	658	rBV	146	126	0.02%	0.002%
13	3.545	777	779	781	rBB	315	163	0.02%	0.003%
14	3.786	846	854	887	rBV2	41208	118071	14.54%	2.015%
15	4.600	1105	1107	1111	rBV3	299	216	0.03%	0.004%
16	4.690	1132	1135	1138	rBB2	256	206	0.03%	0.004%
17	4.735	1144	1149	1152	rBV2	259	289	0.04%	0.005%
18	4.957	1200	1218	1249	rBV2	305661	811782	100.00%	13.854%
19	5.468	1374	1377	1379	rBB2	249	137	0.02%	0.002%
20	5.490	1380	1384	1385	rBV	272	205	0.03%	0.003%
21	5.532	1386	1397	1432	rVV	215287	450503	55.50%	7.688%
22	5.889	1507	1508	1512	rBV	346	206	0.03%	0.004%
23	5.928	1517	1520	1525	rVB2	229	180	0.02%	0.003%
24	5.986	1525	1538	1560	rBV	164255	339506	41.82%	5.794%
25	6.195	1599	1603	1606	rBB2	329	230	0.03%	0.004%
26	6.211	1606	1608	1611	rBB	214	130	0.02%	0.002%
27	6.304	1634	1637	1639	rBB	283	175	0.02%	0.003%
28	6.330	1641	1645	1648	rBB	246	181	0.02%	0.003%
29	6.452	1680	1683	1688	rBB	171	180	0.02%	0.003%
30	6.735	1769	1771	1775	rBB	250	136	0.02%	0.002%
31	6.776	1776	1784	1787	rBB	173	280	0.03%	0.005%
32	6.802	1790	1792	1795	rBB	291	139	0.02%	0.002%
33	6.912	1816	1826	1854	rBV	94891	181328	22.34%	3.095%
34	7.185	1908	1911	1913	rBV	293	195	0.02%	0.003%
35	7.243	1918	1929	1957	rBV	390205	686466	84.56%	11.715%
36	7.551	2016	2025	2046	rBV	72562	129992	16.01%	2.218%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033344.D
 Acq On : 14 Dec 2023 18:41
 Operator : SY/MD
 Sample : 05794-11
 Misc : 4.26g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3Q6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	7.728	2078	2080	2081	rBV	286	141	0.02%	0.002%
38	7.992	2159	2162	2163	rBV	258	142	0.02%	0.002%
39	8.024	2163	2172	2210	rBV	160150	300823	37.06%	5.134%
40	8.320	2261	2264	2266	rBV	239	185	0.02%	0.003%
41	8.468	2306	2310	2313	rBB	219	166	0.02%	0.003%
42	8.558	2335	2338	2340	rBB	402	209	0.03%	0.004%
43	8.583	2343	2346	2347	rBV	351	160	0.02%	0.003%
44	8.747	2393	2397	2398	rBV2	242	178	0.02%	0.003%
45	8.783	2398	2408	2431	rBV	353848	580729	71.54%	9.911%
46	9.037	2483	2487	2490	rBB	205	187	0.02%	0.003%
47	9.153	2520	2523	2525	rBV2	268	199	0.02%	0.003%
48	9.239	2548	2550	2556	rBB2	238	225	0.03%	0.004%
49	9.381	2591	2594	2595	rBV2	227	147	0.02%	0.003%
50	9.442	2607	2613	2615	rBV2	258	261	0.03%	0.004%
51	9.490	2624	2628	2633	rBV2	258	301	0.04%	0.005%
52	9.593	2656	2660	2662	rBV	162	145	0.02%	0.002%
53	9.699	2691	2693	2696	rBB	219	130	0.02%	0.002%
54	9.767	2711	2714	2719	rBV	135	190	0.02%	0.003%
55	9.860	2741	2743	2747	rBB	257	193	0.02%	0.003%
56	9.889	2750	2752	2755	rBV	269	161	0.02%	0.003%
57	9.985	2780	2782	2784	rBV	293	189	0.02%	0.003%
58	10.104	2816	2819	2822	rBB2	325	247	0.03%	0.004%
59	10.153	2822	2834	2862	rBV	264259	418283	51.53%	7.139%
60	10.320	2881	2886	2887	rBV	2242	1581	0.19%	0.027%
61	10.590	2966	2970	2973	rBV2	298	257	0.03%	0.004%
62	10.645	2980	2987	2991	rBV	179	298	0.04%	0.005%
63	10.776	3024	3028	3031	rBV	262	177	0.02%	0.003%
64	10.789	3031	3032	3035	rVB	344	139	0.02%	0.002%
65	10.895	3062	3065	3067	rBV	263	183	0.02%	0.003%
66	10.998	3095	3097	3099	rBV	334	159	0.02%	0.003%
67	11.185	3144	3155	3178	rBV	409486	634314	78.14%	10.825%
68	11.458	3234	3240	3242	rBB2	430	236	0.03%	0.004%
69	11.474	3242	3245	3246	rBV2	289	157	0.02%	0.003%
70	11.561	3259	3272	3291	rBV	495605	771221	95.00%	13.162%
71	11.715	3318	3320	3322	rBV	455	160	0.02%	0.003%
72	11.747	3327	3330	3335	rBV	412	371	0.05%	0.006%
73	11.879	3368	3371	3374	rBB	279	243	0.03%	0.004%
74	11.937	3386	3389	3392	rBB	192	157	0.02%	0.003%
75	11.969	3396	3399	3402	rBB	359	175	0.02%	0.003%
76	12.120	3443	3446	3448	rBV	239	194	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033344.D
 Acq On : 14 Dec 2023 18:41
 Operator : SY/MD
 Sample : 05794-11
 Misc : 4.26g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3Q6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.246	3483	3485	3489	rBB	253	140	0.02%	0.002%
78	12.580	3586	3589	3592	rBV	242	172	0.02%	0.003%
79	12.718	3630	3632	3634	rBB	276	139	0.02%	0.002%
80	12.828	3662	3666	3671	rBB	199	204	0.03%	0.003%
81	12.850	3672	3673	3675	rBV	341	153	0.02%	0.003%
82	12.918	3690	3694	3698	rBV2	353	332	0.04%	0.006%
83	12.953	3702	3705	3710	rBB2	272	211	0.03%	0.004%
84	13.111	3752	3754	3757	rBB	374	183	0.02%	0.003%
85	13.278	3803	3806	3808	rBV	181	153	0.02%	0.003%
86	13.326	3819	3821	3823	rVB	325	135	0.02%	0.002%
87	13.378	3835	3837	3841	rBV2	415	313	0.04%	0.005%
88	13.490	3870	3872	3879	rVB2	461	451	0.06%	0.008%
89	13.535	3883	3886	3892	rBB	342	274	0.03%	0.005%
90	13.564	3893	3895	3897	rBV	226	132	0.02%	0.002%
91	13.580	3897	3900	3902	rVB2	399	220	0.03%	0.004%
92	13.596	3902	3905	3907	rBV	467	303	0.04%	0.005%
93	13.638	3916	3918	3924	rBV2	464	471	0.06%	0.008%
94	13.886	3993	3995	3997	rBV	272	157	0.02%	0.003%
95	13.931	4006	4009	4010	rBV2	355	183	0.02%	0.003%
96	14.017	4034	4036	4038	rBV2	371	212	0.03%	0.004%
97	14.233	4101	4103	4105	rBV	349	172	0.02%	0.003%
98	14.358	4138	4142	4143	rBV	425	288	0.04%	0.005%
99	14.458	4170	4173	4180	rBV3	743	899	0.11%	0.015%
100	14.519	4188	4192	4194	rBV2	497	432	0.05%	0.007%




Sum of corrected areas: 5859486

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033344.D
Acq On : 14 Dec 2023 18:41
Operator : SY/MD
Sample : 05794-11
Misc : 4.26g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3Q6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

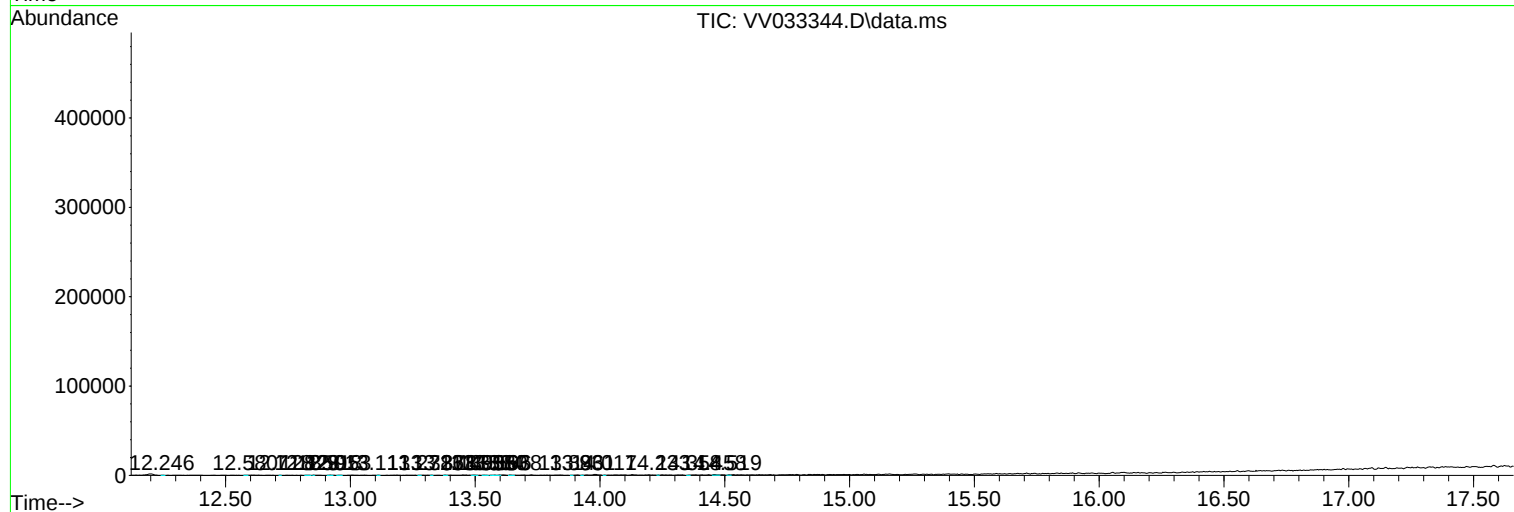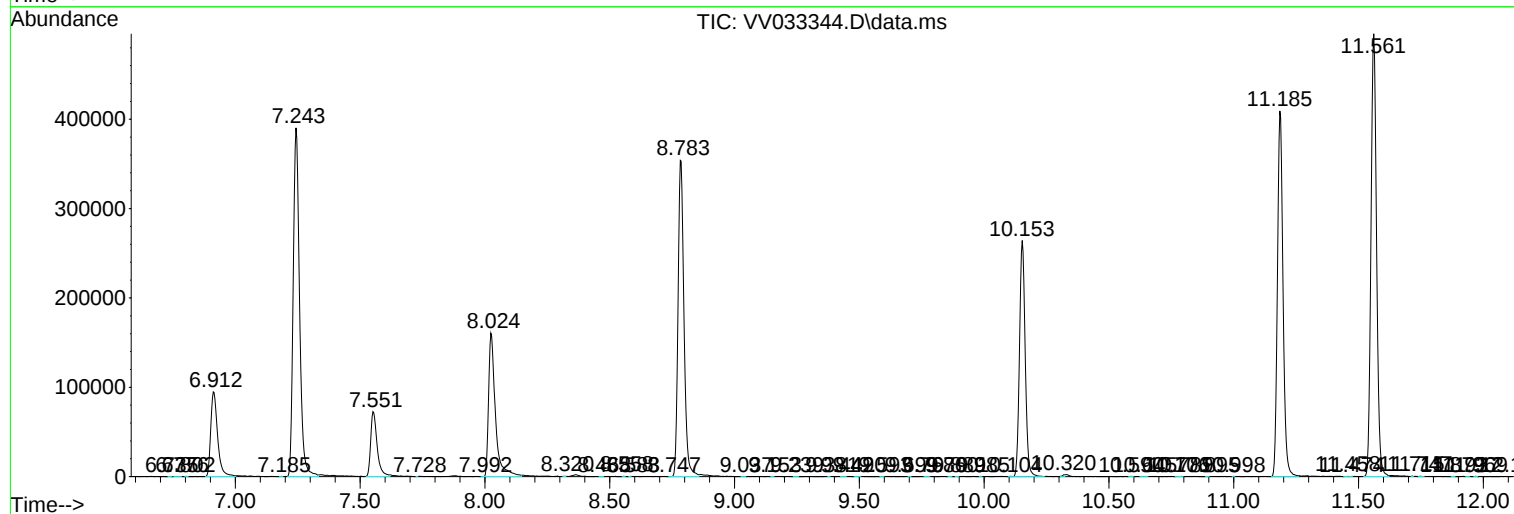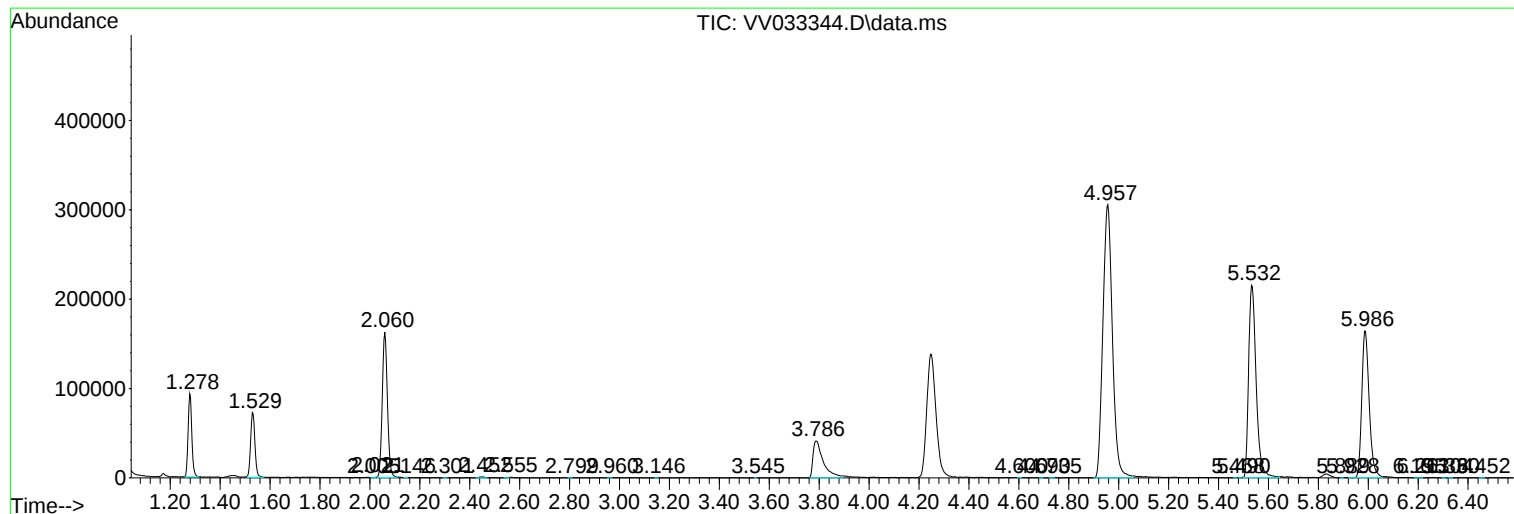

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033344.D
Acq On : 14 Dec 2023 18:41
Operator : SY/MD
Sample : 05794-11
Misc : 4.26g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3Q6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033344.D
Acq On : 14 Dec 2023 18:41
Operator : SY/MD
Sample : 05794-11
Misc : 4.26g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3Q6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------