

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033354.D
 Acq On : 14 Dec 2023 22:56
 Operator : SY/MD
 Sample : 05818-02 50X
 Misc : 4.87g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033354.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	75736	78415	11.58%	1.416%
2	1.532	145	153	166	rBV	62671	72339	10.68%	1.306%
3	1.982	291	293	295	rBV	348	177	0.03%	0.003%
4	2.060	306	317	332	rBV	136873	199568	29.47%	3.603%
5	2.240	371	373	374	rBV	270	146	0.02%	0.003%
6	2.558	461	472	487	rBB	4878	9139	1.35%	0.165%
7	2.767	534	537	541	rBB	165	151	0.02%	0.003%
8	2.921	582	585	589	rBB	188	172	0.03%	0.003%
9	2.976	598	602	606	rBB	136	165	0.02%	0.003%
10	3.053	623	626	630	rBB2	227	173	0.03%	0.003%
11	3.307	702	705	708	rBB	178	132	0.02%	0.002%
12	3.474	754	757	760	rBV	169	163	0.02%	0.003%
13	3.783	845	853	889	rBV2	34914	95073	14.04%	1.717%
14	4.095	948	950	953	rBV	270	183	0.03%	0.003%
15	4.249	981	998	1029	rBV2	114309	298668	44.10%	5.392%
16	4.561	1092	1095	1098	rBV2	286	225	0.03%	0.004%
17	4.606	1103	1109	1113	rBV2	365	394	0.06%	0.007%
18	4.645	1118	1121	1124	rBB	226	172	0.03%	0.003%
19	4.802	1167	1170	1174	rBV	152	168	0.02%	0.003%
20	4.818	1174	1175	1179	rVB	238	127	0.02%	0.002%
21	4.889	1194	1197	1200	rBB	154	131	0.02%	0.002%
22	4.957	1201	1218	1255	rBV2	250515	677232	100.00%	12.227%
23	5.349	1337	1340	1341	rBV	369	221	0.03%	0.004%
24	5.477	1378	1380	1384	rBV2	251	213	0.03%	0.004%
25	5.532	1386	1397	1423	rBV	222986	462131	68.24%	8.344%
26	5.918	1514	1517	1519	rBV	272	206	0.03%	0.004%
27	5.989	1527	1539	1563	rBV	136206	280641	41.44%	5.067%
28	6.207	1600	1607	1611	rBB3	407	470	0.07%	0.008%
29	6.233	1612	1615	1618	rBV	330	197	0.03%	0.004%
30	6.288	1630	1632	1634	rBB	256	132	0.02%	0.002%
31	6.911	1816	1826	1854	rBV	79843	153383	22.65%	2.769%
32	7.175	1899	1908	1917	rBB4	2208	3969	0.59%	0.072%
33	7.243	1917	1929	1955	rBV	324060	575434	84.97%	10.389%
34	7.510	2010	2012	2016	rBV	376	303	0.04%	0.005%
35	7.551	2016	2025	2053	rVV	61661	110598	16.33%	1.997%
36	7.870	2118	2124	2125	rBV	908	624	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033354.D
 Acq On : 14 Dec 2023 22:56
 Operator : SY/MD
 Sample : 05818-02 50X
 Misc : 4.87g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	7.979	2156	2158	2160	rBB	314	121	0.02%	0.002%
38	8.024	2163	2172	2197	rBV	128707	237617	35.09%	4.290%
39	8.310	2258	2261	2263	rBV2	289	227	0.03%	0.004%
40	8.452	2302	2305	2308	rBB	251	136	0.02%	0.002%
41	8.635	2358	2362	2364	rBV	172	160	0.02%	0.003%
42	8.786	2398	2409	2436	rBV	361443	595306	87.90%	10.748%
43	9.024	2481	2483	2485	rBB	271	143	0.02%	0.003%
44	9.046	2488	2490	2493	rBV	140	119	0.02%	0.002%
45	9.178	2529	2531	2534	rBB	217	144	0.02%	0.003%
46	9.246	2549	2552	2555	rBB2	268	192	0.03%	0.003%
47	9.358	2585	2587	2590	rBV	154	135	0.02%	0.002%
48	9.596	2657	2661	2663	rBB	175	142	0.02%	0.003%
49	9.657	2676	2680	2685	rBB	160	181	0.03%	0.003%
50	9.709	2693	2696	2698	rBV	228	133	0.02%	0.002%
51	9.857	2739	2742	2744	rBV	163	133	0.02%	0.002%
52	9.879	2746	2749	2752	rVB	305	191	0.03%	0.003%
53	10.017	2789	2792	2794	rBB2	256	139	0.02%	0.003%
54	10.153	2823	2834	2852	rBV	226190	354791	52.39%	6.406%
55	10.326	2879	2888	2897	rBB4	3179	4660	0.69%	0.084%
56	10.378	2902	2904	2907	rBB	300	177	0.03%	0.003%
57	10.493	2936	2940	2942	rBB	154	126	0.02%	0.002%
58	10.506	2942	2944	2947	rBV	152	117	0.02%	0.002%
59	10.593	2969	2971	2974	rBV	134	114	0.02%	0.002%
60	10.802	3034	3036	3039	rBB2	273	143	0.02%	0.003%
61	10.850	3049	3051	3053	rBV	168	115	0.02%	0.002%
62	10.937	3074	3078	3080	rBB	232	145	0.02%	0.003%
63	11.034	3107	3108	3111	rBV	228	122	0.02%	0.002%
64	11.133	3136	3139	3140	rBV	246	141	0.02%	0.003%
65	11.185	3144	3155	3180	rBV	414625	653052	96.43%	11.791%
66	11.458	3237	3240	3241	rBV	210	134	0.02%	0.002%
67	11.561	3259	3272	3291	rBV	412649	657132	97.03%	11.864%
68	11.792	3343	3344	3348	rBV	224	152	0.02%	0.003%
69	12.005	3407	3410	3413	rBB2	262	171	0.03%	0.003%
70	12.197	3462	3470	3478	rVB5	2133	3139	0.46%	0.057%
71	12.252	3485	3487	3492	rBB	255	170	0.03%	0.003%
72	12.326	3507	3510	3513	rBV	233	208	0.03%	0.004%
73	12.378	3524	3526	3529	rBV2	297	211	0.03%	0.004%
74	12.419	3536	3539	3541	rBV	251	143	0.02%	0.003%
75	12.535	3571	3575	3578	rBB	229	199	0.03%	0.004%
76	12.622	3600	3602	3606	rBB	173	147	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033354.D
 Acq On : 14 Dec 2023 22:56
 Operator : SY/MD
 Sample : 05818-02 50X
 Misc : 4.87g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGRG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.673	3613	3618	3621	rBV	230	231	0.03%	0.004%
78	12.869	3677	3679	3681	rBB	262	118	0.02%	0.002%
79	13.005	3717	3721	3724	rBV	245	204	0.03%	0.004%
80	13.037	3727	3731	3733	rBV	347	239	0.04%	0.004%
81	13.095	3746	3749	3751	rBB2	252	137	0.02%	0.002%
82	13.143	3763	3764	3769	rBB	308	182	0.03%	0.003%
83	13.213	3781	3786	3793	rBB3	650	700	0.10%	0.013%
84	13.307	3812	3815	3818	rBB	258	166	0.02%	0.003%
85	13.323	3818	3820	3823	rBV	351	187	0.03%	0.003%
86	13.355	3826	3830	3832	rBB	393	228	0.03%	0.004%
87	13.377	3833	3837	3840	rBV2	290	239	0.04%	0.004%
88	13.442	3854	3857	3858	rBV	227	152	0.02%	0.003%
89	13.609	3905	3909	3912	rBV2	302	281	0.04%	0.005%
90	13.824	3973	3976	3979	rBB	202	157	0.02%	0.003%
91	13.885	3991	3995	3997	rBV	246	183	0.03%	0.003%
92	13.921	4004	4006	4009	rBV2	374	190	0.03%	0.003%
93	14.046	4042	4045	4047	rBV	403	278	0.04%	0.005%
94	14.130	4067	4071	4073	rBV2	343	279	0.04%	0.005%
95	14.223	4097	4100	4103	rVB	485	325	0.05%	0.006%
96	14.262	4104	4112	4113	rBV2	583	664	0.10%	0.012%
97	14.291	4117	4121	4122	rBV2	379	277	0.04%	0.005%
98	14.355	4139	4141	4143	rBV	392	189	0.03%	0.003%
99	14.410	4152	4158	4161	rBV2	561	514	0.08%	0.009%
100	14.561	4203	4205	4208	rVB	540	195	0.03%	0.004%

Sum of corrected areas: 5538678




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033354.D
Acq On : 14 Dec 2023 22:56
Operator : SY/MD
Sample : 05818-02 50X
Misc : 4.87g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

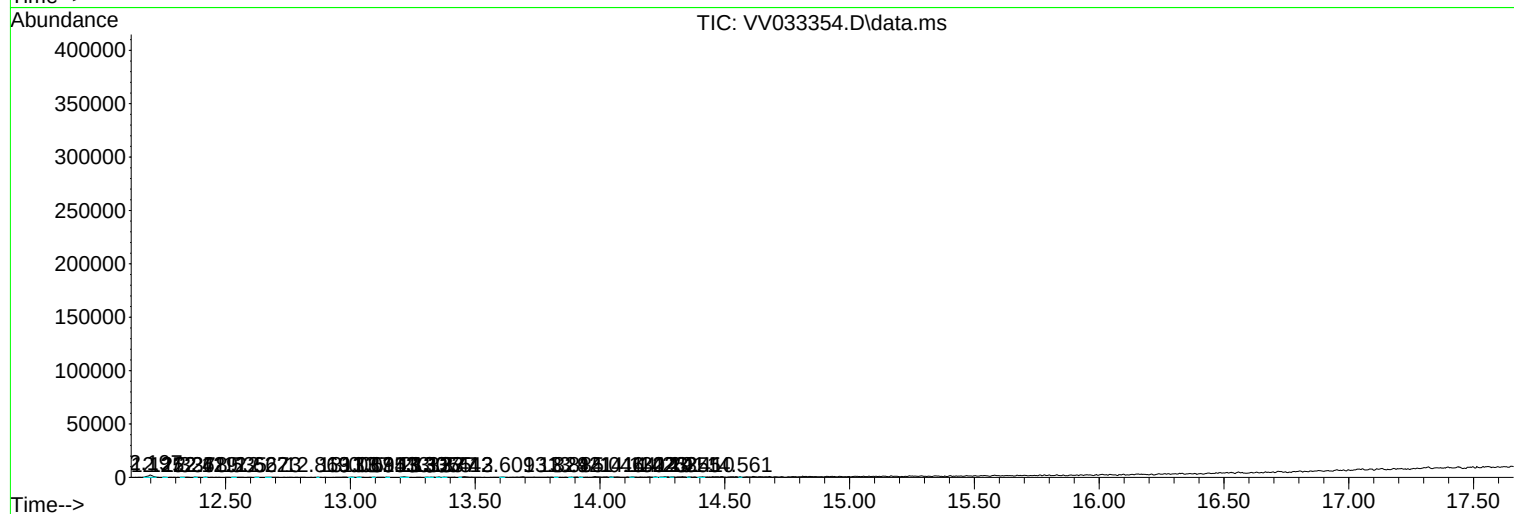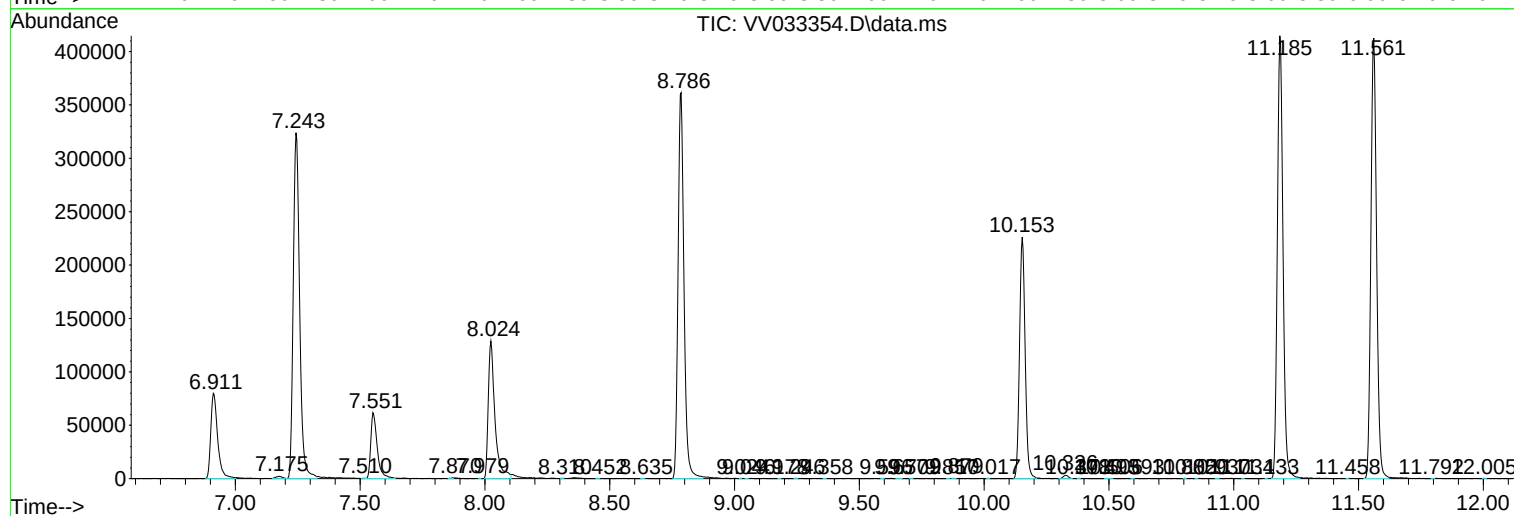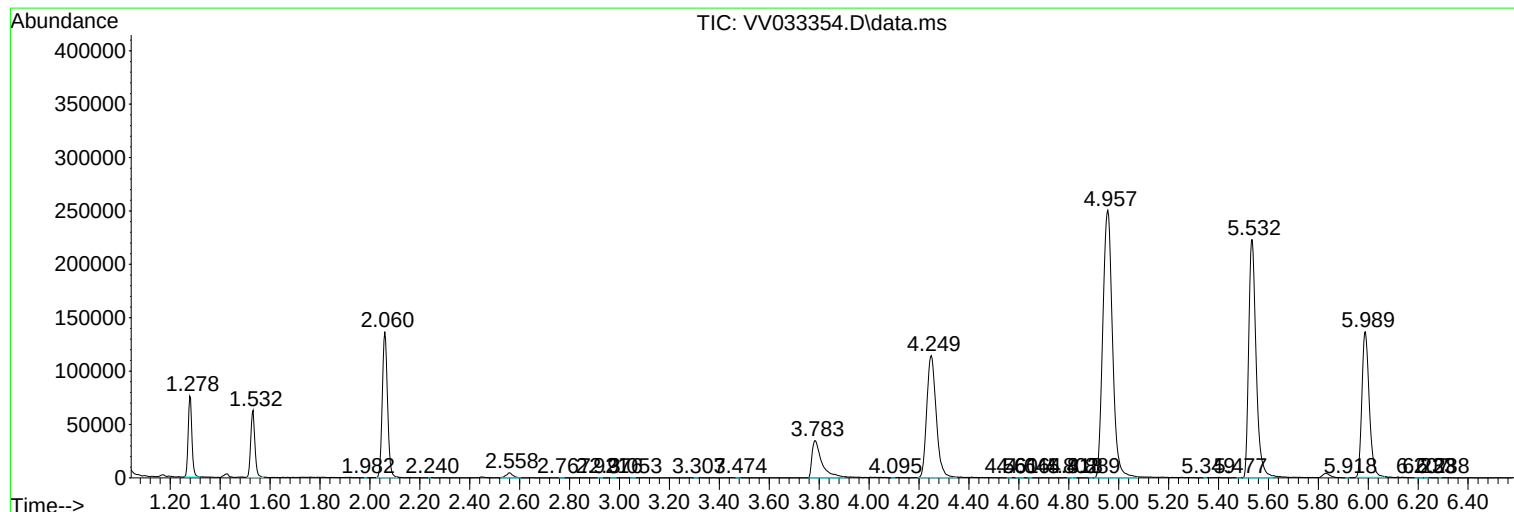

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033354.D
Acq On : 14 Dec 2023 22:56
Operator : SY/MD
Sample : 05818-02 50X
Misc : 4.87g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033354.D
Acq On : 14 Dec 2023 22:56
Operator : SY/MD
Sample : 05818-02 50X
Misc : 4.87g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGRG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc