

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033357.D
 Acq On : 15 Dec 2023 00:05
 Operator : SY/MD
 Sample : 05807-08 100X
 Misc : 1.94g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033357.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	81948	79957	11.53%	1.398%
2	1.532	146	153	171	rVB	60338	73374	10.58%	1.283%
3	1.983	289	293	295	rBV	249	175	0.03%	0.003%
4	2.060	306	317	332	rBV	137651	202262	29.16%	3.537%
5	2.143	342	343	347	rVB	468	202	0.03%	0.004%
6	2.246	373	375	378	rBV	212	137	0.02%	0.002%
7	2.288	385	388	391	rBB	188	144	0.02%	0.003%
8	2.449	433	438	444	rBB	857	979	0.14%	0.017%
9	2.552	463	470	473	rBV	872	1052	0.15%	0.018%
10	3.783	843	853	891	rBV2	36274	102373	14.76%	1.790%
11	4.108	950	954	955	rBV	450	273	0.04%	0.005%
12	4.156	964	969	973	rBB	354	351	0.05%	0.006%
13	4.182	974	977	981	rBB2	300	233	0.03%	0.004%
14	4.246	981	997	1022	rBV2	119031	305362	44.03%	5.341%
15	4.500	1073	1076	1078	rBB	273	167	0.02%	0.003%
16	4.519	1079	1082	1083	rBV	349	169	0.02%	0.003%
17	4.896	1196	1199	1201	rBB	215	107	0.02%	0.002%
18	4.957	1201	1218	1244	rBV2	259737	693528	100.00%	12.129%
19	5.253	1306	1310	1314	rBV3	594	505	0.07%	0.009%
20	5.346	1332	1339	1343	rBV	405	553	0.08%	0.010%
21	5.391	1349	1353	1354	rBB	316	166	0.02%	0.003%
22	5.452	1369	1372	1375	rBV2	217	151	0.02%	0.003%
23	5.532	1386	1397	1425	rBV	218387	449585	64.83%	7.863%
24	5.989	1526	1539	1559	rBV2	137670	289421	41.73%	5.062%
25	6.146	1585	1588	1590	rVB3	767	421	0.06%	0.007%
26	6.298	1633	1635	1640	rBB	255	161	0.02%	0.003%
27	6.912	1816	1826	1855	rBV	83121	156590	22.58%	2.739%
28	7.124	1888	1892	1893	rBB	321	145	0.02%	0.003%
29	7.159	1899	1903	1905	rBV2	430	353	0.05%	0.006%
30	7.243	1915	1929	1954	rBV	330104	586087	84.51%	10.250%
31	7.551	2015	2025	2048	rBV2	61950	113079	16.30%	1.978%
32	7.712	2072	2075	2079	rVB2	442	308	0.04%	0.005%
33	7.735	2080	2082	2083	rBV2	242	116	0.02%	0.002%
34	7.812	2103	2106	2107	rBV2	221	113	0.02%	0.002%
35	7.857	2117	2120	2121	rBV	378	174	0.03%	0.003%
36	8.024	2163	2172	2202	rBV	133264	251028	36.20%	4.390%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033357.D
 Acq On : 15 Dec 2023 00:05
 Operator : SY/MD
 Sample : 05807-08 100X
 Misc : 1.94g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	8.359	2268	2276	2287	rBV2	1230	2548	0.37%	0.045%
38	8.497	2317	2319	2321	rBB	241	110	0.02%	0.002%
39	8.783	2398	2408	2438	rBV2	360676	679916	98.04%	11.891%
40	9.002	2472	2476	2478	rBB	231	113	0.02%	0.002%
41	9.031	2479	2485	2489	rBV2	305	337	0.05%	0.006%
42	9.236	2544	2549	2551	rBV2	269	246	0.04%	0.004%
43	9.323	2573	2576	2578	rBB	196	118	0.02%	0.002%
44	9.394	2595	2598	2601	rBB2	232	137	0.02%	0.002%
45	9.510	2631	2634	2635	rBV	253	136	0.02%	0.002%
46	9.680	2684	2687	2688	rBV	240	123	0.02%	0.002%
47	9.876	2746	2748	2750	rBV	245	151	0.02%	0.003%
48	10.153	2823	2834	2855	rBV2	236442	368380	53.12%	6.443%
49	10.256	2864	2866	2869	rBB2	297	158	0.02%	0.003%
50	10.326	2880	2888	2898	rBB3	3146	4873	0.70%	0.085%
51	10.381	2903	2905	2908	rBB	255	126	0.02%	0.002%
52	10.751	3017	3020	3022	rBB	272	124	0.02%	0.002%
53	10.940	3075	3079	3081	rBV	147	142	0.02%	0.002%
54	11.101	3126	3129	3131	rBB	259	158	0.02%	0.003%
55	11.124	3133	3136	3138	rBV	464	298	0.04%	0.005%
56	11.185	3144	3155	3179	rBV	420004	659808	95.14%	11.539%
57	11.445	3234	3236	3240	rBB	176	128	0.02%	0.002%
58	11.490	3248	3250	3252	rVB	277	108	0.02%	0.002%
59	11.561	3260	3272	3298	rBV	434712	678184	97.79%	11.861%
60	11.709	3314	3318	3321	rVB2	450	332	0.05%	0.006%
61	11.841	3356	3359	3360	rBB	333	111	0.02%	0.002%
62	11.876	3366	3370	3371	rBB	224	128	0.02%	0.002%
63	11.924	3383	3385	3387	rBB	244	110	0.02%	0.002%
64	11.966	3396	3398	3401	rBV	167	137	0.02%	0.002%
65	11.979	3401	3402	3405	rVB	347	142	0.02%	0.002%
66	12.165	3456	3460	3461	rBV	343	176	0.03%	0.003%
67	12.194	3463	3469	3477	rVB2	1732	2487	0.36%	0.043%
68	12.448	3546	3548	3552	rBB2	337	181	0.03%	0.003%
69	12.522	3569	3571	3574	rBV	179	138	0.02%	0.002%
70	12.558	3579	3582	3585	rBB	139	125	0.02%	0.002%
71	12.606	3593	3597	3599	rBB	137	112	0.02%	0.002%
72	12.635	3604	3606	3610	rBB	214	130	0.02%	0.002%
73	12.670	3614	3617	3619	rBV	140	116	0.02%	0.002%
74	12.735	3634	3637	3638	rBV	206	126	0.02%	0.002%
75	12.850	3671	3673	3675	rBV	269	126	0.02%	0.002%
76	12.972	3709	3711	3713	rBV	234	114	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033357.D
 Acq On : 15 Dec 2023 00:05
 Operator : SY/MD
 Sample : 05807-08 100X
 Misc : 1.94g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.995	3715	3718	3719	rBV	145	105	0.02%	0.002%
78	13.066	3738	3740	3742	rBB	261	123	0.02%	0.002%
79	13.169	3769	3772	3774	rBV	249	183	0.03%	0.003%
80	13.214	3783	3786	3789	rVB2	612	315	0.05%	0.006%
81	13.317	3816	3818	3820	rBB	247	135	0.02%	0.002%
82	13.419	3847	3850	3852	rBB	237	135	0.02%	0.002%
83	13.432	3852	3854	3856	rBV	178	110	0.02%	0.002%
84	13.516	3878	3880	3882	rBB	348	156	0.02%	0.003%
85	13.609	3907	3909	3911	rBV	445	229	0.03%	0.004%
86	13.648	3920	3921	3924	rVB	361	139	0.02%	0.002%
87	13.667	3924	3927	3930	rBB2	355	199	0.03%	0.003%
88	13.844	3980	3982	3984	rBB	360	158	0.02%	0.003%
89	13.860	3985	3987	3989	rBV	432	215	0.03%	0.004%
90	13.905	3999	4001	4004	rBV2	413	339	0.05%	0.006%
91	13.950	4013	4015	4019	rBV2	487	325	0.05%	0.006%
92	13.979	4019	4024	4027	rBV3	606	629	0.09%	0.011%
93	14.072	4050	4053	4057	rBV	293	270	0.04%	0.005%
94	14.117	4065	4067	4070	rBV2	238	158	0.02%	0.003%
95	14.143	4071	4075	4081	rVB2	632	641	0.09%	0.011%
96	14.239	4103	4105	4109	rVB	420	316	0.05%	0.006%
97	14.275	4110	4116	4118	rBV2	626	480	0.07%	0.008%
98	14.339	4132	4136	4140	rBV2	429	443	0.06%	0.008%
99	14.394	4149	4153	4155	rBV	620	474	0.07%	0.008%
100	14.506	4183	4188	4190	rBV2	544	541	0.08%	0.009%




Sum of corrected areas: 5717832

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033357.D
Acq On : 15 Dec 2023 00:05
Operator : SY/MD
Sample : 05807-08 100X
Misc : 1.94g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

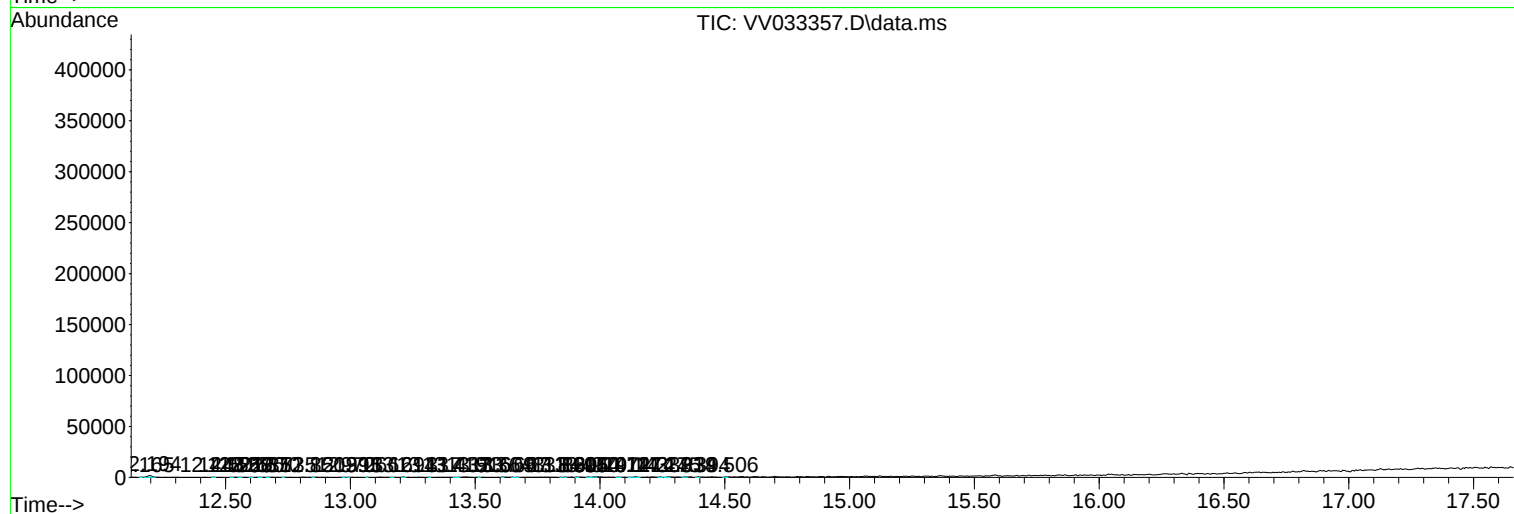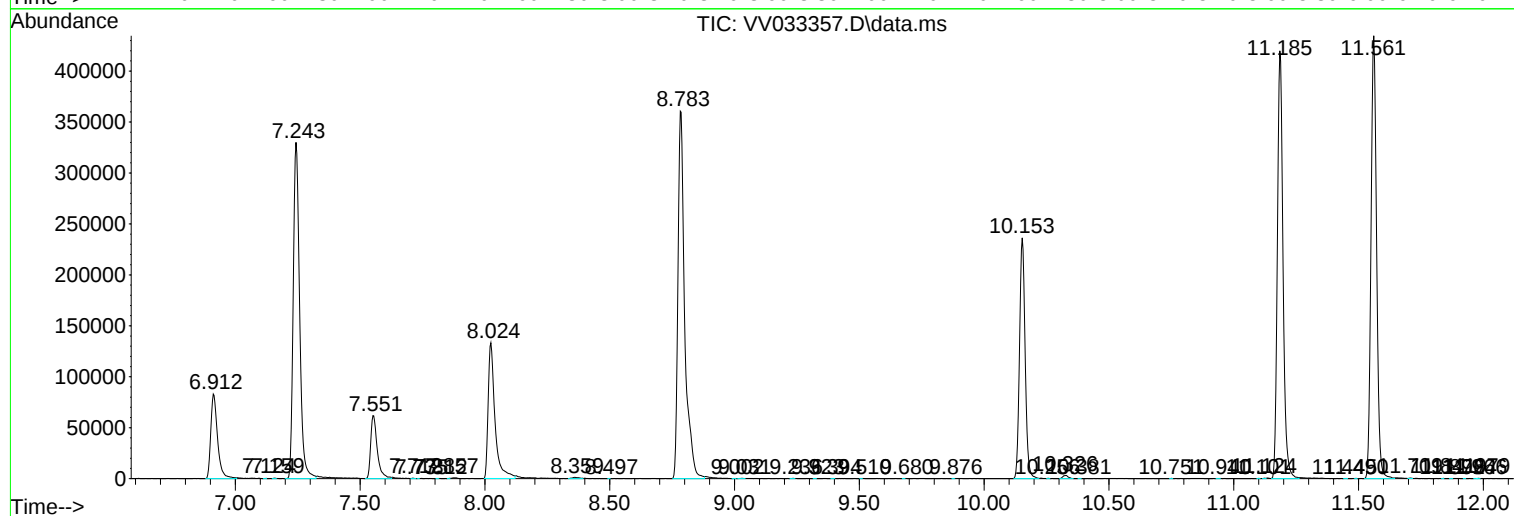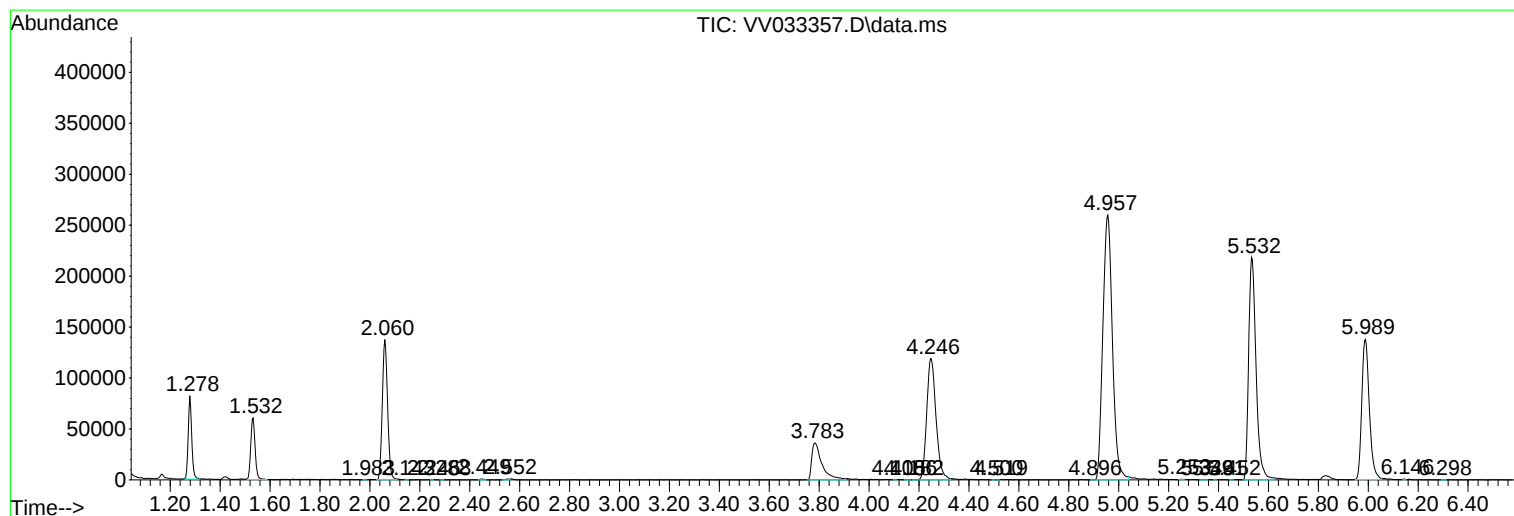

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033357.D
Acq On : 15 Dec 2023 00:05
Operator : SY/MD
Sample : 05807-08 100X
Misc : 1.94g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033357.D
Acq On : 15 Dec 2023 00:05
Operator : SY/MD
Sample : 05807-08 100X
Misc : 1.94g/5.0mL/100uL/5.00mL/MSVOA_V/MEOH
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AY0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc