

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033358.D
 Acq On : 15 Dec 2023 00:29
 Operator : SY/MD
 Sample : 05802-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033358.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.060	307	317	334	rBV	132736	194864	28.82%	3.882%
2	2.304	390	393	395	rBV	346	211	0.03%	0.004%
3	2.346	403	406	407	rBV	223	108	0.02%	0.002%
4	2.449	433	438	442	rBB3	762	666	0.10%	0.013%
5	2.558	463	472	484	rBV2	1663	3423	0.51%	0.068%
6	2.625	491	493	496	rBB	135	96	0.01%	0.002%
7	2.703	515	517	520	rBB	163	109	0.02%	0.002%
8	2.796	543	546	548	rBB	161	111	0.02%	0.002%
9	2.915	581	583	586	rBV	177	137	0.02%	0.003%
10	3.330	708	712	714	rBB	168	135	0.02%	0.003%
11	3.783	845	853	883	rBV	37125	96044	14.21%	1.913%
12	4.140	962	964	965	rBV	380	172	0.03%	0.003%
13	4.185	974	978	981	rBV2	380	340	0.05%	0.007%
14	4.481	1069	1070	1072	rBV	212	96	0.01%	0.002%
15	4.555	1091	1093	1096	rBB	150	102	0.02%	0.002%
16	4.577	1097	1100	1101	rBV	241	143	0.02%	0.003%
17	4.957	1201	1218	1243	rBV3	254477	676033	100.00%	13.468%
18	5.371	1345	1347	1350	rBB3	213	123	0.02%	0.002%
19	5.407	1356	1358	1360	rBV2	248	140	0.02%	0.003%
20	5.471	1375	1378	1383	rBV2	337	320	0.05%	0.006%
21	5.535	1386	1398	1426	rBV	213647	441919	65.37%	8.804%
22	5.921	1513	1518	1520	rBB	376	205	0.03%	0.004%
23	5.937	1521	1523	1525	rBV	271	144	0.02%	0.003%
24	5.989	1527	1539	1568	rBV	136470	286394	42.36%	5.706%
25	6.169	1593	1595	1597	rBV	373	183	0.03%	0.004%
26	6.301	1634	1636	1642	rBB	175	162	0.02%	0.003%
27	6.458	1682	1685	1687	rBB	150	98	0.01%	0.002%
28	6.616	1732	1734	1736	rBV	248	139	0.02%	0.003%
29	6.683	1751	1755	1758	rBV	160	183	0.03%	0.004%
30	6.850	1804	1807	1809	rBB	129	93	0.01%	0.002%
31	6.911	1817	1826	1849	rBV	81369	151618	22.43%	3.021%
32	7.085	1876	1880	1883	rBV	440	361	0.05%	0.007%
33	7.178	1906	1909	1911	rBB	128	91	0.01%	0.002%
34	7.243	1918	1929	1960	rBV	319030	565326	83.62%	11.263%
35	7.554	2016	2026	2045	rBV2	61614	109324	16.17%	2.178%
36	7.805	2100	2104	2106	rBB	245	149	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033358.D
 Acq On : 15 Dec 2023 00:29
 Operator : SY/MD
 Sample : 05802-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	7.879	2114	2127	2139	rBB3	8481	15505	2.29%	0.309%
38	8.024	2163	2172	2200	rBV	131510	252215	37.31%	5.025%
39	8.271	2245	2249	2251	rBV	288	273	0.04%	0.005%
40	8.355	2273	2275	2277	rBB	248	94	0.01%	0.002%
41	8.368	2277	2279	2281	rBV	254	161	0.02%	0.003%
42	8.403	2288	2290	2293	rBB	252	139	0.02%	0.003%
43	8.786	2396	2409	2435	rBV	344641	572838	84.74%	11.412%
44	8.963	2460	2464	2467	rBV	361	361	0.05%	0.007%
45	9.027	2480	2484	2488	rBB3	365	287	0.04%	0.006%
46	9.066	2493	2496	2498	rBB	143	97	0.01%	0.002%
47	9.442	2611	2613	2615	rBB	259	101	0.01%	0.002%
48	9.503	2630	2632	2636	rBB	224	132	0.02%	0.003%
49	9.545	2642	2645	2647	rBB	138	92	0.01%	0.002%
50	9.609	2662	2665	2666	rBB	223	125	0.02%	0.002%
51	9.751	2707	2709	2712	rBB	185	123	0.02%	0.002%
52	9.792	2719	2722	2724	rBB	139	95	0.01%	0.002%
53	10.043	2799	2800	2802	rBV	233	94	0.01%	0.002%
54	10.152	2823	2834	2855	rBV	231725	359879	53.23%	7.170%
55	10.390	2905	2908	2910	rBB	168	106	0.02%	0.002%
56	10.406	2911	2913	2916	rBB	160	102	0.02%	0.002%
57	10.496	2937	2941	2944	rBB	306	228	0.03%	0.005%
58	10.821	3040	3042	3045	rBB	278	170	0.03%	0.003%
59	10.841	3045	3048	3051	rBB	230	159	0.02%	0.003%
60	10.866	3054	3056	3060	rBB	148	95	0.01%	0.002%
61	11.005	3096	3099	3102	rBB2	223	135	0.02%	0.003%
62	11.185	3144	3155	3184	rBV	400549	626363	92.65%	12.479%
63	11.419	3224	3228	3233	rBB2	259	269	0.04%	0.005%
64	11.471	3238	3244	3247	rBV2	365	393	0.06%	0.008%
65	11.500	3250	3253	3255	rBB	245	110	0.02%	0.002%
66	11.561	3260	3272	3289	rBV	415631	650356	96.20%	12.957%
67	11.837	3356	3358	3361	rBV	203	162	0.02%	0.003%
68	11.992	3403	3406	3409	rBV2	238	181	0.03%	0.004%
69	12.049	3423	3424	3428	rBV	235	157	0.02%	0.003%
70	12.194	3461	3469	3477	rBB3	1670	2593	0.38%	0.052%
71	12.239	3480	3483	3486	rBV2	425	279	0.04%	0.006%
72	12.320	3505	3508	3511	rBB	147	121	0.02%	0.002%
73	12.349	3514	3517	3519	rBB	253	146	0.02%	0.003%
74	12.413	3534	3537	3539	rBV2	223	127	0.02%	0.003%
75	12.484	3556	3559	3561	rBV2	268	170	0.03%	0.003%
76	12.522	3568	3571	3574	rBB2	238	164	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033358.D
 Acq On : 15 Dec 2023 00:29
 Operator : SY/MD
 Sample : 05802-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.548	3577	3579	3582	rBB	139	94	0.01%	0.002%
78	12.683	3616	3621	3624	rBB	137	140	0.02%	0.003%
79	12.902	3686	3689	3692	rBB	156	99	0.01%	0.002%
80	12.918	3692	3694	3697	rBB2	370	196	0.03%	0.004%
81	13.027	3725	3728	3731	rBB	146	121	0.02%	0.002%
82	13.053	3734	3736	3739	rBB	248	117	0.02%	0.002%
83	13.249	3794	3797	3801	rBB	175	159	0.02%	0.003%
84	13.303	3812	3814	3816	rBB	275	148	0.02%	0.003%
85	13.339	3822	3825	3827	rBV	374	238	0.04%	0.005%
86	13.387	3838	3840	3845	rBB3	366	255	0.04%	0.005%
87	13.419	3846	3850	3852	rBV2	229	178	0.03%	0.004%
88	13.455	3858	3861	3864	rBV2	398	406	0.06%	0.008%
89	13.503	3873	3876	3878	rBB	241	109	0.02%	0.002%
90	13.529	3882	3884	3887	rBV	260	149	0.02%	0.003%
91	13.570	3895	3897	3899	rBV2	297	185	0.03%	0.004%
92	13.699	3935	3937	3938	rBV	282	133	0.02%	0.003%
93	13.741	3949	3950	3953	rBB	241	100	0.01%	0.002%
94	13.776	3956	3961	3963	rBV2	342	284	0.04%	0.006%
95	13.879	3990	3993	3995	rBB	185	121	0.02%	0.002%
96	13.937	4010	4011	4016	rVB3	501	329	0.05%	0.007%
97	13.969	4016	4021	4022	rBV	403	367	0.05%	0.007%
98	14.030	4038	4040	4042	rBV2	426	224	0.03%	0.004%
99	14.133	4069	4072	4074	rBB2	230	117	0.02%	0.002%
100	14.178	4081	4086	4088	rBV2	300	285	0.04%	0.006%




Sum of corrected areas: 5019513

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033358.D
Acq On : 15 Dec 2023 00:29
Operator : SY/MD
Sample : 05802-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

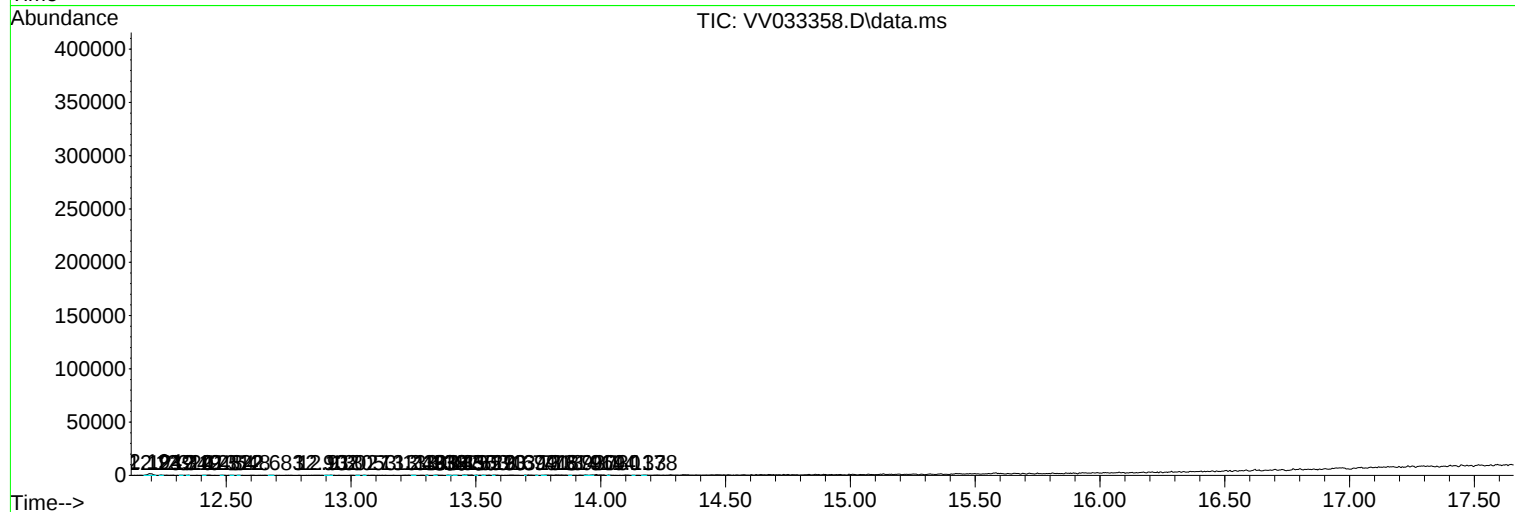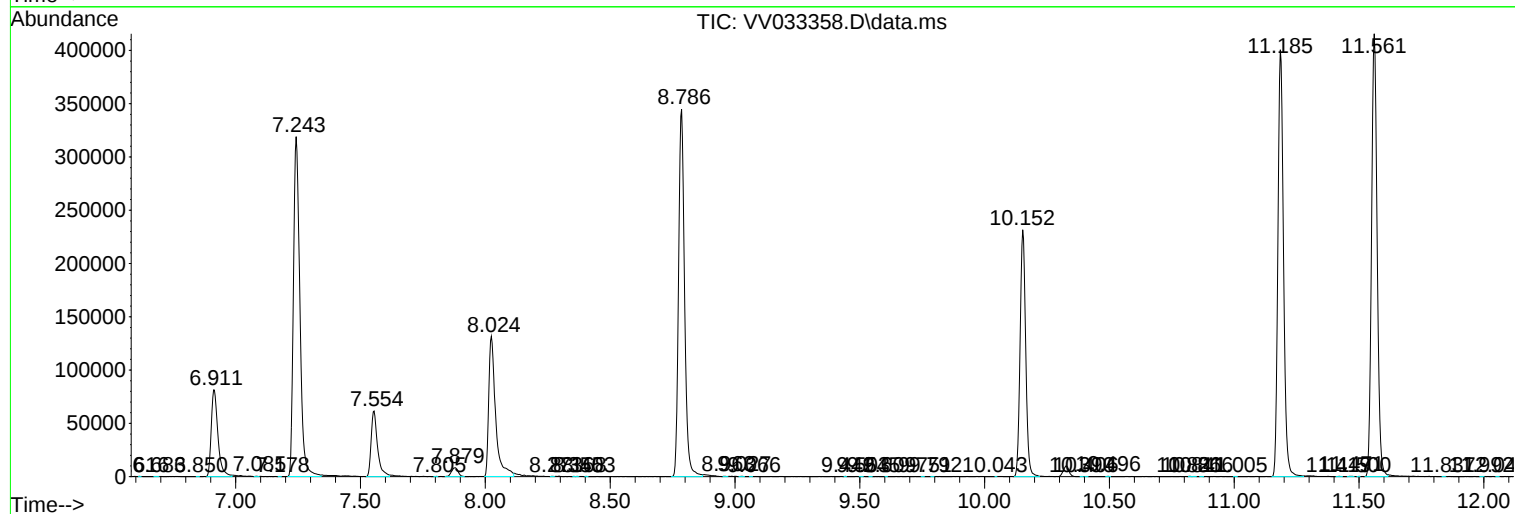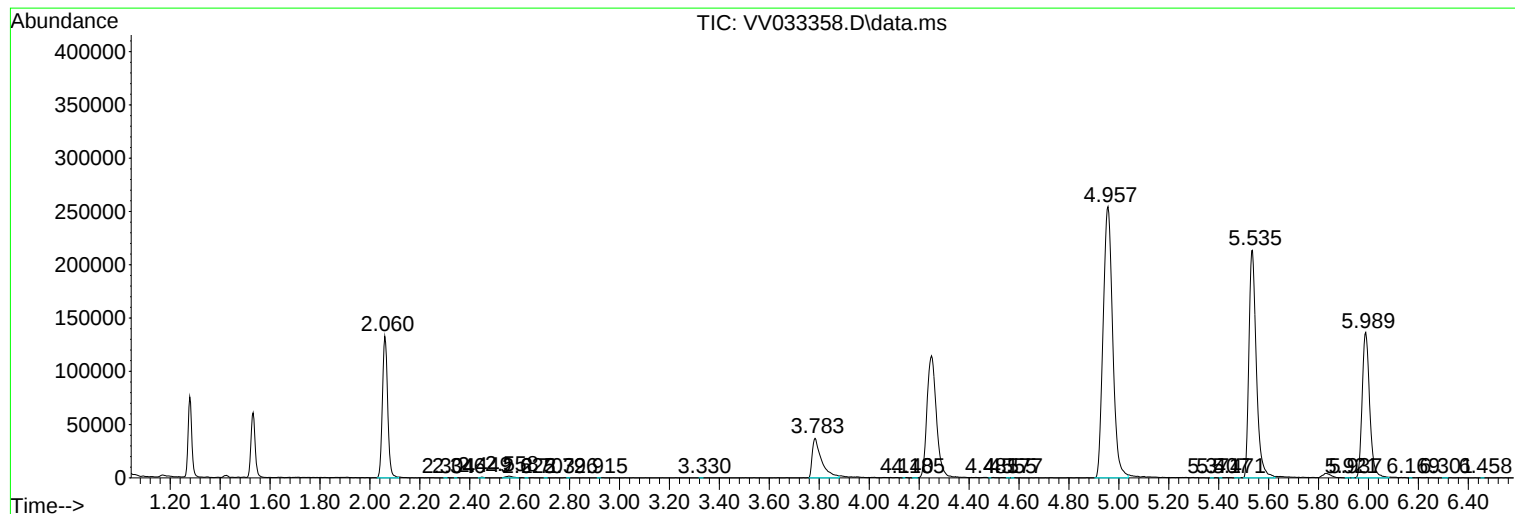

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033358.D
Acq On : 15 Dec 2023 00:29
Operator : SY/MD
Sample : 05802-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033358.D
Acq On : 15 Dec 2023 00:29
Operator : SY/MD
Sample : 05802-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------