

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033359.D
 Acq On : 15 Dec 2023 00:52
 Operator : SY/MD
 Sample : 05802-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rVB2	122038	132237	0.93%	0.669%
2	1.532	146	153	165	rVB	62233	72088	0.51%	0.365%
3	2.069	307	320	345	rBV	9955892	14200981	100.00%	71.869%
4	3.053	624	626	628	rBV	250	152	0.00%	0.001%
5	3.114	631	645	666	rBV2	40473	84999	0.60%	0.430%
6	3.246	682	686	688	rBB	271	143	0.00%	0.001%
7	3.278	694	696	698	rBV	149	107	0.00%	0.001%
8	3.786	844	854	858	rBV	35809	63761	0.45%	0.323%
9	4.249	981	998	1028	rBV	118171	308577	2.17%	1.562%
10	4.529	1081	1085	1086	rBV	197	160	0.00%	0.001%
11	4.680	1130	1132	1135	rBB	251	145	0.00%	0.001%
12	4.841	1179	1182	1184	rBV2	579	319	0.00%	0.002%
13	4.957	1202	1218	1231	rBV2	255515	684775	4.82%	3.466%
14	5.313	1327	1329	1330	rBV	227	105	0.00%	0.001%
15	5.336	1334	1336	1339	rBV2	420	304	0.00%	0.002%
16	5.387	1348	1352	1355	rBB	250	203	0.00%	0.001%
17	5.407	1356	1358	1361	rBB	236	108	0.00%	0.001%
18	5.445	1367	1370	1372	rBV	252	148	0.00%	0.001%
19	5.535	1386	1398	1431	rBV	216258	445903	3.14%	2.257%
20	5.989	1526	1539	1570	rBV2	139650	290959	2.05%	1.473%
21	6.172	1593	1596	1599	rVB3	646	347	0.00%	0.002%
22	6.284	1627	1631	1633	rBV	129	135	0.00%	0.001%
23	6.387	1661	1663	1666	rBB	231	132	0.00%	0.001%
24	6.574	1719	1721	1723	rBB	287	129	0.00%	0.001%
25	6.911	1815	1826	1846	rBV	81340	154457	1.09%	0.782%
26	7.146	1896	1899	1902	rBB2	267	148	0.00%	0.001%
27	7.243	1918	1929	1955	rBV	332220	585432	4.12%	2.963%
28	7.551	2014	2025	2046	rBV	61723	111978	0.79%	0.567%
29	7.770	2090	2093	2097	rBB	138	116	0.00%	0.001%
30	7.815	2104	2107	2109	rBB	171	108	0.00%	0.001%
31	7.879	2113	2127	2137	rBV	21863	43665	0.31%	0.221%
32	8.024	2163	2172	2194	rBV	124372	227814	1.60%	1.153%
33	8.255	2242	2244	2247	rVB2	288	140	0.00%	0.001%
34	8.275	2248	2250	2256	rVB2	507	449	0.00%	0.002%
35	8.403	2286	2290	2292	rBB2	329	187	0.00%	0.001%
36	8.484	2313	2315	2317	rBB	267	119	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033359.D
 Acq On : 15 Dec 2023 00:52
 Operator : SY/MD
 Sample : 05802-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	8.500	2317	2320	2323	rBB	242	159	0.00%	0.001%
38	8.590	2347	2348	2350	rBV	243	113	0.00%	0.001%
39	8.670	2370	2373	2375	rBB	304	180	0.00%	0.001%
40	8.786	2397	2409	2434	rBV	353090	585357	4.12%	2.962%
41	9.021	2480	2482	2484	rBB	310	123	0.00%	0.001%
42	9.040	2485	2488	2490	rBB	222	109	0.00%	0.001%
43	9.156	2520	2524	2527	rBB2	233	171	0.00%	0.001%
44	9.220	2541	2544	2546	rBB	269	148	0.00%	0.001%
45	9.490	2623	2628	2631	rBV2	635	543	0.00%	0.003%
46	9.571	2649	2653	2656	rBB	140	136	0.00%	0.001%
47	9.760	2708	2712	2713	rBB	334	161	0.00%	0.001%
48	9.792	2720	2722	2725	rBB	171	110	0.00%	0.001%
49	9.853	2737	2741	2743	rBV	184	169	0.00%	0.001%
50	10.152	2823	2834	2861	rBV	224151	355702	2.50%	1.800%
51	10.326	2877	2888	2900	rBB	27543	44999	0.32%	0.228%
52	10.429	2918	2920	2922	rBB	246	113	0.00%	0.001%
53	10.525	2946	2950	2952	rBB	179	137	0.00%	0.001%
54	10.702	2998	3005	3010	rBV4	2305	3235	0.02%	0.016%
55	10.853	3049	3052	3054	rBB	216	106	0.00%	0.001%
56	10.866	3054	3056	3059	rBB	370	163	0.00%	0.001%
57	10.898	3064	3066	3068	rBV	454	271	0.00%	0.001%
58	11.127	3129	3137	3143	rBV2	2922	3921	0.03%	0.020%
59	11.185	3145	3155	3182	rVB	406020	650266	4.58%	3.291%
60	11.365	3210	3211	3215	rBB	370	201	0.00%	0.001%
61	11.387	3215	3218	3220	rBV	274	223	0.00%	0.001%
62	11.561	3260	3272	3291	rBV	433062	684583	4.82%	3.465%
63	11.767	3334	3336	3338	rBV	226	129	0.00%	0.001%
64	11.808	3347	3349	3350	rBV	337	137	0.00%	0.001%
65	11.866	3365	3367	3370	rBB	368	191	0.00%	0.001%
66	11.934	3383	3388	3390	rBB2	266	208	0.00%	0.001%
67	11.992	3403	3406	3407	rBV	224	124	0.00%	0.001%
68	12.095	3433	3438	3441	rBB	223	174	0.00%	0.001%
69	12.133	3446	3450	3453	rBB	300	178	0.00%	0.001%
70	12.152	3454	3456	3459	rBB	212	106	0.00%	0.001%
71	12.194	3459	3469	3479	rBV2	5708	8956	0.06%	0.045%
72	12.307	3502	3504	3507	rBV	140	114	0.00%	0.001%
73	12.567	3582	3585	3587	rBB	341	133	0.00%	0.001%
74	12.738	3635	3638	3640	rBB	379	171	0.00%	0.001%
75	12.821	3660	3664	3666	rBB	139	120	0.00%	0.001%
76	12.844	3669	3671	3674	rBB2	303	185	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033359.D
 Acq On : 15 Dec 2023 00:52
 Operator : SY/MD
 Sample : 05802-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.882	3681	3683	3685	rBB	361	177	0.00%	0.001%
78	12.911	3690	3692	3695	rBB	379	210	0.00%	0.001%
79	13.014	3719	3724	3728	rBB2	348	304	0.00%	0.002%
80	13.075	3740	3743	3745	rBV2	238	150	0.00%	0.001%
81	13.130	3757	3760	3762	rBV2	244	117	0.00%	0.001%
82	13.201	3777	3782	3785	rBV	579	570	0.00%	0.003%
83	13.252	3795	3798	3803	rBV	212	229	0.00%	0.001%
84	13.294	3809	3811	3814	rBV2	236	173	0.00%	0.001%
85	13.332	3819	3823	3824	rBV	167	131	0.00%	0.001%
86	13.355	3828	3830	3833	rBB	303	168	0.00%	0.001%
87	13.448	3857	3859	3860	rBV	443	219	0.00%	0.001%
88	13.519	3878	3881	3882	rBB	224	106	0.00%	0.001%
89	13.577	3896	3899	3901	rBB	350	161	0.00%	0.001%
90	13.599	3901	3906	3910	rBB2	280	341	0.00%	0.002%
91	13.622	3910	3913	3916	rBV2	255	218	0.00%	0.001%
92	13.702	3937	3938	3942	rVB	254	139	0.00%	0.001%
93	13.776	3959	3961	3962	rBV	248	110	0.00%	0.001%
94	13.831	3976	3978	3981	rBV2	216	113	0.00%	0.001%
95	13.918	4003	4005	4008	rBV	233	146	0.00%	0.001%
96	14.062	4047	4050	4057	rBV3	635	741	0.01%	0.004%
97	14.152	4076	4078	4080	rBV	320	151	0.00%	0.001%
98	14.223	4097	4100	4103	rBV3	725	517	0.00%	0.003%
99	14.422	4160	4162	4165	rBV	541	265	0.00%	0.001%
100	14.490	4181	4183	4184	rBV	361	167	0.00%	0.001%




Sum of corrected areas: 19759478

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033359.D
Acq On : 15 Dec 2023 00:52
Operator : SY/MD
Sample : 05802-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

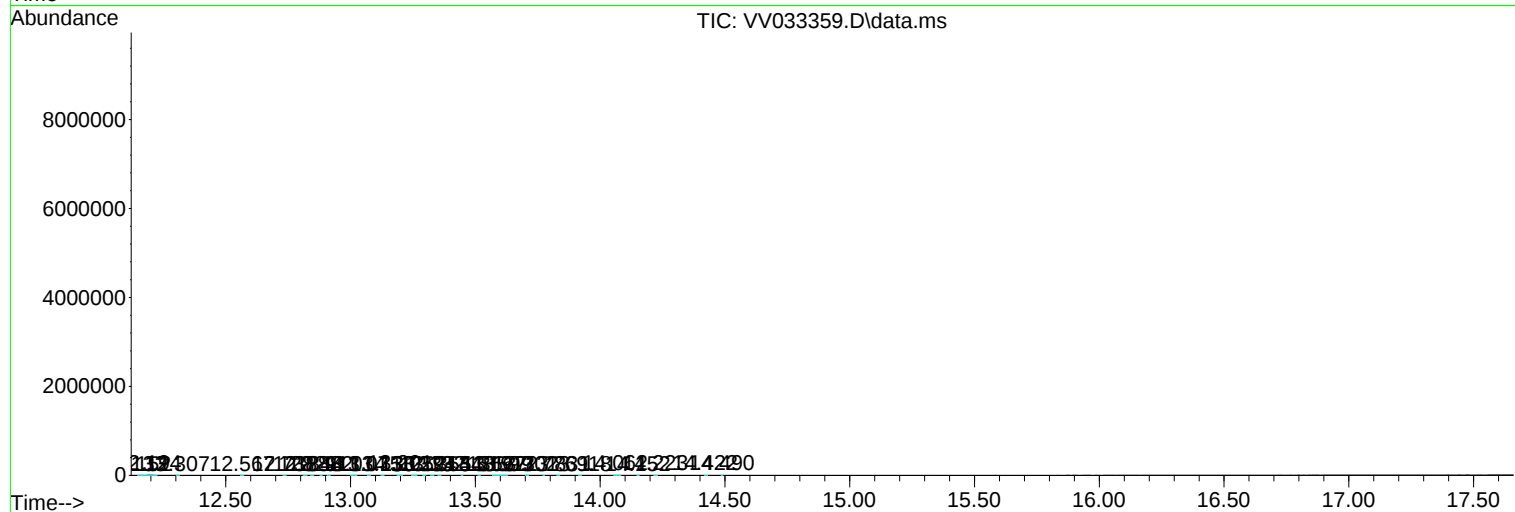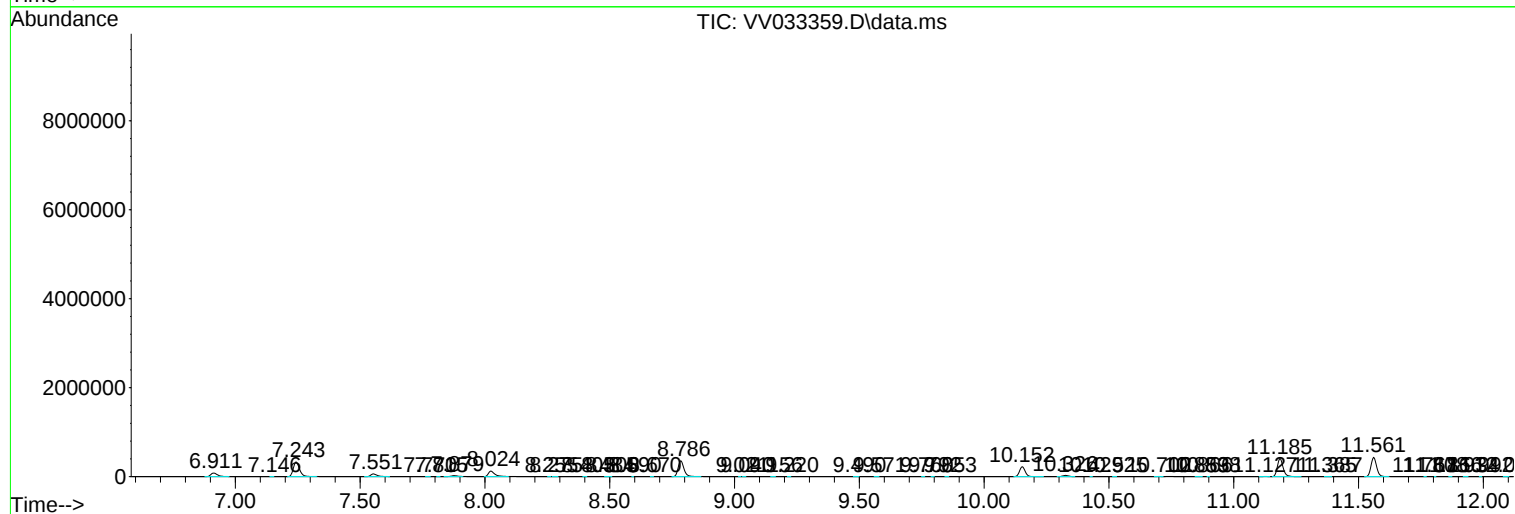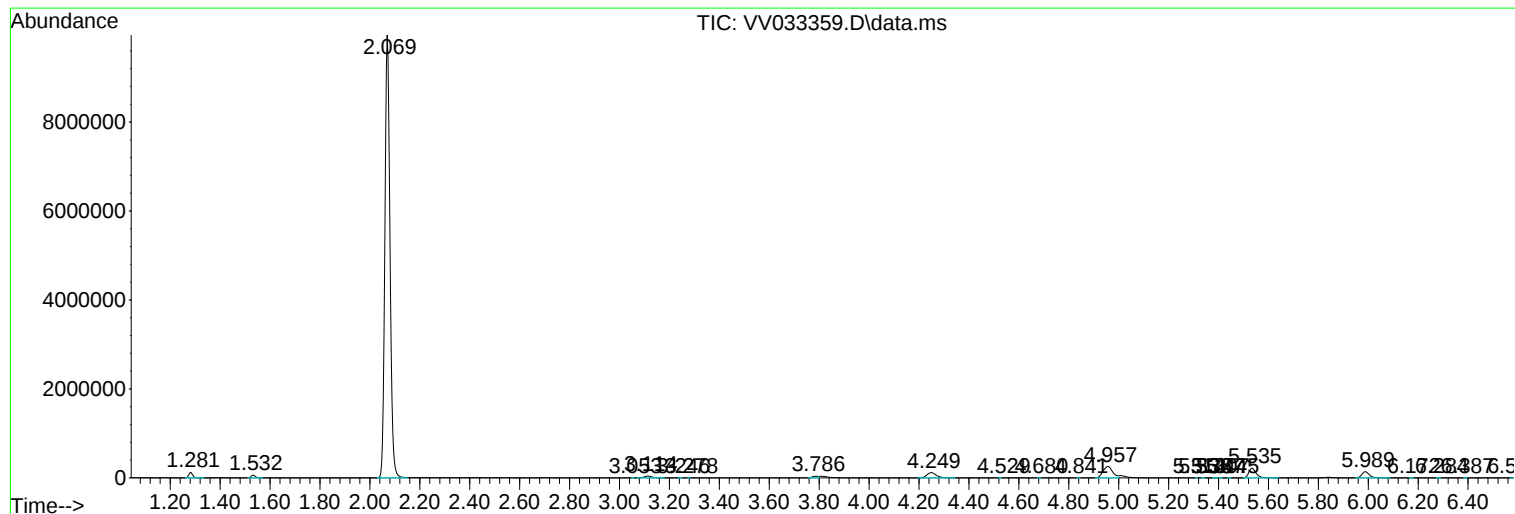

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033359.D
Acq On : 15 Dec 2023 00:52
Operator : SY/MD
Sample : 05802-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033359.D
Acq On : 15 Dec 2023 00:52
Operator : SY/MD
Sample : 05802-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------