

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033362.D
 Acq On : 15 Dec 2023 02:01
 Operator : SY/MD
 Sample : 05802-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033362.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rBV	69658	71312	10.84%	1.351%
2	1.532	146	153	168	rVB	50645	60418	9.18%	1.145%
3	2.008	299	301	303	rBV	156	102	0.02%	0.002%
4	2.059	307	317	331	rBV	111677	167119	25.40%	3.167%
5	2.223	366	368	371	rBB	134	94	0.01%	0.002%
6	2.449	436	438	442	rBB2	291	201	0.03%	0.004%
7	2.555	467	471	472	rBV	432	310	0.05%	0.006%
8	2.934	587	589	592	rBB	167	113	0.02%	0.002%
9	3.339	713	715	718	rBB	117	86	0.01%	0.002%
10	3.654	810	813	815	rBB	139	98	0.01%	0.002%
11	3.783	845	853	877	rBV2	30888	82418	12.53%	1.562%
12	4.130	957	961	964	rBV2	238	167	0.03%	0.003%
13	4.188	975	979	982	rBV	283	282	0.04%	0.005%
14	4.249	982	998	1023	rBV2	117806	303699	46.16%	5.755%
15	4.522	1081	1083	1084	rBV	245	137	0.02%	0.003%
16	4.657	1123	1125	1126	rBV	243	96	0.01%	0.002%
17	4.956	1202	1218	1252	rBV2	246382	657987	100.00%	12.469%
18	5.378	1347	1349	1350	rBV	158	87	0.01%	0.002%
19	5.458	1373	1374	1377	rBB	218	104	0.02%	0.002%
20	5.532	1385	1397	1425	rBV2	206410	432171	65.68%	8.190%
21	5.989	1527	1539	1560	rBV2	132880	272042	41.34%	5.155%
22	6.201	1603	1605	1608	rBB2	223	123	0.02%	0.002%
23	6.265	1622	1625	1629	rBB	176	167	0.03%	0.003%
24	6.426	1673	1675	1679	rBB	164	133	0.02%	0.003%
25	6.477	1690	1691	1696	rBB	149	129	0.02%	0.002%
26	6.670	1749	1751	1753	rBB	252	95	0.01%	0.002%
27	6.915	1816	1827	1850	rBV	79209	147734	22.45%	2.800%
28	7.165	1903	1905	1907	rBB	234	126	0.02%	0.002%
29	7.243	1918	1929	1955	rBV	316819	558425	84.87%	10.582%
30	7.519	2013	2015	2016	rBV	281	127	0.02%	0.002%
31	7.554	2016	2026	2051	rVV2	57867	105350	16.01%	1.996%
32	7.802	2102	2103	2108	rBB2	319	197	0.03%	0.004%
33	7.879	2115	2127	2141	rBB	9896	17076	2.60%	0.324%
34	8.024	2163	2172	2199	rBV	117179	221801	33.71%	4.203%
35	8.294	2253	2256	2258	rBV	269	181	0.03%	0.003%
36	8.355	2271	2275	2279	rBB2	270	217	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033362.D
 Acq On : 15 Dec 2023 02:01
 Operator : SY/MD
 Sample : 05802-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	8.378	2280	2282	2284	rBB	389	182	0.03%	0.003%
38	8.403	2287	2290	2292	rBB	231	109	0.02%	0.002%
39	8.452	2302	2305	2307	rBB	160	102	0.02%	0.002%
40	8.497	2317	2319	2322	rBV	152	123	0.02%	0.002%
41	8.538	2330	2332	2336	rBB	162	102	0.02%	0.002%
42	8.603	2346	2352	2353	rBV	234	171	0.03%	0.003%
43	8.786	2398	2409	2428	rBV	335741	556862	84.63%	10.553%
44	9.050	2488	2491	2494	rBB	120	109	0.02%	0.002%
45	9.082	2499	2501	2502	rBV	350	184	0.03%	0.003%
46	9.162	2524	2526	2530	rBB	170	132	0.02%	0.003%
47	9.497	2626	2630	2635	rBB3	428	365	0.06%	0.007%
48	9.567	2650	2652	2654	rBB	260	117	0.02%	0.002%
49	9.596	2657	2661	2664	rBB	235	173	0.03%	0.003%
50	9.706	2692	2695	2697	rBB	167	106	0.02%	0.002%
51	9.979	2778	2780	2782	rBB	173	86	0.01%	0.002%
52	10.050	2800	2802	2805	rBB	130	91	0.01%	0.002%
53	10.152	2823	2834	2863	rBB	215712	341694	51.93%	6.475%
54	10.326	2877	2888	2899	rBB	15134	23442	3.56%	0.444%
55	10.426	2916	2919	2921	rBB	236	129	0.02%	0.002%
56	10.451	2924	2927	2929	rBB2	303	169	0.03%	0.003%
57	10.718	3008	3010	3012	rBB	236	93	0.01%	0.002%
58	10.779	3027	3029	3032	rBB	136	92	0.01%	0.002%
59	10.863	3048	3055	3057	rBV	312	365	0.06%	0.007%
60	11.185	3144	3155	3175	rBV	387257	603412	91.71%	11.435%
61	11.432	3228	3232	3233	rBV	211	103	0.02%	0.002%
62	11.464	3240	3242	3244	rBB	196	99	0.02%	0.002%
63	11.561	3259	3272	3294	rBV	400745	635040	96.51%	12.034%
64	12.194	3461	3469	3477	rBB4	3276	4947	0.75%	0.094%
65	12.236	3480	3482	3484	rBB	243	129	0.02%	0.002%
66	12.393	3527	3531	3534	rBB2	355	307	0.05%	0.006%
67	12.770	3646	3648	3650	rBV	144	97	0.01%	0.002%
68	12.921	3693	3695	3698	rBB	128	89	0.01%	0.002%
69	12.956	3701	3706	3708	rBB	222	163	0.02%	0.003%
70	13.004	3717	3721	3725	rBB2	264	205	0.03%	0.004%
71	13.062	3734	3739	3743	rBB	186	188	0.03%	0.004%
72	13.104	3750	3752	3756	rBV	224	174	0.03%	0.003%
73	13.175	3770	3774	3776	rBV	318	264	0.04%	0.005%
74	13.239	3791	3794	3797	rBB2	400	256	0.04%	0.005%
75	13.262	3798	3801	3802	rBV	334	134	0.02%	0.003%
76	13.323	3817	3820	3823	rBB	122	103	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033362.D
 Acq On : 15 Dec 2023 02:01
 Operator : SY/MD
 Sample : 05802-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B03

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.361	3829	3832	3836	rBB	306	196	0.03%	0.004%
78	13.416	3846	3849	3851	rBV2	277	193	0.03%	0.004%
79	13.448	3857	3859	3860	rBV2	228	103	0.02%	0.002%
80	13.487	3869	3871	3873	rBV	254	157	0.02%	0.003%
81	13.545	3886	3889	3890	rBV	231	128	0.02%	0.002%
82	13.580	3897	3900	3902	rBB	245	93	0.01%	0.002%
83	13.612	3905	3910	3915	rBB3	486	435	0.07%	0.008%
84	13.635	3916	3917	3919	rBB3	253	95	0.01%	0.002%
85	13.651	3919	3922	3923	rBV	327	154	0.02%	0.003%
86	13.741	3948	3950	3952	rBB	272	143	0.02%	0.003%
87	13.789	3962	3965	3968	rBB2	354	249	0.04%	0.005%
88	13.815	3971	3973	3977	rBB2	239	153	0.02%	0.003%
89	13.850	3978	3984	3987	rBB4	537	559	0.08%	0.011%
90	13.882	3991	3994	3996	rBB	128	88	0.01%	0.002%
91	13.898	3997	3999	4001	rBV	251	128	0.02%	0.002%
92	13.930	4006	4009	4010	rBV	187	94	0.01%	0.002%
93	13.979	4019	4024	4026	rBV2	512	467	0.07%	0.009%
94	14.033	4039	4041	4042	rBV2	349	124	0.02%	0.002%
95	14.082	4054	4056	4059	rBB	143	103	0.02%	0.002%
96	14.104	4060	4063	4065	rVV2	379	279	0.04%	0.005%
97	14.143	4069	4075	4077	rBV	205	224	0.03%	0.004%
98	14.181	4082	4087	4089	rBV2	377	329	0.05%	0.006%
99	14.348	4137	4139	4140	rBV	373	192	0.03%	0.004%
100	14.647	4227	4232	4234	rBV3	634	563	0.09%	0.011%




Sum of corrected areas: 5276881

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033362.D
Acq On : 15 Dec 2023 02:01
Operator : SY/MD
Sample : 05802-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

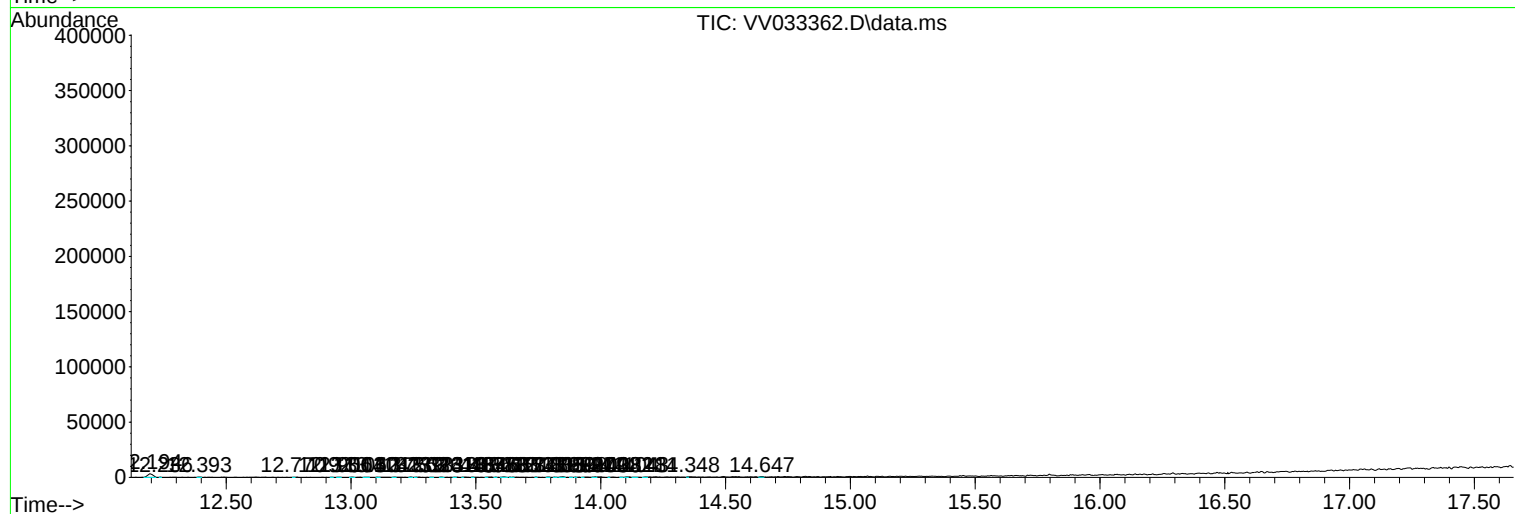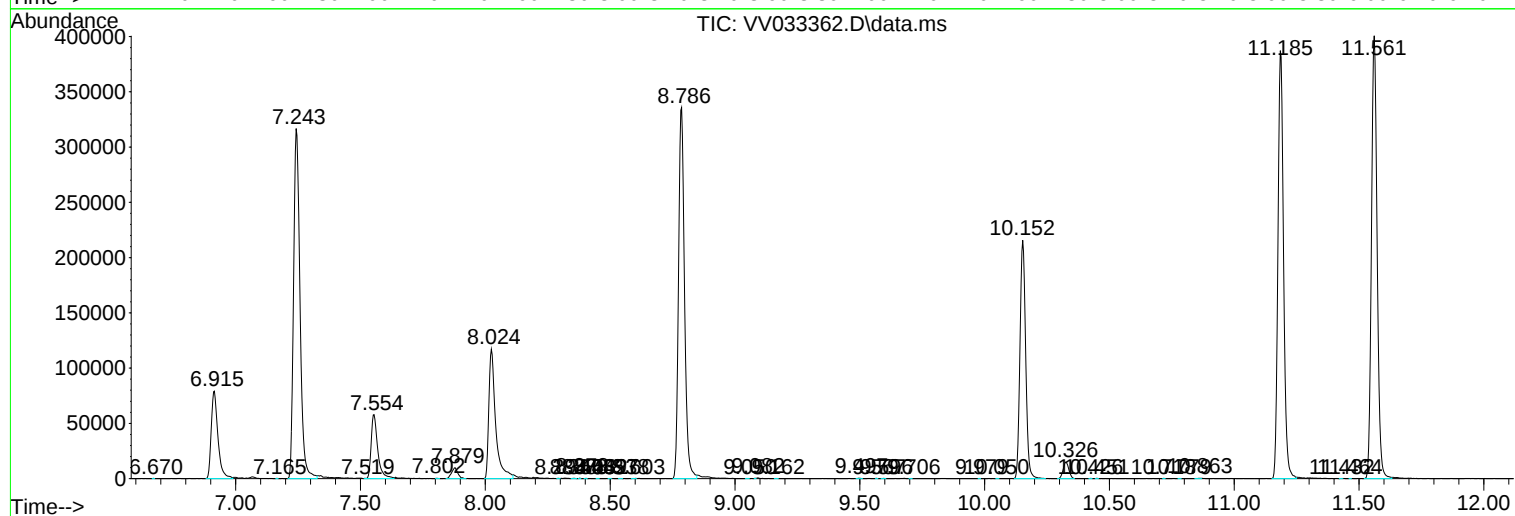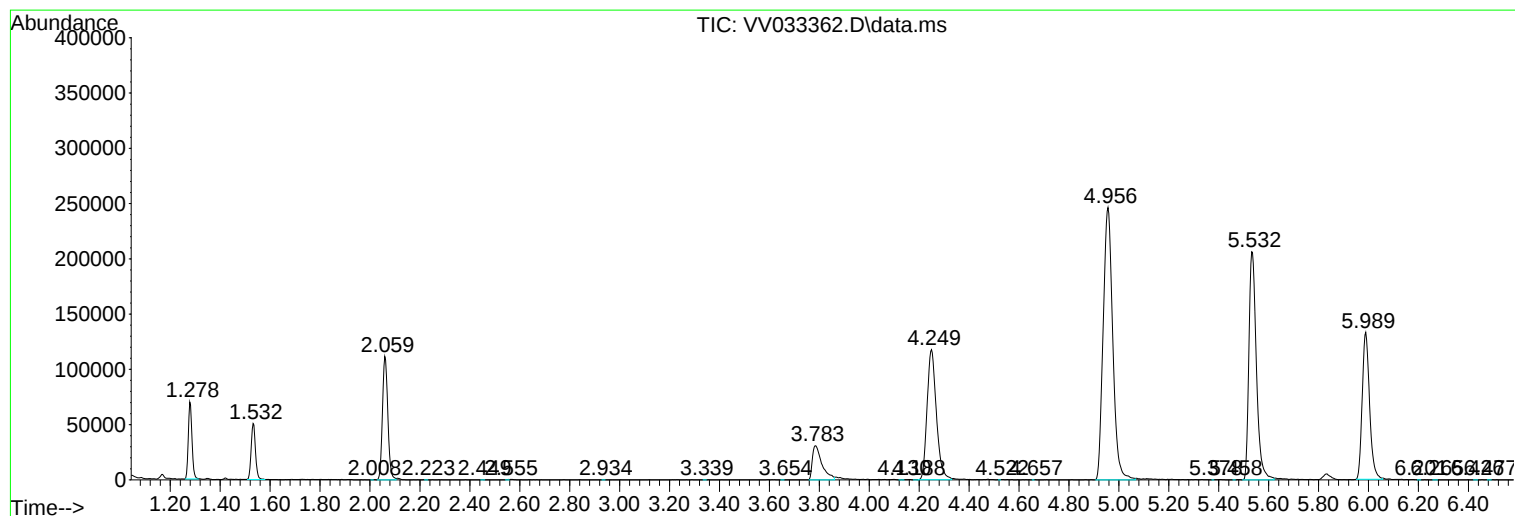

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033362.D
Acq On : 15 Dec 2023 02:01
Operator : SY/MD
Sample : 05802-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033362.D
Acq On : 15 Dec 2023 02:01
Operator : SY/MD
Sample : 05802-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B03

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------