

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033363.D
 Acq On : 15 Dec 2023 02:24
 Operator : SY/MD
 Sample : 05802-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	67621	69752	10.82%	1.348%
2	1.532	145	153	167	rVB	48329	55997	8.68%	1.082%
3	1.947	280	282	287	rBB	234	168	0.03%	0.003%
4	1.986	292	294	296	rBB	230	91	0.01%	0.002%
5	2.060	307	317	334	rBV	108512	160918	24.96%	3.110%
6	2.243	368	374	381	rBV2	781	1054	0.16%	0.020%
7	2.445	433	437	439	rBV	250	186	0.03%	0.004%
8	2.552	465	470	472	rBV	246	250	0.04%	0.005%
9	2.770	536	538	542	rBB	126	107	0.02%	0.002%
10	3.783	845	853	881	rBV	27842	73544	11.41%	1.422%
11	4.098	949	951	954	rBB	145	98	0.02%	0.002%
12	4.117	955	957	959	rBB	206	103	0.02%	0.002%
13	4.249	979	998	1028	rBV	104988	271566	42.12%	5.249%
14	4.474	1066	1068	1071	rVB2	405	219	0.03%	0.004%
15	4.535	1085	1087	1090	rVB	374	128	0.02%	0.002%
16	4.957	1201	1218	1245	rBV2	237979	629613	97.65%	12.170%
17	5.465	1374	1376	1379	rBB	152	102	0.02%	0.002%
18	5.532	1386	1397	1428	rBV2	200309	413786	64.18%	7.998%
19	5.937	1520	1523	1526	rBV	157	166	0.03%	0.003%
20	5.989	1526	1539	1568	rVV	128570	266070	41.27%	5.143%
21	6.211	1606	1608	1610	rBB	236	111	0.02%	0.002%
22	6.265	1623	1625	1627	rBV	146	94	0.01%	0.002%
23	6.336	1644	1647	1648	rBB	240	101	0.02%	0.002%
24	6.690	1755	1757	1760	rBB	129	88	0.01%	0.002%
25	6.767	1778	1781	1783	rBB	125	89	0.01%	0.002%
26	6.915	1816	1827	1849	rBV	77283	145400	22.55%	2.810%
27	7.108	1884	1887	1890	rBV2	271	220	0.03%	0.004%
28	7.149	1898	1900	1903	rBV2	404	294	0.05%	0.006%
29	7.243	1917	1929	1953	rBV	307891	547397	84.90%	10.581%
30	7.555	2016	2026	2052	rBV	56168	101908	15.81%	1.970%
31	7.725	2076	2079	2080	rBV	160	106	0.02%	0.002%
32	7.754	2086	2088	2089	rBB	222	85	0.01%	0.002%
33	7.876	2115	2126	2140	rBB2	11914	21824	3.38%	0.422%
34	8.024	2163	2172	2202	rBV	116079	222219	34.47%	4.295%
35	8.310	2258	2261	2265	rBB2	231	201	0.03%	0.004%
36	8.368	2276	2279	2281	rBB	165	106	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033363.D
 Acq On : 15 Dec 2023 02:24
 Operator : SY/MD
 Sample : 05802-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	8.516	2321	2325	2328	rBB	141	120	0.02%	0.002%
38	8.542	2329	2333	2334	rBV	211	103	0.02%	0.002%
39	8.635	2360	2362	2365	rVB	270	165	0.03%	0.003%
40	8.702	2378	2383	2384	rBV	230	153	0.02%	0.003%

41	8.783	2398	2408	2435	rBV	334026	551514	85.54%	10.660%
42	9.021	2479	2482	2486	rBB	240	182	0.03%	0.004%
43	9.085	2498	2502	2504	rBV	491	328	0.05%	0.006%
44	9.497	2628	2630	2634	rBB2	344	188	0.03%	0.004%
45	9.564	2649	2651	2653	rBB2	300	115	0.02%	0.002%

46	9.915	2756	2760	2762	rBB	131	115	0.02%	0.002%
47	9.998	2782	2786	2788	rBB	127	117	0.02%	0.002%
48	10.107	2815	2820	2821	rBV	169	158	0.02%	0.003%
49	10.152	2823	2834	2857	rVB	210934	332300	51.54%	6.423%
50	10.265	2867	2869	2870	rVB	338	87	0.01%	0.002%

51	10.326	2877	2888	2900	rBB2	20723	32707	5.07%	0.632%
52	10.458	2926	2929	2931	rBB	128	89	0.01%	0.002%
53	10.590	2967	2970	2972	rBB	228	107	0.02%	0.002%
54	10.815	3037	3040	3042	rBB2	296	159	0.02%	0.003%
55	10.857	3052	3053	3056	rBB	238	102	0.02%	0.002%

56	11.056	3113	3115	3117	rBB	249	94	0.01%	0.002%
57	11.091	3124	3126	3128	rBB	250	102	0.02%	0.002%
58	11.111	3129	3132	3135	rBB2	234	157	0.02%	0.003%
59	11.185	3144	3155	3180	rBV	395523	610843	94.74%	11.807%
60	11.419	3224	3228	3231	rBB	294	242	0.04%	0.005%

61	11.435	3231	3233	3235	rBB	336	127	0.02%	0.002%
62	11.493	3248	3251	3252	rBV	220	127	0.02%	0.002%
63	11.561	3260	3272	3293	rBV	411732	644757	100.00%	12.462%
64	12.059	3424	3427	3429	rBB	317	180	0.03%	0.003%
65	12.156	3455	3457	3460	rBB	291	172	0.03%	0.003%

66	12.194	3460	3469	3479	rBB3	5155	7905	1.23%	0.153%
67	12.268	3490	3492	3494	rBB	263	122	0.02%	0.002%
68	12.304	3495	3503	3504	rBV2	646	503	0.08%	0.010%
69	12.352	3515	3518	3521	rBB2	244	147	0.02%	0.003%
70	12.368	3521	3523	3525	rBB	277	146	0.02%	0.003%

71	12.381	3525	3527	3528	rBB	235	87	0.01%	0.002%
72	12.394	3528	3531	3533	rBB	161	105	0.02%	0.002%
73	12.455	3548	3550	3552	rBV	158	102	0.02%	0.002%
74	12.625	3601	3603	3605	rBV	140	96	0.01%	0.002%
75	12.712	3628	3630	3633	rBB	166	108	0.02%	0.002%

76	12.757	3640	3644	3646	rBB	255	161	0.02%	0.003%
----	--------	------	------	------	-----	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033363.D
 Acq On : 15 Dec 2023 02:24
 Operator : SY/MD
 Sample : 05802-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.911	3689	3692	3694	rBB	215	103	0.02%	0.002%
78	13.069	3739	3741	3743	rBV	141	102	0.02%	0.002%
79	13.114	3751	3755	3758	rBB	240	186	0.03%	0.004%
80	13.175	3772	3774	3776	rBB	238	109	0.02%	0.002%
81	13.194	3777	3780	3782	rBB	149	100	0.02%	0.002%
82	13.246	3793	3796	3798	rBB	282	157	0.02%	0.003%
83	13.291	3807	3810	3811	rBB	215	89	0.01%	0.002%
84	13.352	3825	3829	3832	rBB2	264	172	0.03%	0.003%
85	13.371	3833	3835	3836	rBV	230	93	0.01%	0.002%
86	13.435	3851	3855	3858	rBV2	258	241	0.04%	0.005%
87	13.496	3870	3874	3877	rBB3	393	274	0.04%	0.005%
88	13.535	3882	3886	3888	rBB	152	123	0.02%	0.002%
89	13.551	3888	3891	3893	rBV	161	124	0.02%	0.002%
90	13.567	3893	3896	3898	rBV	165	102	0.02%	0.002%
91	13.612	3906	3910	3913	rBB2	258	197	0.03%	0.004%
92	13.696	3934	3936	3939	rBB	271	150	0.02%	0.003%
93	13.712	3939	3941	3943	rBV2	245	135	0.02%	0.003%
94	13.731	3943	3947	3950	rBV2	357	284	0.04%	0.005%
95	13.766	3956	3958	3962	rBB2	396	233	0.04%	0.005%
96	13.815	3971	3973	3975	rVB	273	85	0.01%	0.002%
97	13.898	3997	3999	4000	rBV	278	122	0.02%	0.002%
98	14.091	4053	4059	4063	rBV3	525	597	0.09%	0.012%
99	14.303	4122	4125	4128	rBV3	395	324	0.05%	0.006%
100	14.435	4164	4166	4169	rBV	393	277	0.04%	0.005%




Sum of corrected areas: 5173632

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033363.D
Acq On : 15 Dec 2023 02:24
Operator : SY/MD
Sample : 05802-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

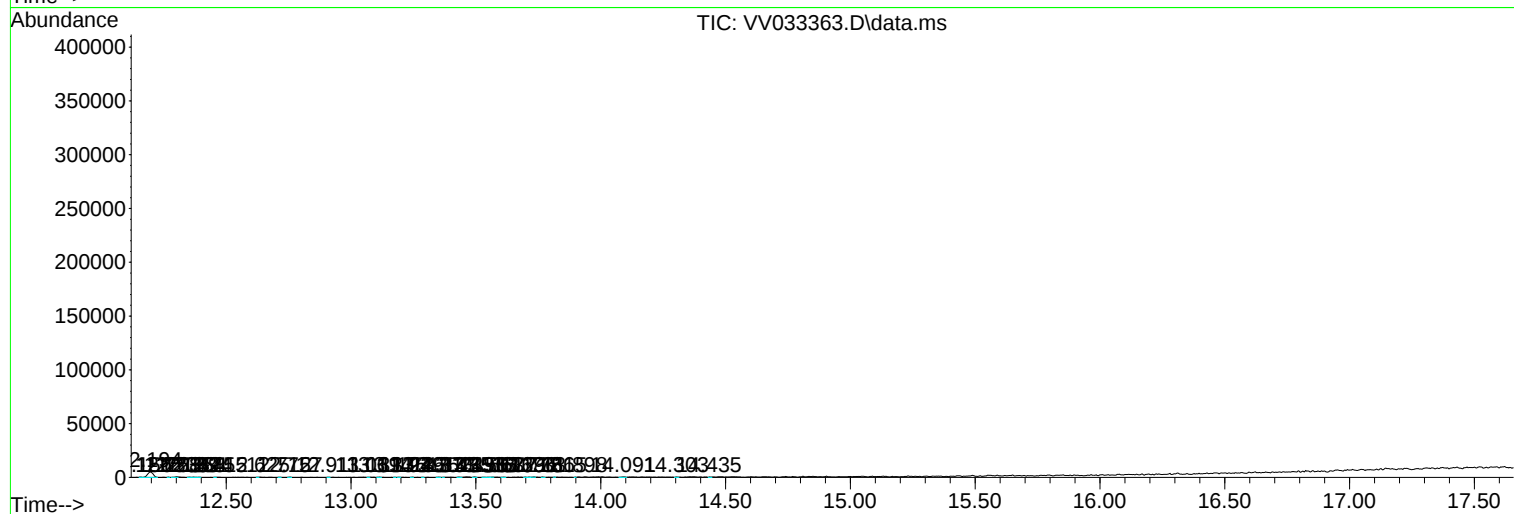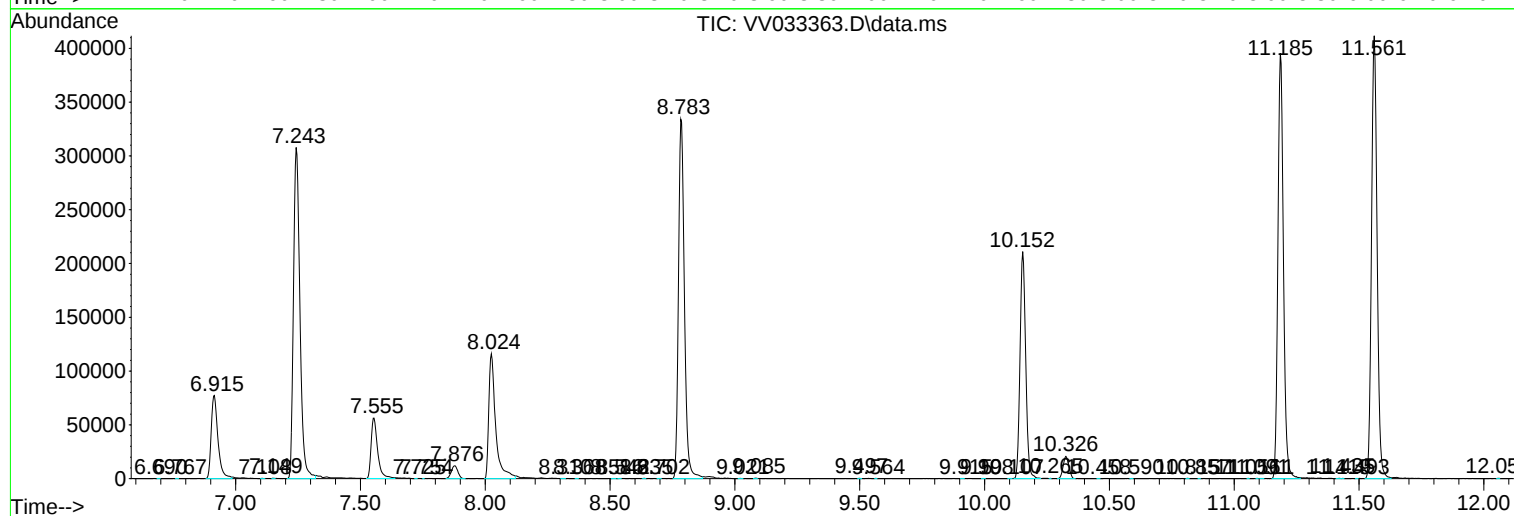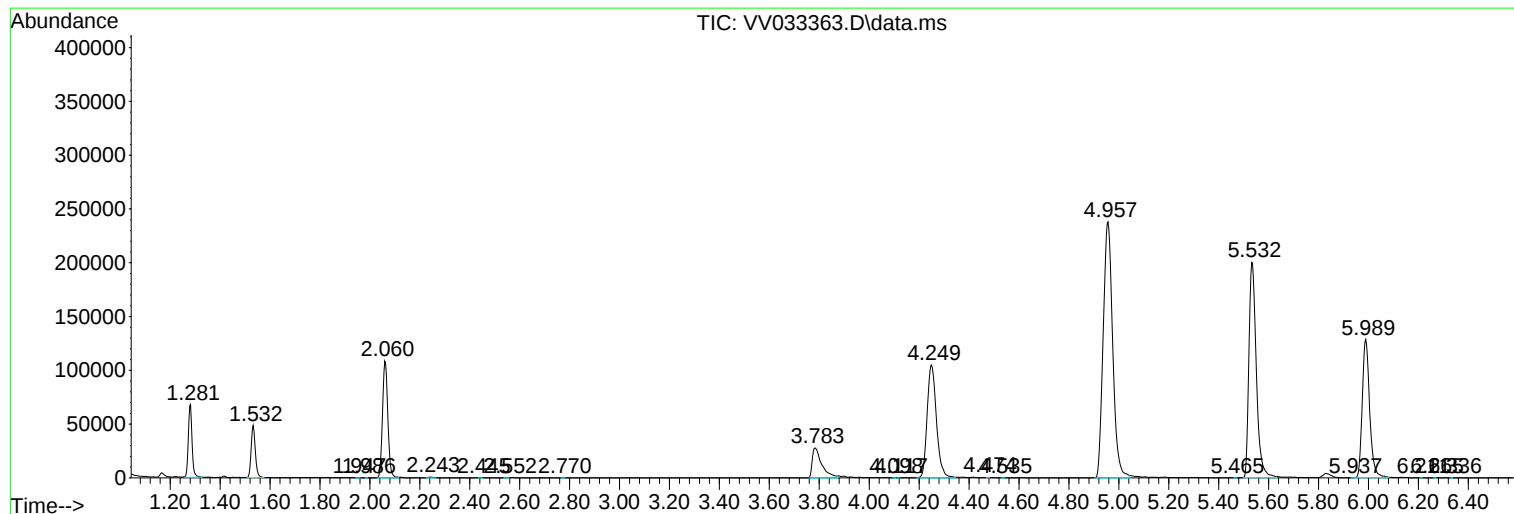

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033363.D
Acq On : 15 Dec 2023 02:24
Operator : SY/MD
Sample : 05802-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033363.D
Acq On : 15 Dec 2023 02:24
Operator : SY/MD
Sample : 05802-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------