

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033364.D
 Acq On : 15 Dec 2023 02:47
 Operator : SY/MD
 Sample : 05802-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rVB	64507	67774	0.10%	0.070%
2	1.384	103	107	114	rVB	2456	2423	0.00%	0.002%
3	1.532	145	153	167	rVB	47720	56342	0.08%	0.058%
4	2.060	307	317	333	rBV2	111402	170649	0.24%	0.176%
5	2.449	436	438	441	rBV2	489	289	0.00%	0.000%
6	2.548	466	469	471	rBV	269	186	0.00%	0.000%
7	2.696	505	515	533	rBV2	57882	102041	0.15%	0.105%
8	3.812	844	862	899	rBV	1237378	2993273	4.26%	3.079%
9	4.249	983	998	1023	rBV	105640	262584	0.37%	0.270%
10	4.567	1093	1097	1100	rBV2	466	318	0.00%	0.000%
11	4.590	1100	1104	1106	rVB2	502	363	0.00%	0.000%
12	4.609	1107	1110	1116	rBB	370	350	0.00%	0.000%
13	4.674	1124	1130	1133	rBB3	511	362	0.00%	0.000%
14	4.957	1202	1218	1235	rBV2	230013	609074	0.87%	0.626%
15	5.191	1289	1291	1296	rBV	352	300	0.00%	0.000%
16	5.304	1321	1326	1330	rBB	344	298	0.00%	0.000%
17	5.326	1330	1333	1335	rBV2	501	330	0.00%	0.000%
18	5.371	1342	1347	1353	rBB2	300	340	0.00%	0.000%
19	5.535	1386	1398	1425	rBV	199502	415085	0.59%	0.427%
20	5.831	1474	1490	1527	rBV	10024510	19223887	27.38%	19.772%
21	6.329	1640	1645	1648	rBV3	484	507	0.00%	0.001%
22	6.391	1662	1664	1666	rVB	306	124	0.00%	0.000%
23	6.448	1680	1682	1685	rBB	265	130	0.00%	0.000%
24	6.545	1708	1712	1714	rBV2	276	210	0.00%	0.000%
25	6.911	1816	1826	1848	rBV	76933	141217	0.20%	0.145%
26	7.082	1875	1879	1882	rBB	200	177	0.00%	0.000%
27	7.101	1883	1885	1887	rBB	275	124	0.00%	0.000%
28	7.165	1902	1905	1907	rBB	289	152	0.00%	0.000%
29	7.243	1918	1929	1953	rBV	310744	544870	0.78%	0.560%
30	7.551	2016	2025	2045	rBV2	55426	100125	0.14%	0.103%
31	7.718	2074	2077	2079	rVB2	284	199	0.00%	0.000%
32	7.744	2082	2085	2088	rBB	267	170	0.00%	0.000%
33	7.786	2096	2098	2103	rVB	348	280	0.00%	0.000%
34	7.918	2114	2139	2164	rBV	39314360	70200091	100.00%	72.201%
35	8.294	2253	2256	2262	rVB3	379	373	0.00%	0.000%
36	8.345	2270	2272	2275	rBV	309	187	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033364.D
 Acq On : 15 Dec 2023 02:47
 Operator : SY/MD
 Sample : 05802-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	8.445	2301	2303	2306	rBV2	366	206	0.00%	0.000%
38	8.471	2306	2311	2313	rBV3	566	532	0.00%	0.001%
39	8.567	2338	2341	2344	rBV	269	203	0.00%	0.000%
40	8.596	2348	2350	2353	rVB	237	133	0.00%	0.000%
41	8.680	2373	2376	2380	rBB2	316	271	0.00%	0.000%
42	8.786	2397	2409	2439	rBV	330488	557305	0.79%	0.573%
43	9.079	2496	2500	2502	rBV2	293	229	0.00%	0.000%
44	9.487	2623	2627	2629	rBV	351	287	0.00%	0.000%
45	9.625	2668	2670	2673	rBB	201	130	0.00%	0.000%
46	9.937	2764	2767	2770	rBB	166	123	0.00%	0.000%
47	10.152	2823	2834	2852	rBV	219983	343829	0.49%	0.354%
48	10.326	2879	2888	2900	rBB2	10573	16053	0.02%	0.017%
49	10.532	2947	2952	2955	rBB	139	160	0.00%	0.000%
50	10.693	2999	3002	3005	rBB2	269	204	0.00%	0.000%
51	10.857	3051	3053	3056	rBV	177	141	0.00%	0.000%
52	11.133	3136	3139	3142	rBV	306	234	0.00%	0.000%
53	11.185	3142	3155	3177	rBV	420105	642440	0.92%	0.661%
54	11.339	3201	3203	3207	rVV2	270	134	0.00%	0.000%
55	11.561	3260	3272	3293	rBV	419872	664500	0.95%	0.683%
56	11.808	3347	3349	3350	rBV	276	125	0.00%	0.000%
57	12.120	3443	3446	3448	rBB	264	154	0.00%	0.000%
58	12.194	3461	3469	3476	rBB3	1909	2865	0.00%	0.003%
59	12.265	3487	3491	3494	rBB	140	135	0.00%	0.000%
60	12.300	3495	3502	3508	rBV5	1641	1897	0.00%	0.002%
61	12.477	3554	3557	3560	rBB	134	120	0.00%	0.000%
62	12.580	3586	3589	3591	rBV	183	148	0.00%	0.000%
63	12.750	3638	3642	3645	rBB2	225	172	0.00%	0.000%
64	12.783	3650	3652	3655	rBB	248	133	0.00%	0.000%
65	12.837	3667	3669	3671	rBB	254	119	0.00%	0.000%
66	12.866	3674	3678	3681	rBV	191	201	0.00%	0.000%
67	13.201	3772	3782	3802	rBV2	58249	92050	0.13%	0.095%
68	13.342	3823	3826	3828	rBV	237	144	0.00%	0.000%
69	13.371	3833	3835	3837	rBV	257	128	0.00%	0.000%
70	13.429	3850	3853	3855	rVV	316	224	0.00%	0.000%
71	13.455	3858	3861	3865	rVV	327	284	0.00%	0.000%
72	13.480	3865	3869	3871	rVV3	449	371	0.00%	0.000%
73	13.496	3871	3874	3875	rVB	358	165	0.00%	0.000%
74	13.516	3876	3880	3883	rBB	259	203	0.00%	0.000%
75	13.574	3896	3898	3902	rBV	279	214	0.00%	0.000%
76	13.625	3910	3914	3918	rBB2	268	243	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033364.D
 Acq On : 15 Dec 2023 02:47
 Operator : SY/MD
 Sample : 05802-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.654	3921	3923	3926	rBV2	252	211	0.00%	0.000%
78	13.693	3932	3935	3938	rBB	247	139	0.00%	0.000%
79	13.895	3995	3998	4000	rVB	277	180	0.00%	0.000%
80	13.940	4009	4012	4017	rBV2	427	286	0.00%	0.000%
81	13.992	4021	4028	4029	rBV	561	538	0.00%	0.001%
82	14.043	4042	4044	4046	rBV	364	230	0.00%	0.000%
83	14.069	4050	4052	4054	rVV	333	137	0.00%	0.000%
84	14.104	4060	4063	4065	rBV2	266	187	0.00%	0.000%
85	14.136	4071	4073	4076	rBV2	231	155	0.00%	0.000%
86	14.204	4091	4094	4099	rBV2	484	433	0.00%	0.000%
87	14.233	4099	4103	4104	rVV2	332	220	0.00%	0.000%
88	14.242	4104	4106	4111	rVB2	206	159	0.00%	0.000%
89	14.274	4113	4116	4118	rVB2	253	128	0.00%	0.000%
90	14.307	4119	4126	4130	rVB2	529	666	0.00%	0.001%
91	14.326	4130	4132	4134	rBV	371	243	0.00%	0.000%
92	14.403	4154	4156	4158	rBV	238	129	0.00%	0.000%
93	14.467	4173	4176	4180	rVB	352	235	0.00%	0.000%
94	14.493	4180	4184	4186	rBV2	363	331	0.00%	0.000%
95	14.583	4208	4212	4214	rBV	517	347	0.00%	0.000%
96	14.638	4227	4229	4234	rBV3	481	353	0.00%	0.000%
97	14.731	4256	4258	4260	rBV2	309	168	0.00%	0.000%
98	14.844	4291	4293	4297	rVB2	731	422	0.00%	0.000%
99	14.985	4334	4337	4340	rBV2	674	426	0.00%	0.000%
100	15.069	4361	4363	4365	rBV3	667	380	0.00%	0.000%




Sum of corrected areas: 97229116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033364.D
Acq On : 15 Dec 2023 02:47
Operator : SY/MD
Sample : 05802-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

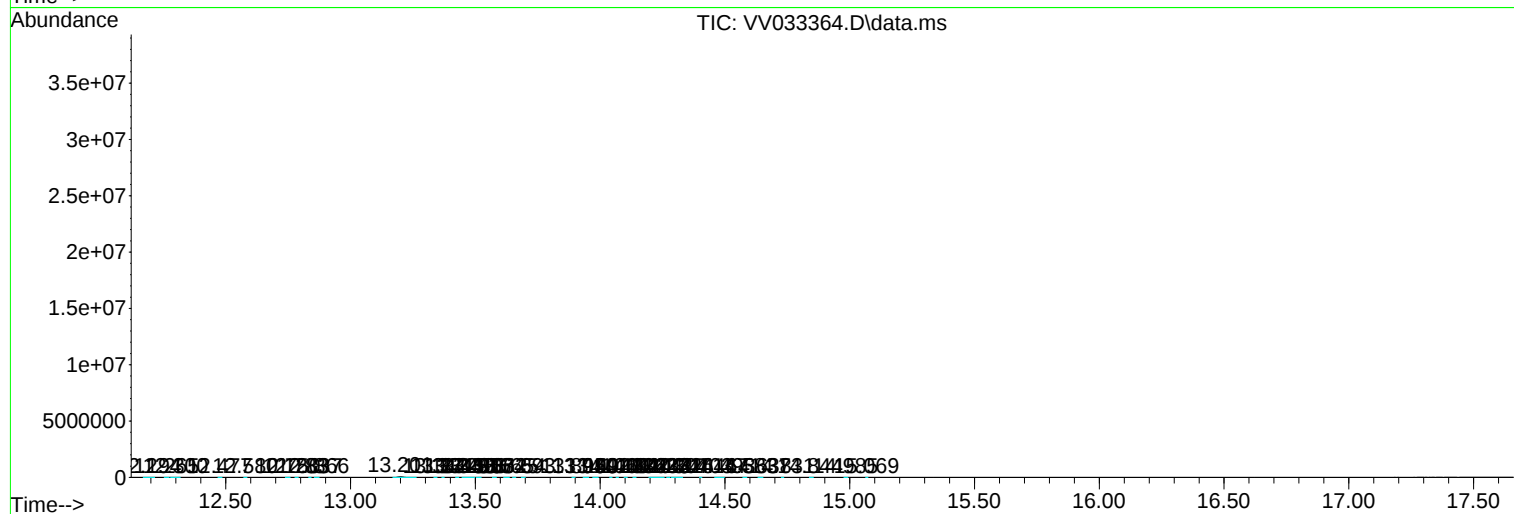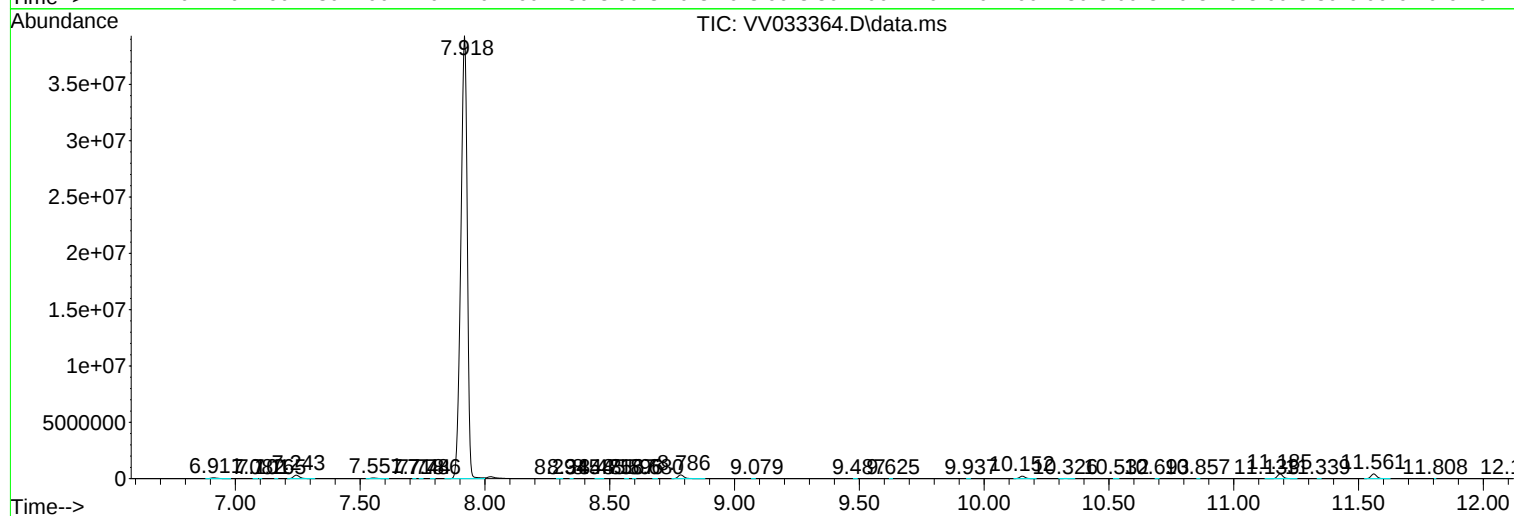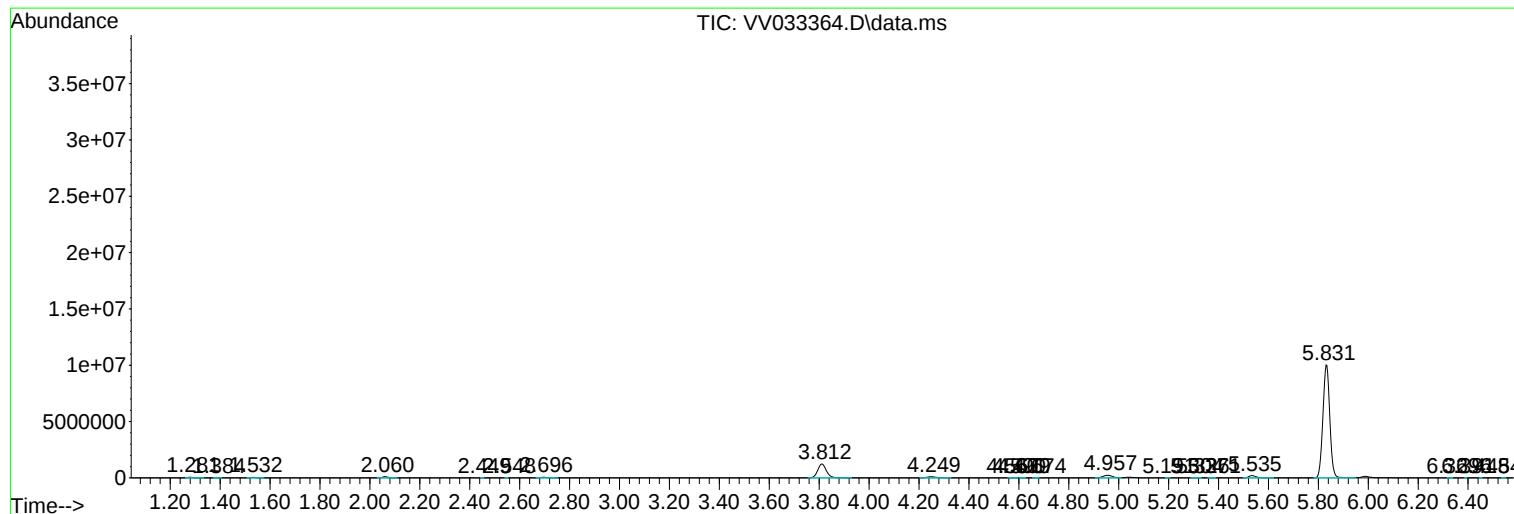

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033364.D
Acq On : 15 Dec 2023 02:47
Operator : SY/MD
Sample : 05802-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033364.D
Acq On : 15 Dec 2023 02:47
Operator : SY/MD
Sample : 05802-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc