

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033365.D
 Acq On : 15 Dec 2023 03:11
 Operator : SY/MD
 Sample : 05802-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	67	76	100	rBV	4984378	5199771	5.26%	3.555%
2	1.532	146	153	168	rVB	48700	57135	0.06%	0.039%
3	2.066	307	319	339	rVB3	211161	361463	0.37%	0.247%
4	2.249	367	376	383	rBV3	2482	4893	0.00%	0.003%
5	2.449	434	438	446	rVB4	710	930	0.00%	0.001%
6	2.696	504	515	542	rBV2	207186	376070	0.38%	0.257%
7	3.114	632	645	664	rBV2	57717	123664	0.13%	0.085%
8	3.818	842	864	898	rBV3	39596580	98901506	100.00%	67.626%
9	4.957	1201	1218	1225	rBV2	243977	600695	0.61%	0.411%
10	5.387	1349	1352	1354	rVB	531	242	0.00%	0.000%
11	5.407	1354	1358	1359	rBV	356	270	0.00%	0.000%
12	5.465	1374	1376	1378	rBV	327	151	0.00%	0.000%
13	5.532	1386	1397	1427	rBV	207273	430056	0.43%	0.294%
14	5.838	1480	1492	1513	rBV2	55446	115670	0.12%	0.079%
15	5.989	1527	1539	1565	rBV	129384	275034	0.28%	0.188%
16	6.140	1579	1586	1588	rBV4	541	579	0.00%	0.000%
17	6.175	1593	1597	1601	rBV2	499	470	0.00%	0.000%
18	6.214	1606	1609	1611	rVB2	388	224	0.00%	0.000%
19	6.275	1623	1628	1632	rBB	344	230	0.00%	0.000%
20	6.458	1682	1685	1689	rBB2	293	193	0.00%	0.000%
21	6.481	1690	1692	1694	rBV	265	166	0.00%	0.000%
22	6.519	1700	1704	1706	rBB	321	185	0.00%	0.000%
23	6.912	1816	1826	1854	rBV	82649	151340	0.15%	0.103%
24	7.072	1874	1876	1878	rVB	361	169	0.00%	0.000%
25	7.085	1878	1880	1884	rVB	329	220	0.00%	0.000%
26	7.130	1889	1894	1896	rBB	257	228	0.00%	0.000%
27	7.243	1914	1929	1940	rBV	330792	563217	0.57%	0.385%
28	7.313	1941	1951	1974	rVB	1280318	2167091	2.19%	1.482%
29	7.551	2017	2025	2047	rVB	64948	114519	0.12%	0.078%
30	7.744	2082	2085	2088	rBB	269	156	0.00%	0.000%
31	7.770	2091	2093	2095	rVV	257	152	0.00%	0.000%
32	7.905	2113	2135	2152	rBV2	242031	425213	0.43%	0.291%
33	8.024	2163	2172	2205	rBV	133306	237825	0.24%	0.163%
34	8.291	2252	2255	2259	rBB2	459	278	0.00%	0.000%
35	8.320	2262	2264	2267	rBV2	413	256	0.00%	0.000%
36	8.484	2310	2315	2318	rBB2	279	255	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033365.D
 Acq On : 15 Dec 2023 03:11
 Operator : SY/MD
 Sample : 05802-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	8.535	2328	2331	2335	rBB	170	155	0.00%	0.000%
38	8.812	2398	2417	2452	rBV	3439581	6030517	6.10%	4.123%
39	9.075	2487	2499	2513	rBV2	37931	64237	0.06%	0.044%
40	9.153	2519	2523	2525	rBV2	286	201	0.00%	0.000%
41	9.233	2546	2548	2551	rVB	414	208	0.00%	0.000%
42	9.255	2551	2555	2558	rBV2	370	279	0.00%	0.000%
43	9.355	2583	2586	2588	rBV2	211	145	0.00%	0.000%
44	9.416	2602	2605	2607	rVB	257	163	0.00%	0.000%
45	9.481	2615	2625	2645	rBV	36805	57927	0.06%	0.040%
46	9.873	2740	2747	2757	rVB2	2574	3697	0.00%	0.003%
47	10.153	2823	2834	2858	rBV	230679	363452	0.37%	0.249%
48	10.297	2870	2879	2882	rBV	5238	7389	0.01%	0.005%
49	10.480	2927	2936	2948	rBV3	8278	12318	0.01%	0.008%
50	10.677	2987	2997	3012	rBV	29443	46602	0.05%	0.032%
51	10.799	3032	3035	3037	rBB	248	160	0.00%	0.000%
52	10.853	3042	3052	3068	rBV	53004	80383	0.08%	0.055%
53	10.915	3068	3071	3076	rVB	549	438	0.00%	0.000%
54	10.950	3080	3082	3085	rBB	267	143	0.00%	0.000%
55	10.995	3089	3096	3098	rBV3	2393	2741	0.00%	0.002%
56	11.117	3121	3134	3147	rBV	4442255	6607878	6.68%	4.518%
57	11.210	3147	3163	3176	rVV	7249538	11495065	11.62%	7.860%
58	11.484	3233	3248	3261	rBV2	82390	197141	0.20%	0.135%
59	11.580	3262	3278	3302	rVV2	5713384	9232724	9.34%	6.313%
60	11.760	3325	3334	3345	rVB	46662	69697	0.07%	0.048%
61	11.850	3353	3362	3370	rBV	76658	121215	0.12%	0.083%
62	11.953	3383	3394	3413	rVB	242442	363497	0.37%	0.249%
63	12.079	3415	3433	3454	rVB3	34798	84629	0.09%	0.058%
64	12.191	3456	3468	3478	rBV5	19826	38110	0.04%	0.026%
65	12.252	3478	3487	3498	rBV	101612	152348	0.15%	0.104%
66	12.352	3510	3518	3528	rVB	197185	289771	0.29%	0.198%
67	12.490	3550	3561	3568	rBV2	13582	19323	0.02%	0.013%
68	12.664	3606	3615	3627	rVB	60582	91355	0.09%	0.062%
69	12.734	3630	3637	3645	rBV4	5437	7103	0.01%	0.005%
70	12.821	3646	3664	3683	rBV2	296280	505867	0.51%	0.346%
71	12.940	3695	3701	3710	rBV	13531	19219	0.02%	0.013%
72	13.107	3744	3753	3756	rBV3	3164	3974	0.00%	0.003%
73	13.207	3775	3784	3797	rBV4	40720	66651	0.07%	0.046%
74	13.339	3819	3825	3839	rVB4	13907	22612	0.02%	0.015%
75	13.400	3839	3844	3847	rBV2	1029	799	0.00%	0.001%
76	13.451	3854	3860	3866	rVB2	2154	2263	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033365.D
 Acq On : 15 Dec 2023 03:11
 Operator : SY/MD
 Sample : 05802-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.564	3886	3895	3907	rBV	7674	13422	0.01%	0.009%
78	13.664	3913	3926	3934	rBV6	4504	10083	0.01%	0.007%
79	13.702	3935	3938	3948	rVV4	3512	4761	0.00%	0.003%
80	13.750	3952	3953	3956	rVB	517	250	0.00%	0.000%
81	13.767	3956	3958	3960	rBV	412	158	0.00%	0.000%
82	13.847	3975	3983	3992	rVV3	8398	12221	0.01%	0.008%
83	13.882	3992	3994	3997	rVV2	342	206	0.00%	0.000%
84	13.953	4013	4016	4017	rBV2	267	155	0.00%	0.000%
85	13.966	4018	4020	4021	rBV	398	148	0.00%	0.000%
86	14.030	4030	4040	4048	rBV5	5619	10152	0.01%	0.007%
87	14.172	4077	4084	4091	rVB	6880	9018	0.01%	0.006%
88	14.239	4096	4105	4107	rBV7	3166	4262	0.00%	0.003%
89	14.332	4132	4134	4138	rVB2	502	233	0.00%	0.000%
90	14.361	4138	4143	4145	rBV3	852	669	0.00%	0.000%
91	14.384	4148	4150	4155	rVB2	512	422	0.00%	0.000%
92	14.413	4155	4159	4161	rBV2	621	443	0.00%	0.000%
93	14.445	4166	4169	4172	rVB2	528	365	0.00%	0.000%
94	14.464	4173	4175	4178	rBV3	309	195	0.00%	0.000%
95	14.516	4189	4191	4196	rBV3	680	616	0.00%	0.000%
96	14.541	4196	4199	4201	rBV2	537	315	0.00%	0.000%
97	14.664	4236	4237	4239	rBV	313	143	0.00%	0.000%
98	14.760	4261	4267	4279	rVB4	4367	6278	0.01%	0.004%
99	14.837	4290	4291	4292	rBV	458	143	0.00%	0.000%
100	15.175	4394	4396	4399	rVB2	853	377	0.00%	0.000%




Sum of corrected areas: 146247947

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033365.D
Acq On : 15 Dec 2023 03:11
Operator : SY/MD
Sample : 05802-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

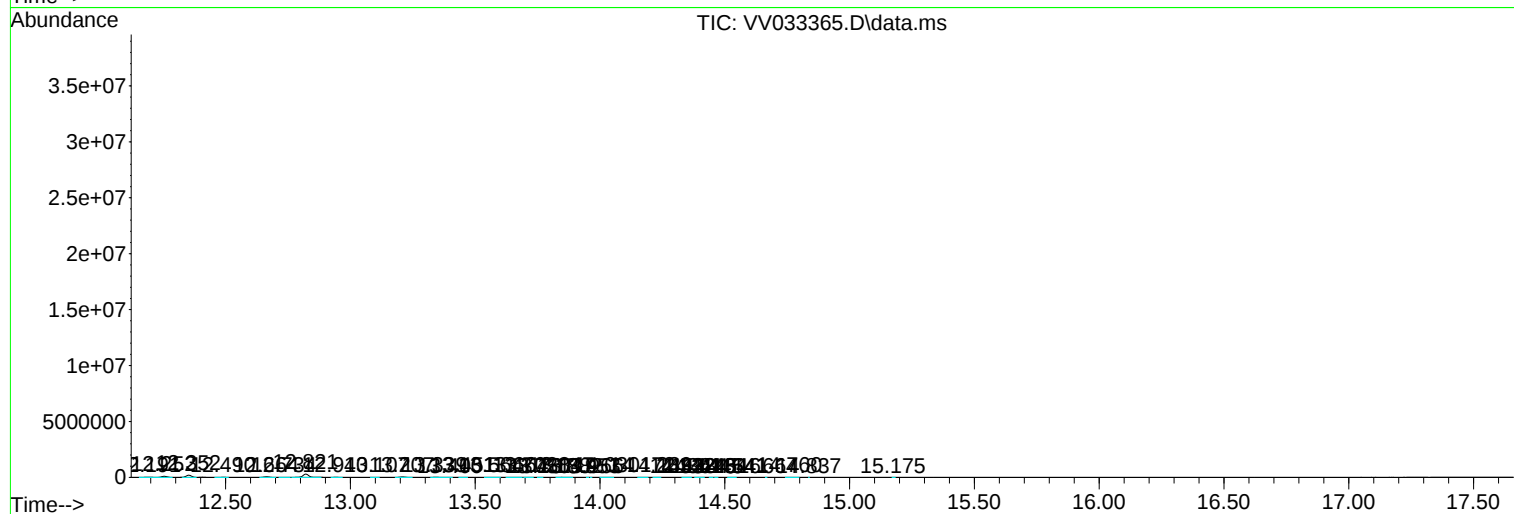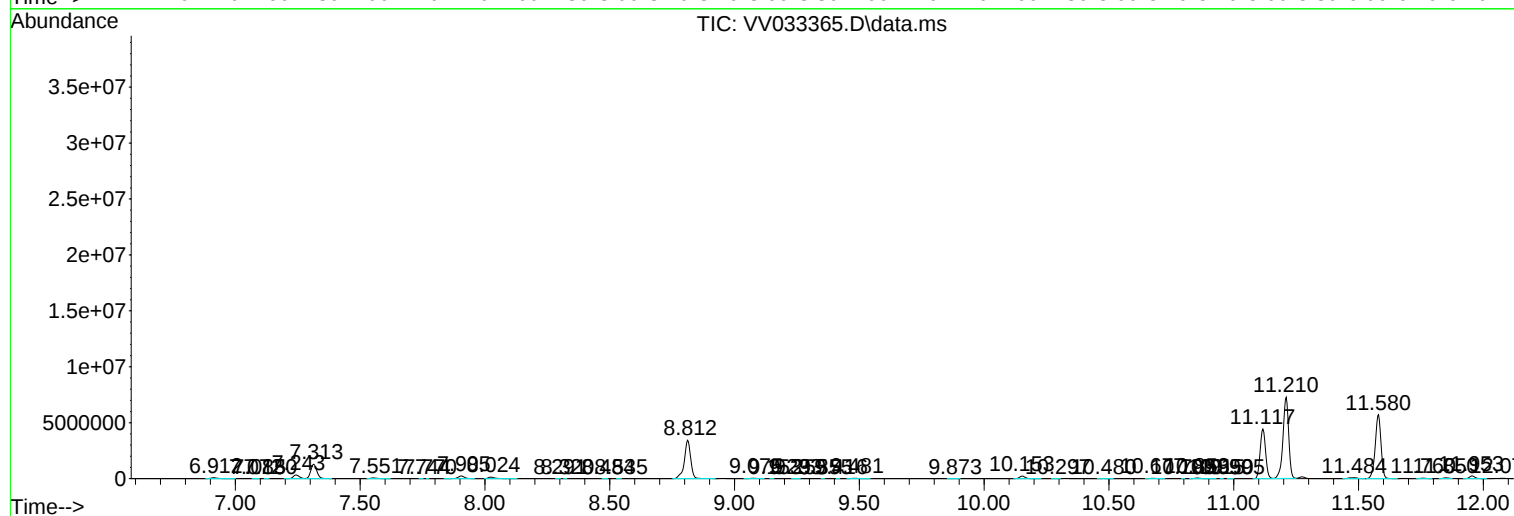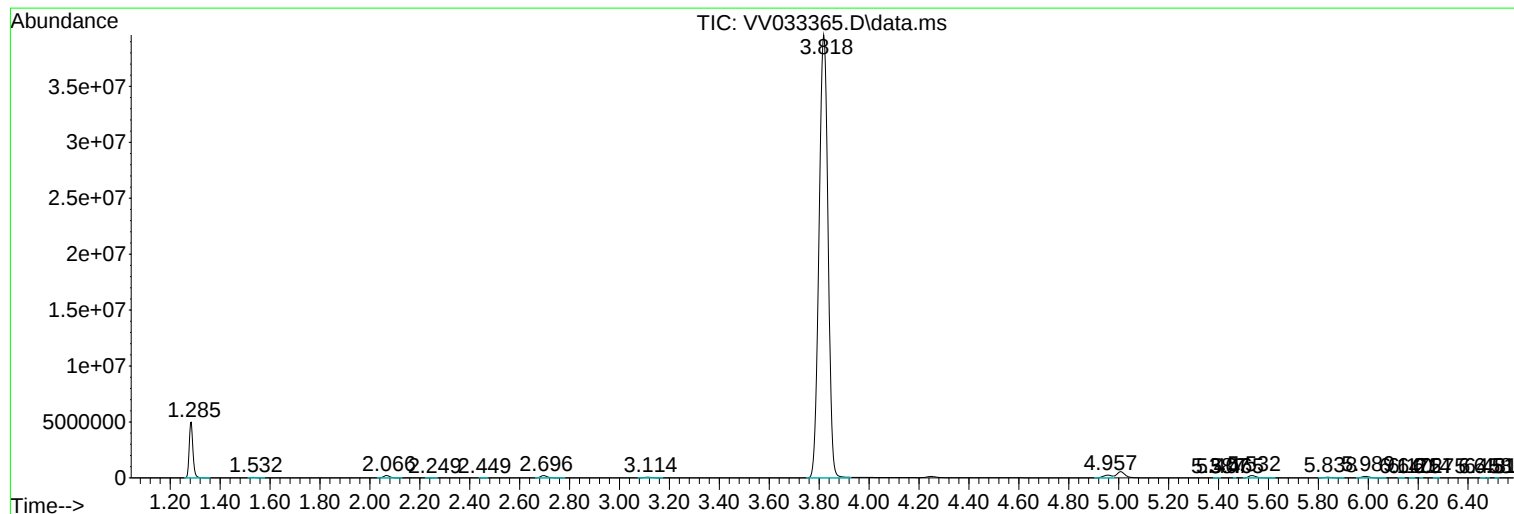

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033365.D
Acq On : 15 Dec 2023 03:11
Operator : SY/MD
Sample : 05802-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033365.D
Acq On : 15 Dec 2023 03:11
Operator : SY/MD
Sample : 05802-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------