

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033367.D
 Acq On : 15 Dec 2023 03:57
 Operator : SY/MD
 Sample : 05802-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	35	40	51	rBV	5643	5878	0.08%	0.038%
2	1.278	67	74	90	rBV2	68901	76061	0.98%	0.495%
3	1.385	104	107	114	rVB2	4011	3818	0.05%	0.025%
4	1.532	146	153	167	rVB	48329	56352	0.73%	0.367%
5	2.060	307	317	336	rVB	105150	154553	2.00%	1.007%
6	2.182	350	355	361	rBV2	1203	1633	0.02%	0.011%
7	2.243	371	374	378	rBV	481	352	0.00%	0.002%
8	2.455	433	440	445	rBB2	603	805	0.01%	0.005%
9	2.558	461	472	491	rBV3	9156	18859	0.24%	0.123%
10	2.703	502	517	537	rBV	146460	302845	3.92%	1.972%
11	2.883	571	573	577	rVB2	446	202	0.00%	0.001%
12	3.021	613	616	618	rBB	163	111	0.00%	0.001%
13	3.111	632	644	664	rBV2	32573	67600	0.87%	0.440%
14	3.211	670	675	678	rBV3	519	490	0.01%	0.003%
15	3.812	845	862	893	rBV2	270738	717951	9.29%	4.676%
16	4.249	982	998	1027	rBV2	110339	284700	3.68%	1.854%
17	4.407	1044	1047	1050	rVB2	555	342	0.00%	0.002%
18	4.433	1052	1055	1058	rBV2	501	322	0.00%	0.002%
19	4.581	1091	1101	1104	rBV4	1384	2120	0.03%	0.014%
20	4.957	1202	1218	1232	rBV3	217301	585511	7.58%	3.813%
21	5.201	1290	1294	1297	rBV	407	341	0.00%	0.002%
22	5.233	1300	1304	1306	rVB2	226	165	0.00%	0.001%
23	5.343	1336	1338	1340	rBV	350	161	0.00%	0.001%
24	5.535	1385	1398	1427	rBV	186168	387613	5.01%	2.524%
25	5.834	1480	1491	1514	rBV2	54078	113465	1.47%	0.739%
26	5.941	1522	1524	1526	rBV	181	116	0.00%	0.001%
27	5.989	1526	1539	1560	rBV2	113254	234234	3.03%	1.525%
28	6.085	1567	1569	1571	rBV	314	116	0.00%	0.001%
29	6.150	1584	1589	1592	rBB3	382	315	0.00%	0.002%
30	6.365	1653	1656	1658	rBB	171	109	0.00%	0.001%
31	6.912	1815	1826	1853	rBV	72262	133173	1.72%	0.867%
32	7.027	1859	1862	1863	rBV	202	116	0.00%	0.001%
33	7.076	1874	1877	1879	rBV2	309	163	0.00%	0.001%
34	7.111	1885	1888	1890	rBV	165	130	0.00%	0.001%
35	7.243	1918	1929	1951	rBV	289467	506228	6.55%	3.297%
36	7.465	1996	1998	2002	rVB2	337	179	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033367.D
 Acq On : 15 Dec 2023 03:57
 Operator : SY/MD
 Sample : 05802-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	7.484	2002	2004	2008	rVB	448	287	0.00%	0.002%
38	7.503	2008	2010	2016	rVB2	295	181	0.00%	0.001%
39	7.555	2016	2026	2050	rBV	52519	92920	1.20%	0.605%
40	7.751	2084	2087	2089	rBB	177	115	0.00%	0.001%
41	7.876	2114	2126	2129	rBV2	7742	12356	0.16%	0.080%
42	8.024	2163	2172	2196	rBV	107230	193070	2.50%	1.257%
43	8.272	2240	2249	2253	rBV3	1390	1809	0.02%	0.012%
44	8.661	2361	2370	2380	rBB2	1448	2222	0.03%	0.014%
45	8.812	2398	2417	2469	rVV	4529811	7729462	100.00%	50.340%
46	9.169	2525	2528	2529	rBV	257	131	0.00%	0.001%
47	9.233	2546	2548	2552	rVB2	485	271	0.00%	0.002%
48	9.320	2571	2575	2577	rBV	345	186	0.00%	0.001%
49	9.416	2602	2605	2611	rBV	217	256	0.00%	0.002%
50	9.442	2611	2613	2618	rVB	293	201	0.00%	0.001%
51	9.484	2621	2626	2629	rBV3	1583	1686	0.02%	0.011%
52	9.870	2738	2746	2760	rBB2	8536	13414	0.17%	0.087%
53	10.111	2814	2821	2824	rBV5	2005	2696	0.03%	0.018%
54	10.153	2824	2834	2860	rVB	194476	308832	4.00%	2.011%
55	10.326	2875	2888	2897	rBV	11733	19038	0.25%	0.124%
56	10.677	2991	2997	3009	rBB5	1181	1882	0.02%	0.012%
57	10.809	3035	3038	3041	rBB	152	125	0.00%	0.001%
58	10.857	3050	3053	3054	rBV	251	133	0.00%	0.001%
59	11.117	3123	3134	3146	rBV	264396	407880	5.28%	2.656%
60	11.207	3146	3162	3190	rVB2	893476	1943133	25.14%	12.655%
61	11.468	3234	3243	3256	rVB2	7524	11073	0.14%	0.072%
62	11.561	3259	3272	3294	rBV2	452093	939460	12.15%	6.118%
63	11.754	3329	3332	3334	rBV	309	250	0.00%	0.002%
64	12.056	3421	3426	3429	rBV2	504	511	0.01%	0.003%
65	12.198	3460	3470	3477	rBB2	3027	4330	0.06%	0.028%
66	12.262	3485	3490	3494	rBB	352	325	0.00%	0.002%
67	12.365	3518	3522	3523	rBB	383	196	0.00%	0.001%
68	12.747	3639	3641	3643	rBB	262	135	0.00%	0.001%
69	12.825	3660	3665	3671	rBV2	1144	1107	0.01%	0.007%
70	13.210	3780	3785	3790	rBB3	580	536	0.01%	0.003%
71	13.268	3802	3803	3805	rVV3	310	119	0.00%	0.001%
72	13.394	3840	3842	3845	rBV	241	141	0.00%	0.001%
73	13.413	3845	3848	3850	rVB	319	177	0.00%	0.001%
74	13.445	3853	3858	3859	rBV	550	405	0.01%	0.003%
75	13.532	3881	3885	3887	rBB	157	128	0.00%	0.001%
76	13.567	3892	3896	3901	rBV	560	630	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033367.D
 Acq On : 15 Dec 2023 03:57
 Operator : SY/MD
 Sample : 05802-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B30

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.590	3901	3903	3905	rVB	353	165	0.00%	0.001%
78	13.689	3930	3934	3936	rBB	301	211	0.00%	0.001%
79	13.812	3970	3972	3975	rBV	161	132	0.00%	0.001%
80	13.847	3978	3983	3985	rBV2	360	214	0.00%	0.001%
81	13.992	4022	4028	4037	rVV3	481	790	0.01%	0.005%
82	14.062	4046	4050	4051	rBV	181	114	0.00%	0.001%
83	14.117	4065	4067	4069	rBV	163	114	0.00%	0.001%
84	14.130	4069	4071	4074	rVV	272	236	0.00%	0.002%
85	14.143	4074	4075	4078	rVB2	378	141	0.00%	0.001%
86	14.165	4078	4082	4083	rBB	243	126	0.00%	0.001%
87	14.175	4083	4085	4087	rBV	229	150	0.00%	0.001%
88	14.188	4087	4089	4093	rVB	384	232	0.00%	0.002%
89	14.220	4093	4099	4101	rBB	529	317	0.00%	0.002%
90	14.265	4110	4113	4115	rBV2	219	125	0.00%	0.001%
91	14.371	4143	4146	4148	rBV	391	237	0.00%	0.002%
92	14.471	4175	4177	4178	rBV	219	106	0.00%	0.001%
93	14.532	4194	4196	4198	rBV	504	238	0.00%	0.002%
94	14.574	4205	4209	4210	rBV2	259	185	0.00%	0.001%
95	14.702	4246	4249	4251	rBV3	384	244	0.00%	0.002%
96	14.734	4256	4259	4260	rBV	214	118	0.00%	0.001%
97	14.760	4265	4267	4273	rBV2	662	729	0.01%	0.005%
98	14.841	4289	4292	4295	rBV3	515	317	0.00%	0.002%
99	14.966	4328	4331	4334	rBV2	482	215	0.00%	0.001%
100	15.397	4463	4465	4467	rBV2	536	261	0.00%	0.002%




Sum of corrected areas: 15354655

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033367.D
Acq On : 15 Dec 2023 03:57
Operator : SY/MD
Sample : 05802-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

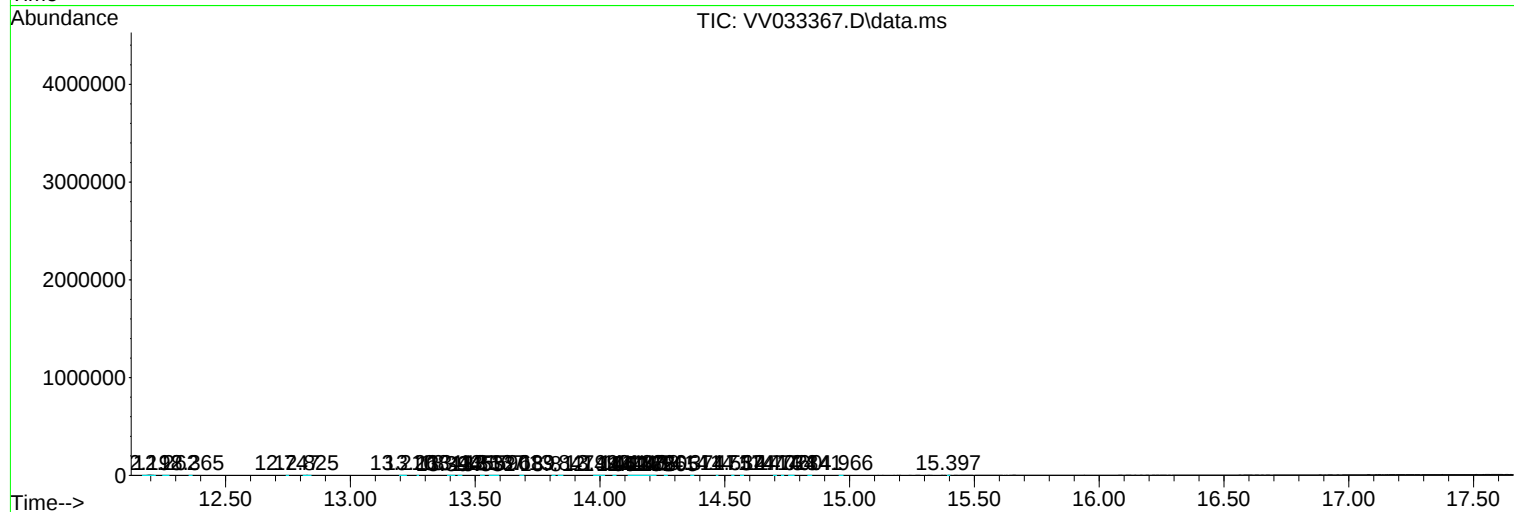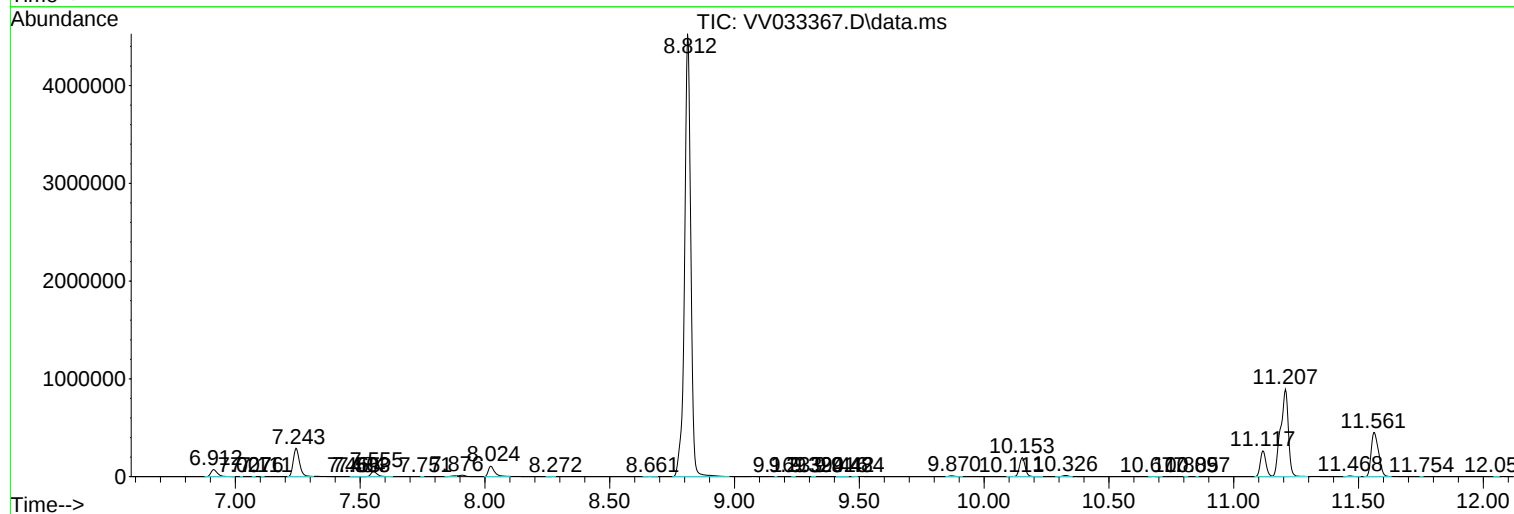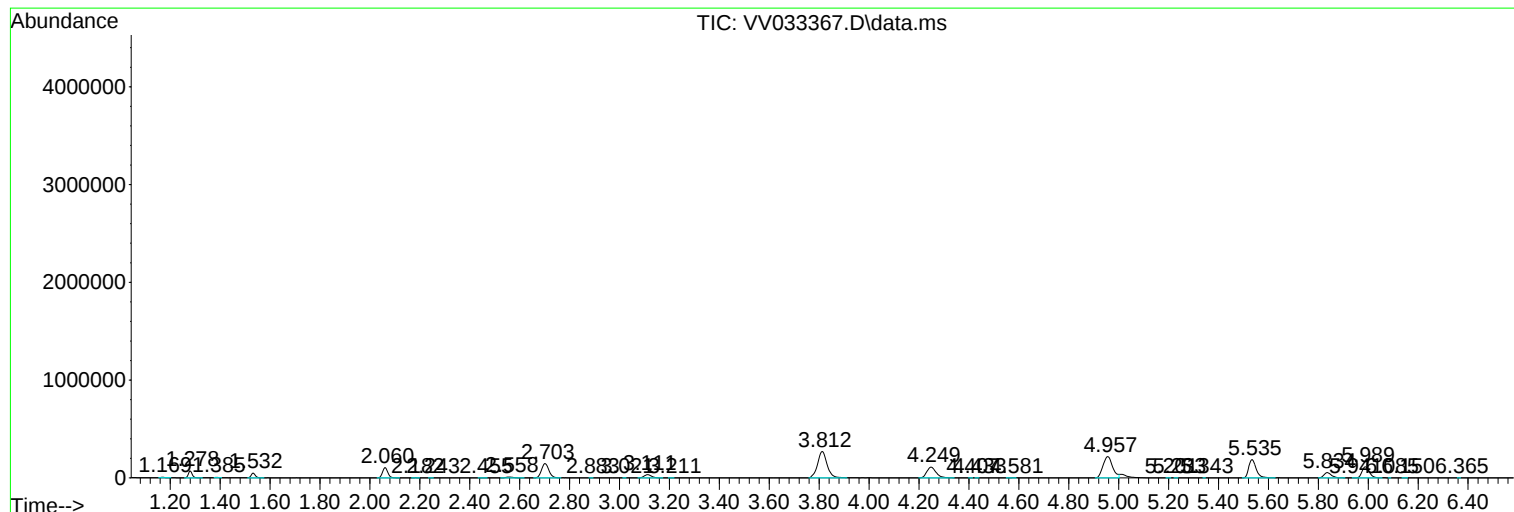

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033367.D
Acq On : 15 Dec 2023 03:57
Operator : SY/MD
Sample : 05802-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033367.D
Acq On : 15 Dec 2023 03:57
Operator : SY/MD
Sample : 05802-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B30

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------