

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121423\
 Data File : VW033369.D
 Acq On : 15 Dec 2023 04:43
 Operator : SY/MD
 Sample : 05802-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VW033369.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.169	35	40	51	rVB	6446	6911	0.21%	0.087%
2	1.281	67	75	88	rBV	61737	64704	1.98%	0.816%
3	1.532	146	153	163	rVB	45954	53077	1.62%	0.669%
4	2.059	307	317	341	rVB	105286	156627	4.79%	1.976%
5	2.182	351	355	362	rBB2	658	876	0.03%	0.011%
6	2.555	465	471	481	rBB	567	983	0.03%	0.012%
7	2.699	511	516	522	rBB2	649	626	0.02%	0.008%
8	3.101	632	641	653	rBB4	2097	4029	0.12%	0.051%
9	3.812	845	862	885	rBV3	54822	188745	5.77%	2.381%
10	4.040	929	933	936	rBV	248	217	0.01%	0.003%
11	4.059	936	939	944	rVB	311	206	0.01%	0.003%
12	4.098	949	951	953	rVB	288	134	0.00%	0.002%
13	4.146	962	966	969	rBB	223	137	0.00%	0.002%
14	4.169	970	973	977	rBB	256	184	0.01%	0.002%
15	4.249	982	998	1024	rBV2	96232	251005	7.68%	3.166%
16	4.419	1049	1051	1055	rBV2	277	170	0.01%	0.002%
17	4.458	1061	1063	1064	rBV	268	147	0.00%	0.002%
18	4.837	1178	1181	1184	rBB	158	129	0.00%	0.002%
19	4.956	1202	1218	1253	rBV2	209884	588408	18.00%	7.421%
20	5.246	1306	1308	1310	rBV2	225	131	0.00%	0.002%
21	5.313	1325	1329	1331	rBV	249	163	0.00%	0.002%
22	5.535	1386	1398	1426	rBV	182392	375153	11.48%	4.732%
23	5.834	1484	1491	1494	rBV4	2404	2815	0.09%	0.036%
24	5.989	1526	1539	1567	rBV	112162	232829	7.12%	2.937%
25	6.140	1582	1586	1587	rBV	295	159	0.00%	0.002%
26	6.911	1815	1826	1848	rBV	67482	125223	3.83%	1.579%
27	7.059	1870	1872	1877	rVB2	302	155	0.00%	0.002%
28	7.243	1918	1929	1955	rBV	280486	494825	15.14%	6.241%
29	7.493	2004	2007	2013	rBB2	495	500	0.02%	0.006%
30	7.554	2016	2026	2044	rBV2	50389	89960	2.75%	1.135%
31	7.712	2071	2075	2077	rVB2	360	212	0.01%	0.003%
32	7.876	2114	2126	2132	rBV2	11132	20104	0.61%	0.254%
33	8.024	2162	2172	2195	rBV	104784	189641	5.80%	2.392%
34	8.259	2243	2245	2247	rBV	251	139	0.00%	0.002%
35	8.271	2247	2249	2253	rVB	365	223	0.01%	0.003%
36	8.291	2253	2255	2257	rBB	280	127	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033369.D
 Acq On : 15 Dec 2023 04:43
 Operator : SY/MD
 Sample : 05802-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	8.786	2398	2409	2414	rBV	307451	511353	15.64%	6.450%
38	9.001	2473	2476	2477	rBB	334	131	0.00%	0.002%
39	9.522	2634	2638	2639	rBV	259	202	0.01%	0.003%
40	9.879	2744	2749	2752	rBB	369	320	0.01%	0.004%
41	10.104	2816	2819	2821	rBV	151	125	0.00%	0.002%
42	10.152	2823	2834	2858	rVB	189765	302406	9.25%	3.814%
43	10.326	2878	2888	2900	rBB2	15759	24911	0.76%	0.314%
44	10.480	2933	2936	2938	rBV	136	120	0.00%	0.002%
45	10.757	3019	3022	3024	rBB	228	118	0.00%	0.001%
46	10.866	3050	3056	3062	rBB	278	308	0.01%	0.004%
47	11.120	3125	3135	3145	rBV	30054	47524	1.45%	0.599%
48	11.184	3145	3155	3181	rVB2	384422	894092	27.35%	11.277%
49	11.387	3215	3218	3219	rVB	332	140	0.00%	0.002%
50	11.471	3236	3244	3250	rBB2	1542	1939	0.06%	0.024%
51	11.577	3260	3277	3302	rBV2	1787061	3268945	100.00%	41.231%
52	11.776	3338	3339	3343	rVB2	364	166	0.01%	0.002%
53	11.799	3344	3346	3347	rBV	332	130	0.00%	0.002%
54	11.837	3354	3358	3362	rBV3	495	496	0.02%	0.006%
55	11.885	3370	3373	3378	rBB2	271	207	0.01%	0.003%
56	11.956	3391	3395	3396	rBV	911	577	0.02%	0.007%
57	12.197	3460	3470	3479	rBB3	3903	5492	0.17%	0.069%
58	12.252	3484	3487	3488	rBV	352	196	0.01%	0.002%
59	12.313	3503	3506	3509	rBB	239	174	0.01%	0.002%
60	12.355	3513	3519	3527	rBB2	971	1582	0.05%	0.020%
61	12.824	3659	3665	3675	rBB2	2080	2674	0.08%	0.034%
62	12.863	3675	3677	3681	rBB	213	126	0.00%	0.002%
63	12.882	3682	3683	3687	rBB	205	119	0.00%	0.002%
64	12.943	3699	3702	3704	rBV	261	187	0.01%	0.002%
65	13.136	3759	3762	3764	rBB	186	120	0.00%	0.002%
66	13.184	3775	3777	3780	rBB	194	124	0.00%	0.002%
67	13.210	3780	3785	3791	rBB3	672	662	0.02%	0.008%
68	13.300	3810	3813	3815	rBB	239	134	0.00%	0.002%
69	13.345	3823	3827	3829	rBB	144	125	0.00%	0.002%
70	13.461	3856	3863	3864	rBV	439	481	0.01%	0.006%
71	13.570	3891	3897	3903	rBV2	795	1039	0.03%	0.013%
72	13.760	3953	3956	3958	rBV	227	146	0.00%	0.002%
73	13.773	3958	3960	3964	rVB	253	155	0.00%	0.002%
74	13.795	3965	3967	3969	rBV	243	146	0.00%	0.002%
75	13.821	3972	3975	3978	rBB2	288	196	0.01%	0.002%
76	13.837	3978	3980	3982	rBV2	466	229	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
 Data File : VV033369.D
 Acq On : 15 Dec 2023 04:43
 Operator : SY/MD
 Sample : 05802-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F7B43

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.850	3982	3984	3986	rVV2	317	152	0.00%	0.002%
78	13.898	3997	3999	4002	rBB2	485	256	0.01%	0.003%
79	13.921	4003	4006	4008	rBV	260	164	0.01%	0.002%
80	14.024	4035	4038	4041	rBV4	533	420	0.01%	0.005%
81	14.056	4046	4048	4050	rVB4	363	137	0.00%	0.002%
82	14.085	4054	4057	4059	rBV	313	207	0.01%	0.003%
83	14.136	4069	4073	4076	rBV2	521	415	0.01%	0.005%
84	14.290	4118	4121	4124	rVB2	429	263	0.01%	0.003%
85	14.310	4124	4127	4134	rBV3	508	596	0.02%	0.008%
86	14.368	4141	4145	4146	rBV	262	154	0.00%	0.002%
87	14.448	4167	4170	4173	rBV2	343	260	0.01%	0.003%
88	14.490	4179	4183	4189	rBB	498	432	0.01%	0.005%
89	14.525	4189	4194	4198	rBV2	640	633	0.02%	0.008%
90	14.561	4202	4205	4211	rBV	352	377	0.01%	0.005%
91	14.606	4215	4219	4220	rBV2	393	271	0.01%	0.003%
92	14.647	4228	4232	4239	rBV3	763	927	0.03%	0.012%
93	14.728	4255	4257	4260	rVB2	435	160	0.00%	0.002%
94	14.763	4261	4268	4276	rBV5	1711	2447	0.07%	0.031%
95	14.802	4276	4280	4284	rBV2	547	531	0.02%	0.007%
96	14.850	4293	4295	4299	rBV	417	269	0.01%	0.003%
97	14.943	4321	4324	4325	rBV	560	318	0.01%	0.004%
98	15.081	4365	4367	4368	rBV2	413	197	0.01%	0.002%
99	15.660	4546	4547	4550	rBV2	846	413	0.01%	0.005%
100	15.750	4573	4575	4577	rBV	911	472	0.01%	0.006%




Sum of corrected areas: 7928462

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033369.D
Acq On : 15 Dec 2023 04:43
Operator : SY/MD
Sample : 05802-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

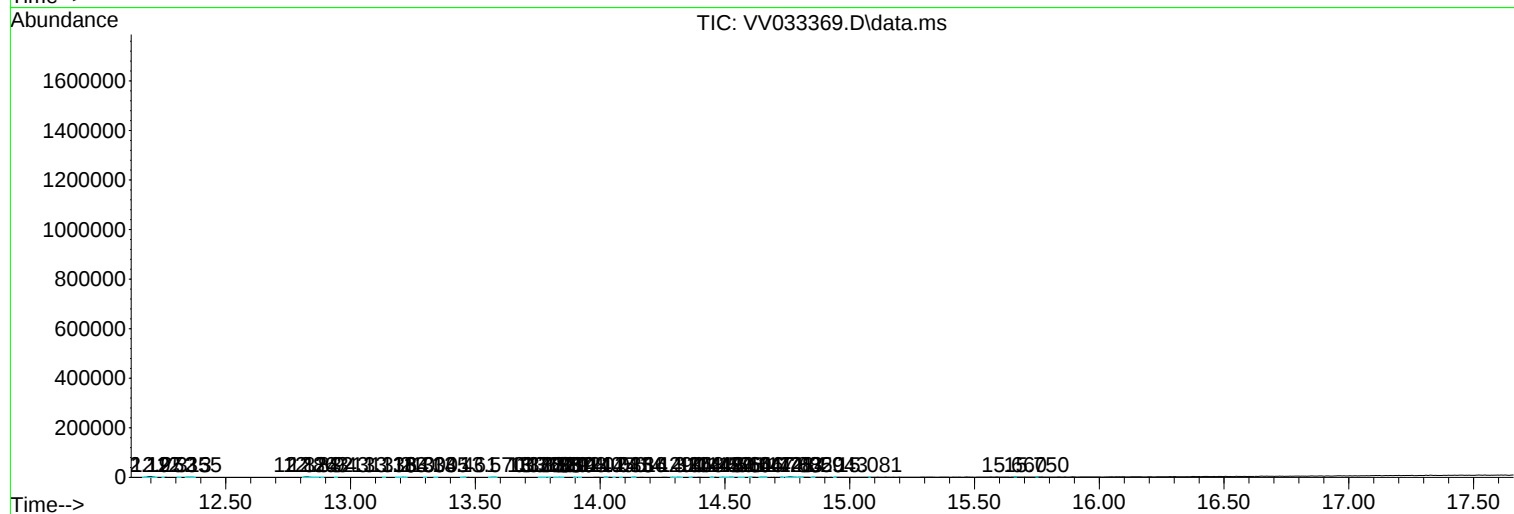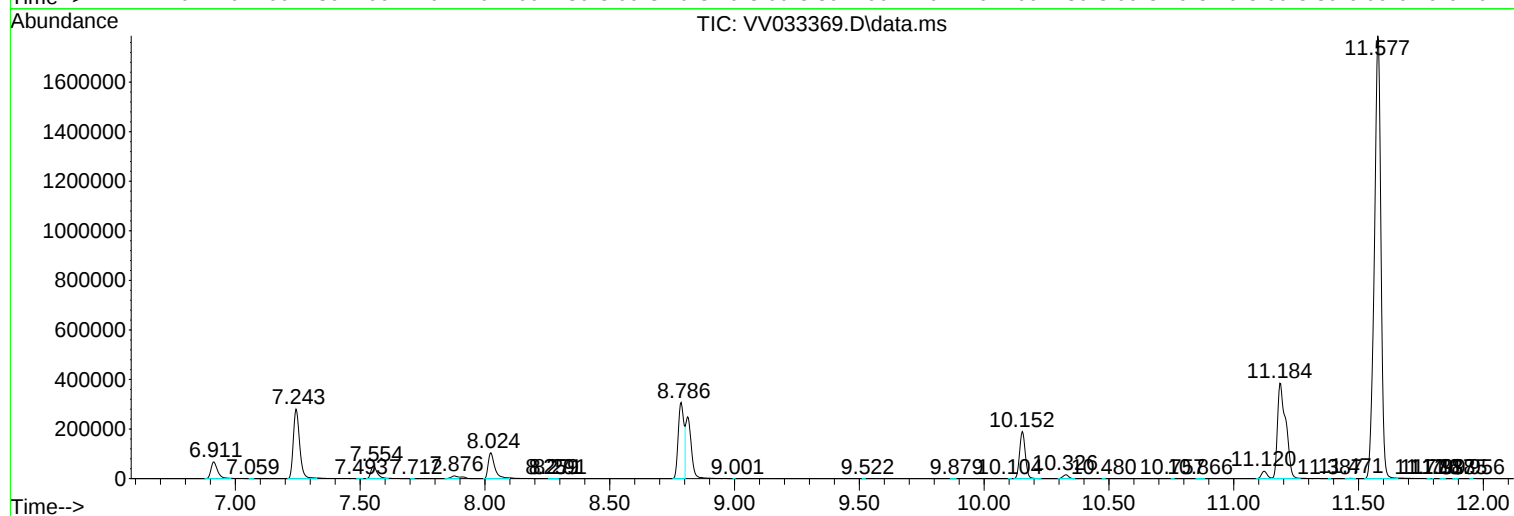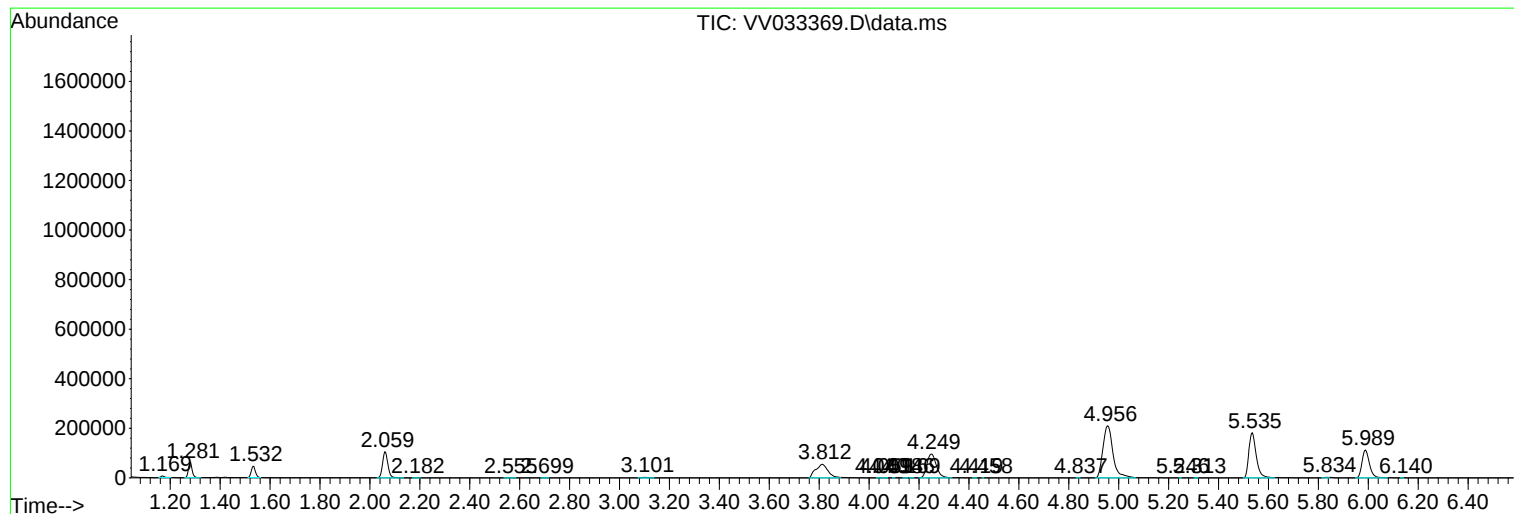

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033369.D
Acq On : 15 Dec 2023 04:43
Operator : SY/MD
Sample : 05802-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033369.D
Acq On : 15 Dec 2023 04:43
Operator : SY/MD
Sample : 05802-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F7B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------