
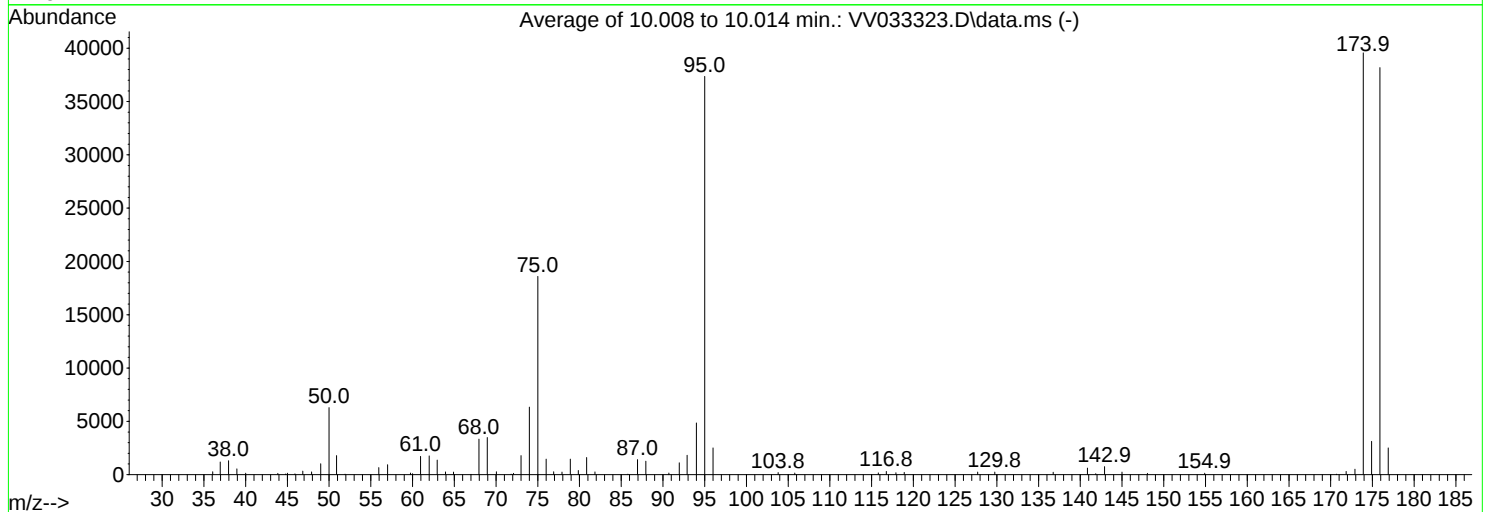


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121423\
Data File : VV033323.D
Acq On : 14 Dec 2023 10:20
Operator : SY/MD
Sample : BFB246
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB246

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis
Last Update : Fri Dec 08 21:51:12 2023

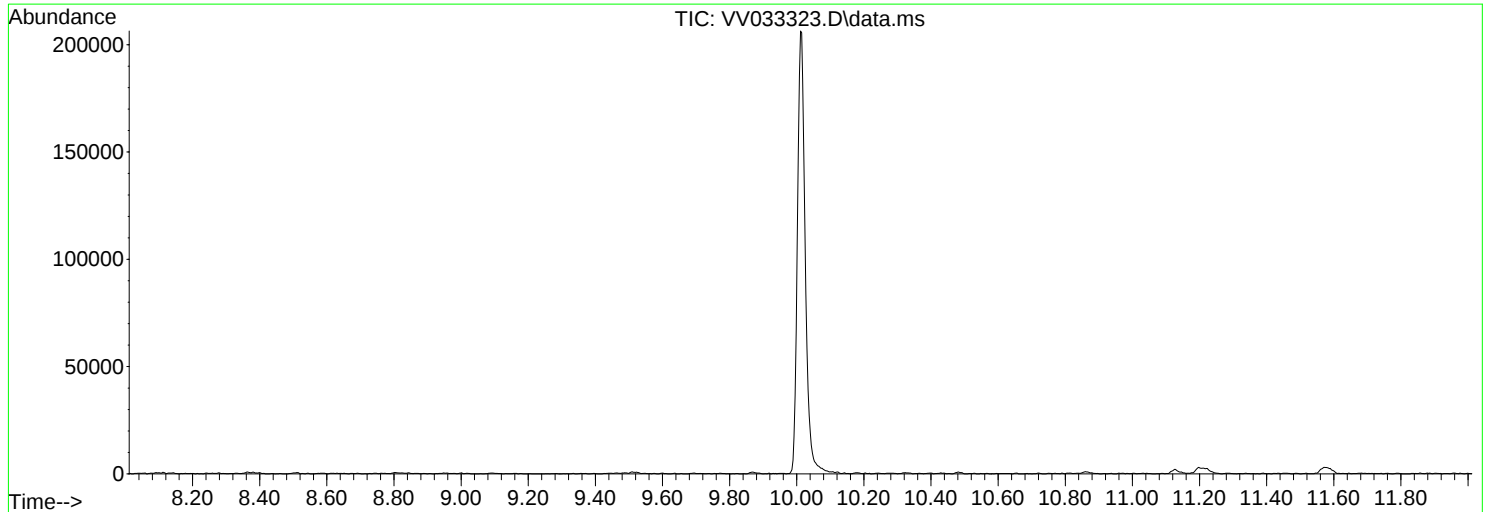

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	6291	PASS
75	95	30	80	49.8	18597	PASS
95	95	100	100	100.0	37357	PASS
96	95	5	9	6.7	2509	PASS
173	174	0.00	2	1.3	507	PASS
174	95	50	120	105.9	39568	PASS
175	174	5	9	7.9	3118	PASS
176	174	95	105	96.5	38189	PASS
177	176	5	10	6.6	2515	PASS

m/z	Abundance
43.90	169.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
36.00	312.0
36.90	1177.0
38.00	1365.0
39.00	456.0
40.00	147.0
43.80	245.0
44.80	191.0
45.90	122.0
46.90	374.0
47.90	241.0
49.00	1037.0
50.00	5734.0
50.90	1641.0
51.90	125.0
56.00	569.0
57.00	816.0
59.70	213.0
60.90	1447.0
62.00	1774.0
63.00	1320.0
64.00	296.0
64.90	254.0
67.90	3061.0
68.90	3398.0
70.00	239.0
71.80	157.0
73.00	1638.0
74.00	6319.0
75.00	18120.0
76.00	1408.0
76.90	212.0
77.90	228.0
78.90	1281.0
79.90	352.0
80.80	1542.0
81.80	252.0
87.00	1302.0
87.90	1145.0
90.60	141.0
92.00	1004.0
92.90	1604.0
94.00	4561.0
95.00	35664.0
96.00	2714.0
103.90	185.0
105.80	150.0
115.80	148.0
116.80	310.0
117.80	159.0
118.90	227.0
127.70	180.0
129.80	255.0
136.70	198.0
140.90	549.0
141.90	162.0
142.90	686.0
145.00	221.0
148.10	116.0
154.90	149.0
171.80	342.0
172.90	560.0
173.90	35344.0
174.90	2893.0
175.90	34320.0
176.90	2411.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
36.10	283.0
36.90	1195.0
38.00	1379.0
39.00	558.0
40.00	152.0
43.90	294.0
45.00	211.0
45.90	110.0
46.80	327.0
47.90	274.0
49.00	1059.0
50.00	6557.0
50.90	1863.0
56.00	718.0
57.00	980.0
59.80	222.0
61.00	1746.0
62.00	1826.0
62.90	1417.0
64.00	258.0
64.90	259.0
68.00	3406.0
69.00	3585.0
70.10	315.0
72.10	192.0
73.00	1888.0
74.00	6583.0
75.00	19328.0
76.00	1490.0
76.90	280.0
77.90	243.0
78.90	1522.0
79.80	405.0
80.80	1672.0
81.80	262.0
85.80	116.0
86.90	1445.0
88.00	1282.0
90.70	154.0
92.00	1143.0
92.90	1924.0
94.00	5061.0
95.00	38624.0
96.00	2613.0
103.80	191.0
105.80	155.0
115.80	178.0
116.70	305.0
117.90	190.0
118.90	209.0
127.70	242.0
129.80	248.0
136.80	244.0
140.80	634.0
141.80	119.0
142.90	761.0
145.00	244.0
148.10	112.0
154.90	136.0
171.90	292.0
172.90	516.0
173.90	40896.0
174.90	3247.0
175.90	39632.0
176.90	2616.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
36.10	220.0
37.00	1203.0
37.90	1192.0
38.90	611.0
40.00	112.0
43.90	343.0
45.00	183.0
46.80	299.0
47.90	268.0
49.00	963.0
50.00	6582.0
50.90	1849.0
55.90	699.0
57.00	984.0
60.00	253.0
61.00	1951.0
62.00	1670.0
62.90	1351.0
63.90	226.0
64.90	228.0
67.00	112.0
68.00	3552.0
69.00	3481.0
70.10	284.0
72.10	196.0
73.00	1855.0
74.00	6122.0
75.00	18344.0
76.00	1474.0
76.90	301.0
77.90	231.0
78.90	1557.0
79.80	405.0
80.90	1618.0
81.90	255.0
86.90	1464.0
88.00	1347.0
90.80	169.0
91.90	1209.0
92.90	1947.0
94.00	4905.0
95.00	37784.0
96.00	2199.0
103.70	197.0
105.80	148.0
115.80	186.0
116.70	302.0
118.00	205.0
118.90	201.0
127.70	279.0
129.70	239.0
136.80	217.0
140.80	675.0
142.90	796.0
145.00	239.0
147.90	113.0
154.90	122.0
170.70	114.0
171.90	275.0
172.90	446.0
173.90	42464.0
174.90	3214.0
175.90	40616.0
176.90	2517.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246