

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019645.D
 Acq On : 15 Dec 2020 13:20
 Operator : SY/MD
 Sample : VV1215WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK69

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	84	rVB	407841	396427	16.00%	2.070%
2	1.569	142	149	160	rBV	299291	334998	13.52%	1.749%
3	2.110	307	317	349	rVB	633202	968092	39.08%	5.055%
4	2.512	433	442	450	rBV6	2670	4946	0.20%	0.026%
5	2.666	484	490	491	rBV3	760	590	0.02%	0.003%
6	2.701	499	501	505	rBV3	781	693	0.03%	0.004%
7	2.917	564	568	569	rBV2	514	334	0.01%	0.002%
8	2.962	579	582	584	rBV2	273	179	0.01%	0.001%
9	3.026	598	602	605	rBV2	822	732	0.03%	0.004%
10	3.148	638	640	642	rBV2	463	229	0.01%	0.001%
11	3.164	642	645	649	rVV2	540	359	0.01%	0.002%
12	3.335	696	698	702	rVB2	411	199	0.01%	0.001%
13	3.354	702	704	706	rBV	205	134	0.01%	0.001%
14	3.373	706	710	716	rVV4	668	710	0.03%	0.004%
15	3.415	718	723	727	rVB3	651	614	0.02%	0.003%
16	3.460	735	737	739	rBV3	407	218	0.01%	0.001%
17	3.544	760	763	765	rBV2	566	420	0.02%	0.002%
18	3.608	781	783	784	rBV2	291	87	0.00%	0.000%
19	3.637	789	792	795	rBV2	357	257	0.01%	0.001%
20	3.675	802	804	806	rBV2	205	115	0.00%	0.001%
21	3.724	813	819	820	rBV	489	471	0.02%	0.002%
22	3.775	833	835	841	rVB3	568	426	0.02%	0.002%
23	3.820	845	849	854	rBV3	363	402	0.02%	0.002%
24	3.884	855	869	908	rBV	170942	520284	21.01%	2.717%
25	4.351	997	1014	1043	rBV	386395	954252	38.53%	4.982%
26	4.978	1207	1209	1211	rBV	254	124	0.01%	0.001%
27	5.048	1211	1231	1263	rBV2	958357	2476910	100.00%	12.933%
28	5.473	1359	1363	1364	rBV2	655	387	0.02%	0.002%
29	5.569	1391	1393	1394	rBV	616	311	0.01%	0.002%
30	5.618	1395	1408	1431	rVV	801890	1591830	64.27%	8.312%
31	5.849	1478	1480	1483	rVB3	860	292	0.01%	0.002%
32	5.907	1487	1498	1518	rVB5	13296	29964	1.21%	0.156%
33	6.071	1535	1549	1572	rBV	547960	1103439	44.55%	5.761%
34	6.293	1614	1618	1620	rBV2	637	486	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019645.D
 Acq On : 15 Dec 2020 13:20
 Operator : SY/MD
 Sample : VV1215WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK69

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.428	1658	1660	1661	rBV	266	69	0.00%	0.000%
36	6.502	1680	1683	1684	rVB	295	116	0.00%	0.001%
37	6.518	1684	1688	1691	rVB2	514	376	0.02%	0.002%
38	6.537	1692	1694	1699	rVB2	395	267	0.01%	0.001%
39	6.753	1757	1761	1762	rBV2	577	298	0.01%	0.002%
40	6.781	1768	1770	1773	rBV2	453	302	0.01%	0.002%
41	6.801	1773	1776	1779	rVB	521	232	0.01%	0.001%
42	6.836	1779	1787	1789	rBV4	554	545	0.02%	0.003%
43	6.849	1789	1791	1795	rVB	673	415	0.02%	0.002%
44	6.871	1795	1798	1799	rBV	142	75	0.00%	0.000%
45	6.884	1799	1802	1806	rBV3	432	350	0.01%	0.002%
46	6.917	1806	1812	1818	rBV5	764	837	0.03%	0.004%
47	6.987	1821	1834	1859	rBV	330243	594155	23.99%	3.102%
48	7.315	1924	1936	1962	rBV	1136785	1986486	80.20%	10.372%
49	7.621	2021	2031	2059	rBV	224677	398536	16.09%	2.081%
50	7.900	2114	2118	2121	rBV3	626	577	0.02%	0.003%
51	7.981	2137	2143	2155	rVB6	2035	3520	0.14%	0.018%
52	8.048	2161	2164	2166	rBV2	378	253	0.01%	0.001%
53	8.087	2166	2176	2205	rBV	625425	1099270	44.38%	5.740%
54	8.630	2343	2345	2346	rBV2	486	185	0.01%	0.001%
55	8.852	2402	2414	2444	rBV	1187862	1940141	78.33%	10.130%
56	9.219	2525	2528	2532	rVB2	769	570	0.02%	0.003%
57	9.415	2587	2589	2590	rBV2	305	161	0.01%	0.001%
58	9.437	2594	2596	2599	rVV3	424	182	0.01%	0.001%
59	9.502	2614	2616	2619	rBV2	219	126	0.01%	0.001%
60	9.669	2666	2668	2671	rVB2	414	150	0.01%	0.001%
61	9.752	2692	2694	2697	rBV	464	338	0.01%	0.002%
62	9.817	2712	2714	2716	rVB	662	242	0.01%	0.001%
63	9.839	2716	2721	2723	rBV3	447	358	0.01%	0.002%
64	9.897	2737	2739	2743	rVB	330	156	0.01%	0.001%
65	10.048	2782	2786	2787	rBV	398	284	0.01%	0.001%
66	10.077	2794	2795	2796	rBV	422	161	0.01%	0.001%
67	10.125	2808	2810	2811	rBV	444	197	0.01%	0.001%
68	10.164	2820	2822	2825	rVB2	679	337	0.01%	0.002%
69	10.219	2827	2839	2863	rVV	675788	1044566	42.17%	5.454%
70	10.421	2900	2902	2903	rBV	319	136	0.01%	0.001%
71	10.624	2963	2965	2969	rBV	394	232	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019645.D
 Acq On : 15 Dec 2020 13:20
 Operator : SY/MD
 Sample : VV1215WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK69

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.817	3021	3025	3028	rBV3	551	444	0.02%	0.002%
73	10.920	3055	3057	3060	rBV4	624	333	0.01%	0.002%
74	11.019	3086	3088	3091	rVB3	629	274	0.01%	0.001%
75	11.061	3100	3101	3103	rBV	312	178	0.01%	0.001%
76	11.087	3107	3109	3111	rBV	403	212	0.01%	0.001%
77	11.103	3111	3114	3118	rVB3	779	550	0.02%	0.003%
78	11.254	3149	3161	3190	rBV	1260320	1920697	77.54%	10.029%
79	11.627	3264	3277	3297	rBV	1118613	1761559	71.12%	9.198%
80	11.965	3379	3382	3385	rBV4	498	349	0.01%	0.002%
81	12.135	3432	3435	3437	rBV	583	345	0.01%	0.002%
82	12.212	3458	3459	3461	rBV2	378	136	0.01%	0.001%
83	12.289	3479	3483	3485	rBV2	586	482	0.02%	0.003%
84	12.498	3544	3548	3549	rBV2	440	264	0.01%	0.001%
85	12.585	3571	3575	3577	rBV3	644	463	0.02%	0.002%
86	12.710	3611	3614	3616	rBV	528	347	0.01%	0.002%
87	13.141	3746	3748	3751	rBV	562	347	0.01%	0.002%


Sum of corrected areas: 19152092

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121520\
Data File : VV019645.D
Acq On : 15 Dec 2020 13:20
Operator : SY/MD
Sample : VV1215WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK69

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

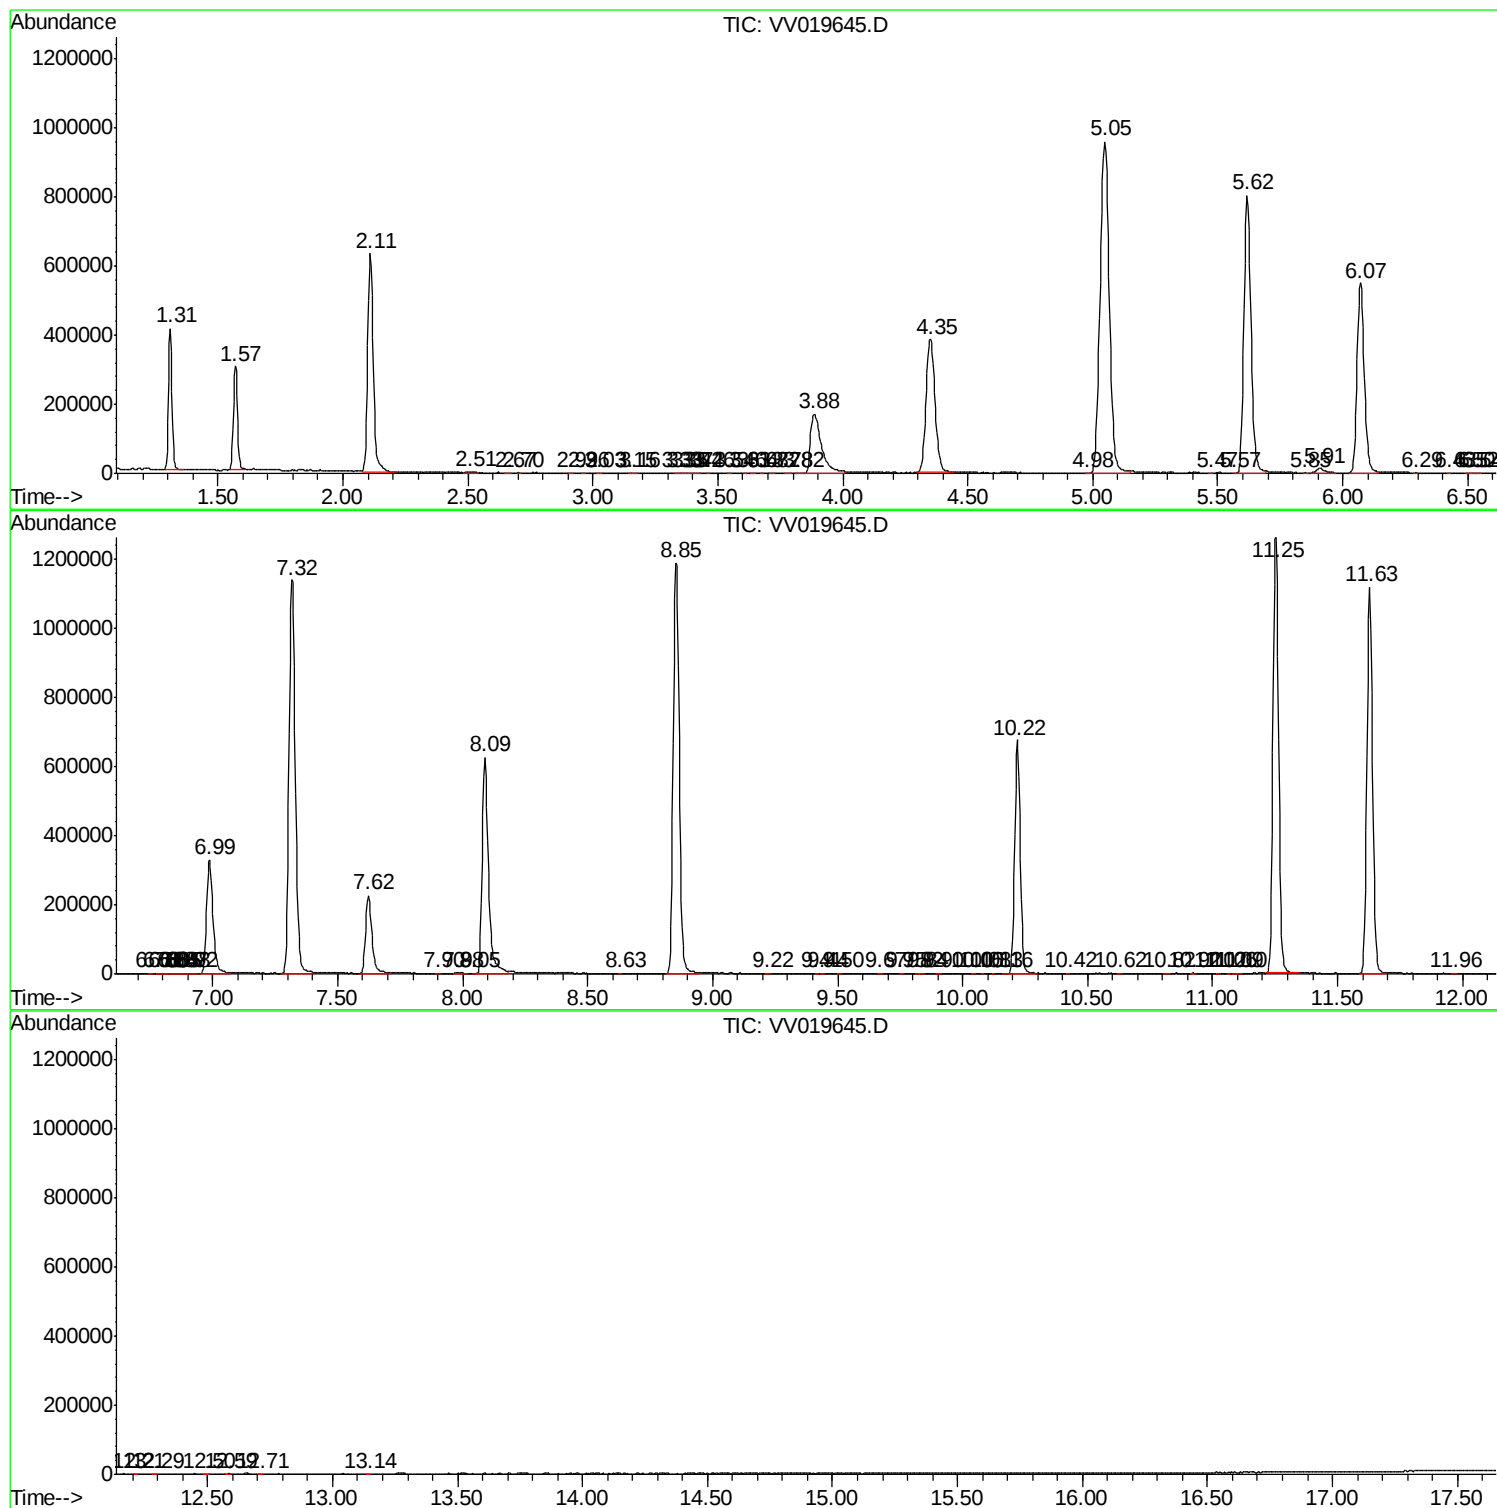

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121520\
Data File : VV019645.D
Acq On : 15 Dec 2020 13:20
Operator : SY/MD
Sample : VV1215WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK69

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121520\
Data File : VV019645.D
Acq On : 15 Dec 2020 13:20
Operator : SY/MD
Sample : VV1215WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK69

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc