

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019646.D
 Acq On : 15 Dec 2020 13:55
 Operator : SY/MD
 Sample : L5099-01 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	82	rVB	404127	406757	8.20%	1.652%
2	1.569	142	149	163	rVB	308639	352274	7.10%	1.431%
3	2.110	307	317	355	rVB	637843	979082	19.75%	3.977%
4	2.724	506	508	510	rBV2	449	205	0.00%	0.001%
5	3.003	593	595	598	rBV2	440	246	0.00%	0.001%
6	3.048	598	609	619	rVV8	2650	5856	0.12%	0.024%
7	3.158	640	643	644	rBV2	434	211	0.00%	0.001%
8	3.254	668	673	676	rBV4	642	547	0.01%	0.002%
9	3.270	676	678	680	rBV3	658	379	0.01%	0.002%
10	3.376	706	711	712	rBV3	408	340	0.01%	0.001%
11	3.425	720	726	728	rBV3	688	626	0.01%	0.003%
12	3.460	735	737	741	rVB2	410	208	0.00%	0.001%
13	3.531	756	759	761	rBV2	523	373	0.01%	0.002%
14	3.563	764	769	770	rBV2	442	329	0.01%	0.001%
15	3.608	781	783	785	rBV	273	68	0.00%	0.000%
16	3.637	788	792	796	rBV4	463	414	0.01%	0.002%
17	3.663	796	800	801	rBV	443	350	0.01%	0.001%
18	3.695	809	810	811	rBV	265	60	0.00%	0.000%
19	3.836	852	854	855	rBV	398	128	0.00%	0.001%
20	3.894	860	872	921	rBV2	158894	552484	11.14%	2.244%
21	4.351	998	1014	1040	rBV	398486	976195	19.69%	3.966%
22	4.830	1160	1163	1165	rBV	592	381	0.01%	0.002%
23	4.843	1165	1167	1171	rVV3	597	561	0.01%	0.002%
24	4.871	1174	1176	1179	rVB3	610	310	0.01%	0.001%
25	4.891	1179	1182	1183	rBV	347	160	0.00%	0.001%
26	5.048	1208	1231	1264	rBV2	987415	2529766	51.02%	10.276%
27	5.457	1356	1358	1359	rBV	502	187	0.00%	0.001%
28	5.531	1376	1381	1383	rBV3	511	524	0.01%	0.002%
29	5.560	1386	1390	1393	rBV4	576	560	0.01%	0.002%
30	5.617	1395	1408	1435	rBV	811356	1620544	32.68%	6.583%
31	5.916	1489	1501	1522	rBV3	70006	150359	3.03%	0.611%
32	6.071	1533	1549	1575	rBV	553661	1130962	22.81%	4.594%
33	6.325	1626	1628	1632	rBV3	434	223	0.00%	0.001%
34	6.363	1637	1640	1643	rBV3	664	525	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019646.D
 Acq On : 15 Dec 2020 13:55
 Operator : SY/MD
 Sample : L5099-01 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.476	1671	1675	1676	rBV	234	157	0.00%	0.001%
36	6.540	1691	1695	1698	rBV2	339	216	0.00%	0.001%
37	6.556	1698	1700	1701	rBV	390	142	0.00%	0.001%
38	6.598	1707	1713	1716	rBV3	692	847	0.02%	0.003%
39	6.688	1739	1741	1742	rBV2	343	144	0.00%	0.001%
40	6.720	1746	1751	1755	rVB3	545	519	0.01%	0.002%
41	6.775	1766	1768	1770	rVB2	419	170	0.00%	0.001%
42	6.797	1771	1775	1778	rBV3	376	324	0.01%	0.001%
43	6.826	1782	1784	1788	rBV3	311	227	0.00%	0.001%
44	6.887	1800	1803	1805	rBV	339	178	0.00%	0.001%
45	6.910	1808	1810	1815	rBV3	360	391	0.01%	0.002%
46	6.987	1822	1834	1858	rBV	338123	608479	12.27%	2.472%
47	7.315	1924	1936	1963	rBV	1155866	2016737	40.67%	8.192%
48	7.621	2020	2031	2052	rBV	232965	405883	8.19%	1.649%
49	7.977	2128	2142	2164	rBV	3000190	4958215	100.00%	20.141%
50	8.090	2167	2177	2214	rVB	638027	1121141	22.61%	4.554%
51	8.518	2304	2310	2314	rBV6	1118	1415	0.03%	0.006%
52	8.785	2390	2393	2399	rBV4	615	714	0.01%	0.003%
53	8.855	2403	2415	2444	rVV	1204307	1966589	39.66%	7.989%
54	9.151	2501	2507	2513	rBV5	1248	1548	0.03%	0.006%
55	9.206	2522	2524	2527	rBV2	611	350	0.01%	0.001%
56	9.315	2555	2558	2563	rVB3	478	341	0.01%	0.001%
57	9.338	2563	2565	2569	rBV4	283	196	0.00%	0.001%
58	9.357	2569	2571	2573	rVB3	602	251	0.01%	0.001%
59	9.370	2573	2575	2576	rBV	388	203	0.00%	0.001%
60	9.395	2582	2583	2584	rBV	447	157	0.00%	0.001%
61	9.424	2589	2592	2598	rVB5	692	600	0.01%	0.002%
62	9.534	2622	2626	2628	rBV3	519	313	0.01%	0.001%
63	9.707	2676	2680	2682	rBV3	490	343	0.01%	0.001%
64	9.720	2682	2684	2686	rVV	309	128	0.00%	0.001%
65	9.920	2744	2746	2749	rBV2	428	265	0.01%	0.001%
66	9.942	2751	2753	2757	rVB3	512	320	0.01%	0.001%
67	10.016	2774	2776	2778	rBV	348	218	0.00%	0.001%
68	10.055	2783	2788	2793	rVV4	570	669	0.01%	0.003%
69	10.087	2793	2798	2801	rBV4	462	506	0.01%	0.002%
70	10.141	2813	2815	2817	rBV2	310	112	0.00%	0.000%
71	10.219	2827	2839	2864	rBV	681453	1079801	21.78%	4.386%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019646.D
 Acq On : 15 Dec 2020 13:55
 Operator : SY/MD
 Sample : L5099-01 200X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4M9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.566	2945	2947	2948	rBV	467	180	0.00%	0.001%
73	10.678	2981	2982	2983	rBV	315	114	0.00%	0.000%
74	10.691	2983	2986	2990	rVV4	755	489	0.01%	0.002%
75	10.717	2992	2994	2998	rBV3	481	323	0.01%	0.001%
76	10.746	2999	3003	3004	rBV2	471	348	0.01%	0.001%
77	10.858	3035	3038	3042	rVB5	1141	848	0.02%	0.003%
78	10.903	3050	3052	3053	rBV	349	119	0.00%	0.000%
79	10.923	3053	3058	3060	rBV3	862	968	0.02%	0.004%
80	11.026	3088	3090	3091	rBV	232	92	0.00%	0.000%
81	11.254	3149	3161	3186	rBV	1250686	1929453	38.91%	7.838%
82	11.630	3266	3278	3298	rBV	1154192	1799622	36.30%	7.310%
83	11.981	3385	3387	3388	rBV	577	230	0.00%	0.001%
84	12.022	3396	3400	3404	rVB	536	410	0.01%	0.002%
85	12.051	3407	3409	3411	rBV2	471	197	0.00%	0.001%
86	12.090	3419	3421	3425	rBV4	616	473	0.01%	0.002%
87	12.180	3447	3449	3451	rBV2	442	197	0.00%	0.001%
88	12.235	3464	3466	3467	rBV2	344	119	0.00%	0.000%
89	12.280	3478	3480	3483	rBV2	534	299	0.01%	0.001%
90	12.717	3614	3616	3619	rBV3	491	274	0.01%	0.001%
91	12.804	3640	3643	3648	rBV3	788	740	0.01%	0.003%
92	14.196	4074	4076	4078	rBV2	616	274	0.01%	0.001%
93	14.241	4088	4090	4093	rBV2	575	387	0.01%	0.002%


Sum of corrected areas: 24617159

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121520\
Data File : VV019646.D
Acq On : 15 Dec 2020 13:55
Operator : SY/MD
Sample : L5099-01 200X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4M9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

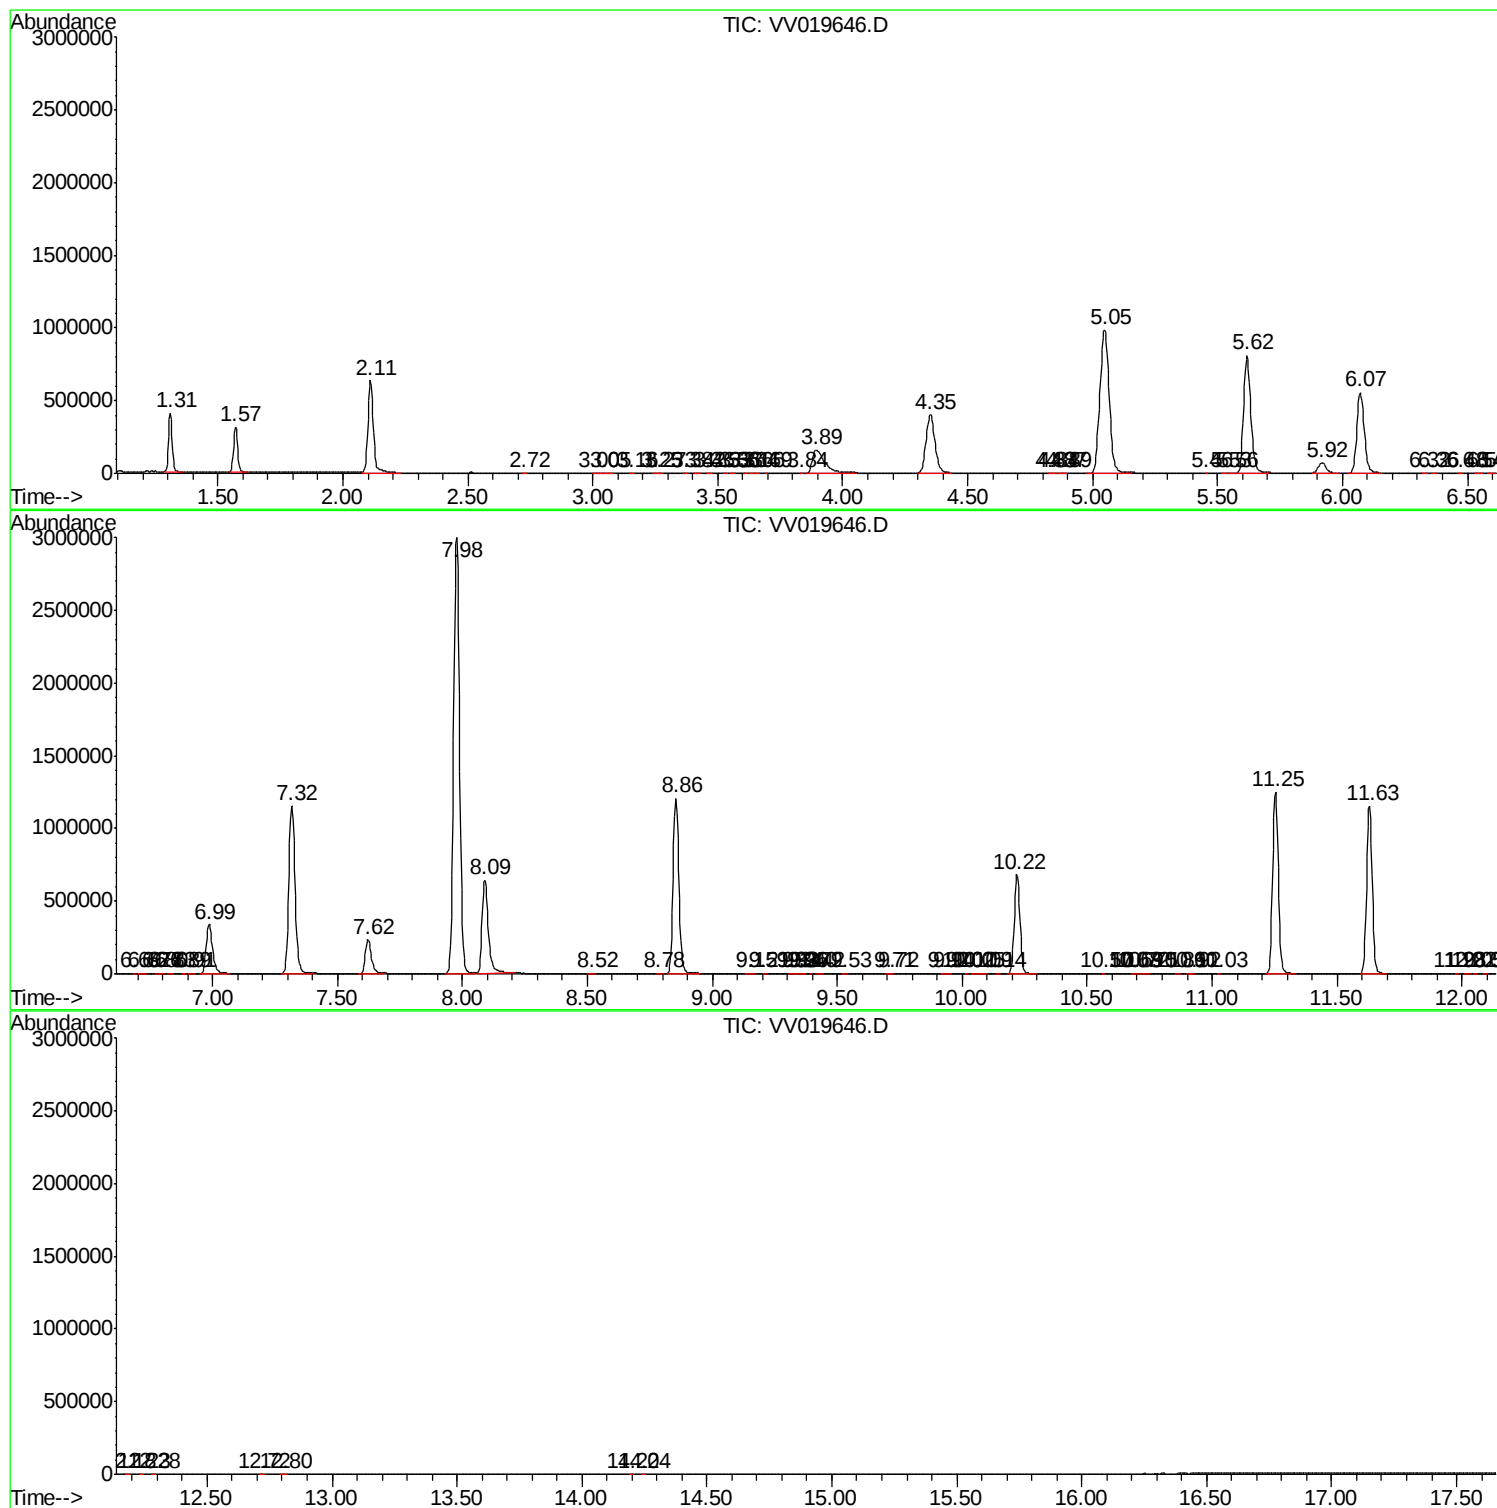

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121520\
Data File : VV019646.D
Acq On : 15 Dec 2020 13:55
Operator : SY/MD
Sample : L5099-01 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4M9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121520\
Data File : VV019646.D
Acq On : 15 Dec 2020 13:55
Operator : SY/MD
Sample : L5099-01 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4M9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc