

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019647.D
 Acq On : 15 Dec 2020 14:19
 Operator : SY/MD
 Sample : VIBLK63
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	81	rVB	400917	400298	15.83%	2.071%
2	1.573	142	150	160	rBV	310504	349152	13.81%	1.807%
3	2.113	308	318	349	rVB	627840	975363	38.58%	5.047%
4	2.560	454	457	460	rBV3	891	798	0.03%	0.004%
5	2.669	488	491	494	rBV2	681	506	0.02%	0.003%
6	2.974	582	586	589	rBV4	520	506	0.02%	0.003%
7	3.113	626	629	630	rBV4	274	152	0.01%	0.001%
8	3.154	640	642	645	rBV3	690	346	0.01%	0.002%
9	3.183	648	651	652	rBV2	453	237	0.01%	0.001%
10	3.225	660	664	666	rBV2	582	391	0.02%	0.002%
11	3.335	696	698	702	rBV2	559	361	0.01%	0.002%
12	3.441	729	731	732	rBV2	497	232	0.01%	0.001%
13	3.482	742	744	746	rBV2	463	236	0.01%	0.001%
14	3.595	777	779	781	rBV2	307	147	0.01%	0.001%
15	3.637	788	792	793	rBV2	361	235	0.01%	0.001%
16	3.695	808	810	814	rVB2	727	453	0.02%	0.002%
17	3.717	814	817	821	rBV2	650	508	0.02%	0.003%
18	3.736	821	823	825	rVB3	331	163	0.01%	0.001%
19	3.762	829	831	835	rBV2	738	678	0.03%	0.004%
20	3.798	839	842	845	rBV3	574	374	0.01%	0.002%
21	3.839	853	855	860	rVB3	608	339	0.01%	0.002%
22	3.891	860	871	912	rBV	186604	583554	23.08%	3.020%
23	4.354	1000	1015	1040	rBV	397424	968762	38.31%	5.013%
24	4.900	1183	1185	1187	rVB2	445	196	0.01%	0.001%
25	4.920	1187	1191	1195	rVV5	392	422	0.02%	0.002%
26	4.939	1195	1197	1200	rVB2	591	291	0.01%	0.002%
27	5.051	1214	1232	1262	rBV2	984669	2528454	100.00%	13.084%
28	5.399	1338	1340	1342	rBV3	584	353	0.01%	0.002%
29	5.621	1395	1409	1434	rBV	776519	1542544	61.01%	7.982%
30	5.910	1489	1499	1515	rBV2	13237	28974	1.15%	0.150%
31	6.074	1535	1550	1578	rBV	564386	1139593	45.07%	5.897%
32	6.408	1651	1654	1656	rBV3	373	240	0.01%	0.001%
33	6.514	1683	1687	1690	rVB2	254	244	0.01%	0.001%
34	6.534	1690	1693	1696	rBV2	645	460	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019647.D
 Acq On : 15 Dec 2020 14:19
 Operator : SY/MD
 Sample : VIBLK63
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.550	1696	1698	1699	rBV	288	121	0.00%	0.001%
36	6.576	1704	1706	1708	rVV	552	309	0.01%	0.002%
37	6.601	1712	1714	1717	rVB2	581	285	0.01%	0.001%
38	6.720	1748	1751	1752	rBV3	436	224	0.01%	0.001%
39	6.736	1754	1756	1758	rVB3	337	118	0.00%	0.001%
40	6.833	1784	1786	1788	rBV2	274	144	0.01%	0.001%
41	6.897	1802	1806	1810	rVB3	437	334	0.01%	0.002%
42	6.923	1810	1814	1822	rBV4	747	972	0.04%	0.005%
43	6.987	1822	1834	1869	rBV	335209	612823	24.24%	3.171%
44	7.318	1925	1937	1963	rBV	1179223	2012500	79.59%	10.414%
45	7.624	2022	2032	2060	rBV	233047	401027	15.86%	2.075%
46	7.842	2098	2100	2106	rVB4	662	604	0.02%	0.003%
47	7.881	2108	2112	2114	rBV3	429	280	0.01%	0.001%
48	7.981	2133	2143	2154	rBV7	7017	11519	0.46%	0.060%
49	8.090	2166	2177	2213	rBV	690951	1202867	47.57%	6.225%
50	8.588	2331	2332	2334	rBV	642	265	0.01%	0.001%
51	8.855	2403	2415	2438	rBV	1164999	1857943	73.48%	9.614%
52	9.244	2534	2536	2538	rBV2	460	172	0.01%	0.001%
53	9.260	2538	2541	2544	rBV2	562	466	0.02%	0.002%
54	9.305	2552	2555	2560	rBV5	472	406	0.02%	0.002%
55	9.370	2572	2575	2580	rBV2	443	440	0.02%	0.002%
56	9.447	2597	2599	2601	rBV2	199	111	0.00%	0.001%
57	9.469	2604	2606	2607	rBV	408	149	0.01%	0.001%
58	9.598	2643	2646	2649	rBV2	447	354	0.01%	0.002%
59	9.665	2662	2667	2669	rBV2	597	493	0.02%	0.003%
60	9.717	2680	2683	2686	rBV2	466	363	0.01%	0.002%
61	9.749	2691	2693	2695	rBV	212	110	0.00%	0.001%
62	9.765	2695	2698	2700	rBV3	900	508	0.02%	0.003%
63	9.804	2705	2710	2711	rBV	492	342	0.01%	0.002%
64	9.846	2721	2723	2730	rVB4	433	432	0.02%	0.002%
65	9.907	2740	2742	2744	rBV3	547	268	0.01%	0.001%
66	9.968	2759	2761	2763	rBV2	311	164	0.01%	0.001%
67	10.067	2787	2792	2794	rBV2	720	636	0.03%	0.003%
68	10.100	2799	2802	2804	rBV2	379	216	0.01%	0.001%
69	10.218	2825	2839	2857	rBV	698814	1104629	43.69%	5.716%
70	10.415	2898	2900	2901	rBV	290	87	0.00%	0.000%
71	10.479	2917	2920	2923	rBV3	702	345	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019647.D
 Acq On : 15 Dec 2020 14:19
 Operator : SY/MD
 Sample : VIBLK63
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.495	2923	2925	2928	rVB2	330	165	0.01%	0.001%
73	10.527	2933	2935	2939	rBV4	588	546	0.02%	0.003%
74	10.636	2967	2969	2971	rBV2	398	190	0.01%	0.001%
75	10.685	2982	2984	2986	rBV	360	141	0.01%	0.001%
76	10.964	3068	3071	3073	rBV2	275	168	0.01%	0.001%
77	11.087	3105	3109	3115	rVB6	703	546	0.02%	0.003%
78	11.122	3116	3120	3124	rBV2	543	381	0.02%	0.002%
79	11.141	3124	3126	3129	rVB2	573	304	0.01%	0.002%
80	11.161	3130	3132	3133	rBV	389	130	0.01%	0.001%
81	11.170	3133	3135	3136	rBV	743	354	0.01%	0.002%
82	11.254	3149	3161	3180	rBV	1180970	1801592	71.25%	9.323%
83	11.630	3265	3278	3303	rBV	1138263	1779741	70.39%	9.210%
84	11.791	3325	3328	3332	rBV2	1087	749	0.03%	0.004%
85	12.386	3511	3513	3516	rBV3	687	465	0.02%	0.002%
86	12.514	3551	3553	3557	rBV2	447	273	0.01%	0.001%
87	12.685	3604	3606	3608	rBV2	261	118	0.00%	0.001%


Sum of corrected areas: 19324451

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121520\
Data File : VV019647.D
Acq On : 15 Dec 2020 14:19
Operator : SY/MD
Sample : VIBLK63
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

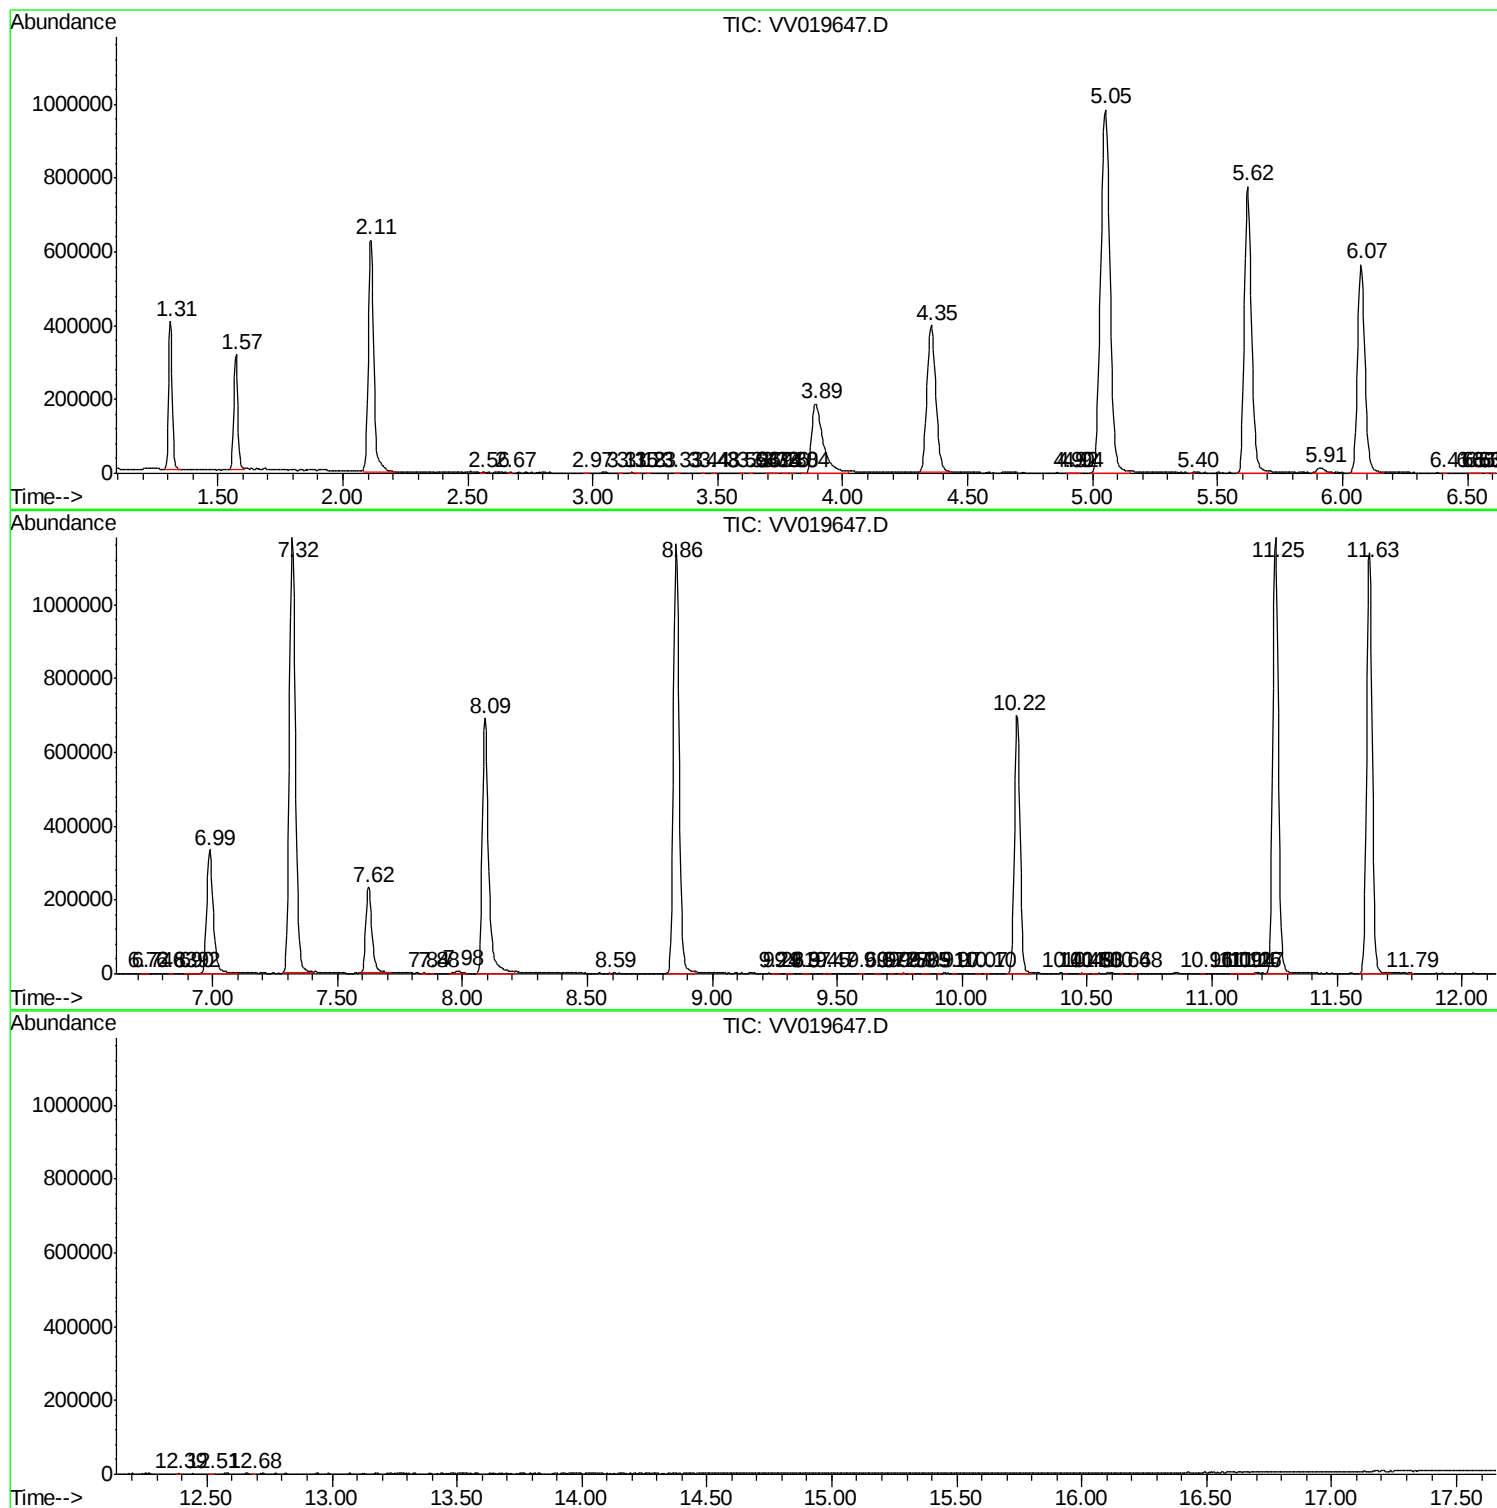

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121520\
Data File : VV019647.D
Acq On : 15 Dec 2020 14:19
Operator : SY/MD
Sample : VIBLK63
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121520\
Data File : VV019647.D
Acq On : 15 Dec 2020 14:19
Operator : SY/MD
Sample : VIBLK63
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK63

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc