

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019649.D
 Acq On : 15 Dec 2020 15:06
 Operator : SY/MD
 Sample : VIBLK64
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	85	rVB	397589	404883	16.10%	2.105%
2	1.569	142	149	165	rVB	320083	353219	14.04%	1.836%
3	2.110	307	317	346	rVB	629665	966551	38.42%	5.024%
4	2.669	488	491	495	rVB3	534	458	0.02%	0.002%
5	2.688	495	497	500	rBV3	648	465	0.02%	0.002%
6	2.724	506	508	510	rBV2	383	213	0.01%	0.001%
7	2.814	534	536	541	rBV2	580	451	0.02%	0.002%
8	2.843	542	545	549	rBV5	629	612	0.02%	0.003%
9	2.949	576	578	581	rBV	581	323	0.01%	0.002%
10	3.039	602	606	608	rBV3	623	411	0.02%	0.002%
11	3.309	687	690	691	rBV	284	175	0.01%	0.001%
12	3.386	712	714	717	rVB3	745	356	0.01%	0.002%
13	3.412	717	722	725	rBV2	402	456	0.02%	0.002%
14	3.528	756	758	761	rVB3	382	188	0.01%	0.001%
15	3.547	761	764	766	rBV3	358	261	0.01%	0.001%
16	3.647	792	795	797	rVB3	489	256	0.01%	0.001%
17	3.704	810	813	815	rBV	178	120	0.00%	0.001%
18	3.717	815	817	820	rVB4	377	117	0.00%	0.001%
19	3.730	820	821	824	rBV2	172	85	0.00%	0.000%
20	3.756	824	829	830	rBV	506	369	0.01%	0.002%
21	3.785	837	838	840	rBV	333	145	0.01%	0.001%
22	3.891	857	871	916	rBV	186722	573304	22.79%	2.980%
23	4.354	1000	1015	1047	rVB	397619	970215	38.57%	5.043%
24	4.643	1103	1105	1107	rBV2	624	301	0.01%	0.002%
25	4.769	1140	1144	1146	rBV3	682	558	0.02%	0.003%
26	4.936	1193	1196	1197	rBV	554	343	0.01%	0.002%
27	5.052	1213	1232	1265	rBV2	985619	2515520	100.00%	13.076%
28	5.621	1396	1409	1442	rBV	766906	1533673	60.97%	7.972%
29	5.981	1519	1521	1525	rVB2	1125	659	0.03%	0.003%
30	6.003	1525	1528	1531	rBV2	467	390	0.02%	0.002%
31	6.074	1535	1550	1577	rBV	554486	1132516	45.02%	5.887%
32	6.376	1642	1644	1646	rBV2	510	249	0.01%	0.001%
33	6.421	1656	1658	1662	rVB2	524	201	0.01%	0.001%
34	6.466	1670	1672	1673	rBV	299	108	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019649.D
 Acq On : 15 Dec 2020 15:06
 Operator : SY/MD
 Sample : VIBLK64
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.524	1688	1690	1693	rBV2	540	198	0.01%	0.001%
36	6.579	1703	1707	1709	rBV2	416	239	0.01%	0.001%
37	6.634	1719	1724	1725	rBV2	384	249	0.01%	0.001%
38	6.762	1760	1764	1766	rBV4	369	256	0.01%	0.001%
39	6.846	1786	1790	1794	rBV2	355	305	0.01%	0.002%
40	6.865	1794	1796	1799	rBV	307	226	0.01%	0.001%
41	6.891	1802	1804	1806	rBV	275	85	0.00%	0.000%
42	6.917	1809	1812	1813	rBV	351	157	0.01%	0.001%
43	6.987	1822	1834	1859	rBV	330763	600070	23.85%	3.119%
44	7.318	1925	1937	1963	rBV	1186239	2011760	79.97%	10.457%
45	7.624	2022	2032	2062	rBV	226857	399535	15.88%	2.077%
46	7.984	2134	2144	2155	rVB3	15522	26344	1.05%	0.137%
47	8.090	2166	2177	2209	rBV	681276	1199044	47.67%	6.233%
48	8.630	2342	2345	2349	rBV3	933	887	0.04%	0.005%
49	8.695	2361	2365	2369	rBV6	1003	996	0.04%	0.005%
50	8.762	2383	2386	2394	rVB5	1028	1303	0.05%	0.007%
51	8.801	2394	2398	2399	rBV3	543	290	0.01%	0.002%
52	8.855	2403	2415	2444	rBV	1163300	1857705	73.85%	9.656%
53	9.135	2500	2502	2503	rBV2	527	181	0.01%	0.001%
54	9.241	2532	2535	2537	rBV3	491	336	0.01%	0.002%
55	9.296	2550	2552	2556	rVB2	556	207	0.01%	0.001%
56	9.351	2564	2569	2571	rBV4	610	666	0.03%	0.003%
57	9.405	2584	2586	2588	rBV	283	128	0.01%	0.001%
58	9.466	2602	2605	2606	rBV	310	142	0.01%	0.001%
59	9.524	2621	2623	2627	rVB3	557	382	0.02%	0.002%
60	9.624	2651	2654	2657	rBV2	442	323	0.01%	0.002%
61	9.653	2661	2663	2666	rBV2	379	216	0.01%	0.001%
62	9.704	2675	2679	2685	rBV4	475	510	0.02%	0.003%
63	9.730	2685	2687	2690	rBV2	346	210	0.01%	0.001%
64	9.794	2705	2707	2710	rVB3	472	240	0.01%	0.001%
65	9.887	2731	2736	2738	rBV3	685	448	0.02%	0.002%
66	9.900	2738	2740	2741	rVB	396	145	0.01%	0.001%
67	9.945	2752	2754	2760	rVB3	534	417	0.02%	0.002%
68	10.039	2782	2783	2790	rVB4	428	323	0.01%	0.002%
69	10.116	2802	2807	2809	rBV5	532	515	0.02%	0.003%
70	10.219	2823	2839	2860	rBV	691303	1094080	43.49%	5.687%
71	10.379	2887	2889	2891	rBV2	533	207	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019649.D
 Acq On : 15 Dec 2020 15:06
 Operator : SY/MD
 Sample : VIBLK64
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK64

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.479	2918	2920	2921	rBV2	406	182	0.01%	0.001%
73	10.547	2936	2941	2944	rBV2	572	601	0.02%	0.003%
74	10.701	2987	2989	2991	rBV	503	246	0.01%	0.001%
75	10.891	3045	3048	3049	rBV2	423	238	0.01%	0.001%
76	10.952	3066	3067	3069	rBV2	483	215	0.01%	0.001%
77	11.039	3093	3094	3096	rBV2	525	280	0.01%	0.001%
78	11.125	3115	3121	3122	rBV3	633	601	0.02%	0.003%
79	11.254	3149	3161	3182	rBV	1177351	1799958	71.55%	9.356%
80	11.457	3222	3224	3225	rBV	576	253	0.01%	0.001%
81	11.559	3254	3256	3258	rBV2	602	322	0.01%	0.002%
82	11.630	3264	3278	3300	rBV	1125168	1773958	70.52%	9.221%
83	11.846	3344	3345	3348	rBV	387	193	0.01%	0.001%
84	11.929	3368	3371	3376	rBV4	651	542	0.02%	0.003%
85	12.006	3391	3395	3398	rBV3	643	594	0.02%	0.003%
86	12.067	3412	3414	3416	rBV2	420	226	0.01%	0.001%
87	12.296	3483	3485	3492	rVB5	670	588	0.02%	0.003%
88	12.370	3506	3508	3512	rBV2	355	263	0.01%	0.001%
89	12.553	3563	3565	3570	rBV2	372	291	0.01%	0.002%
90	13.080	3727	3729	3731	rBV	455	181	0.01%	0.001%
91	13.112	3737	3739	3743	rVB2	781	416	0.02%	0.002%
92	13.222	3771	3773	3775	rBV	582	313	0.01%	0.002%


Sum of corrected areas: 19237937

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121520\
Data File : VV019649.D
Acq On : 15 Dec 2020 15:06
Operator : SY/MD
Sample : VIBLK64
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

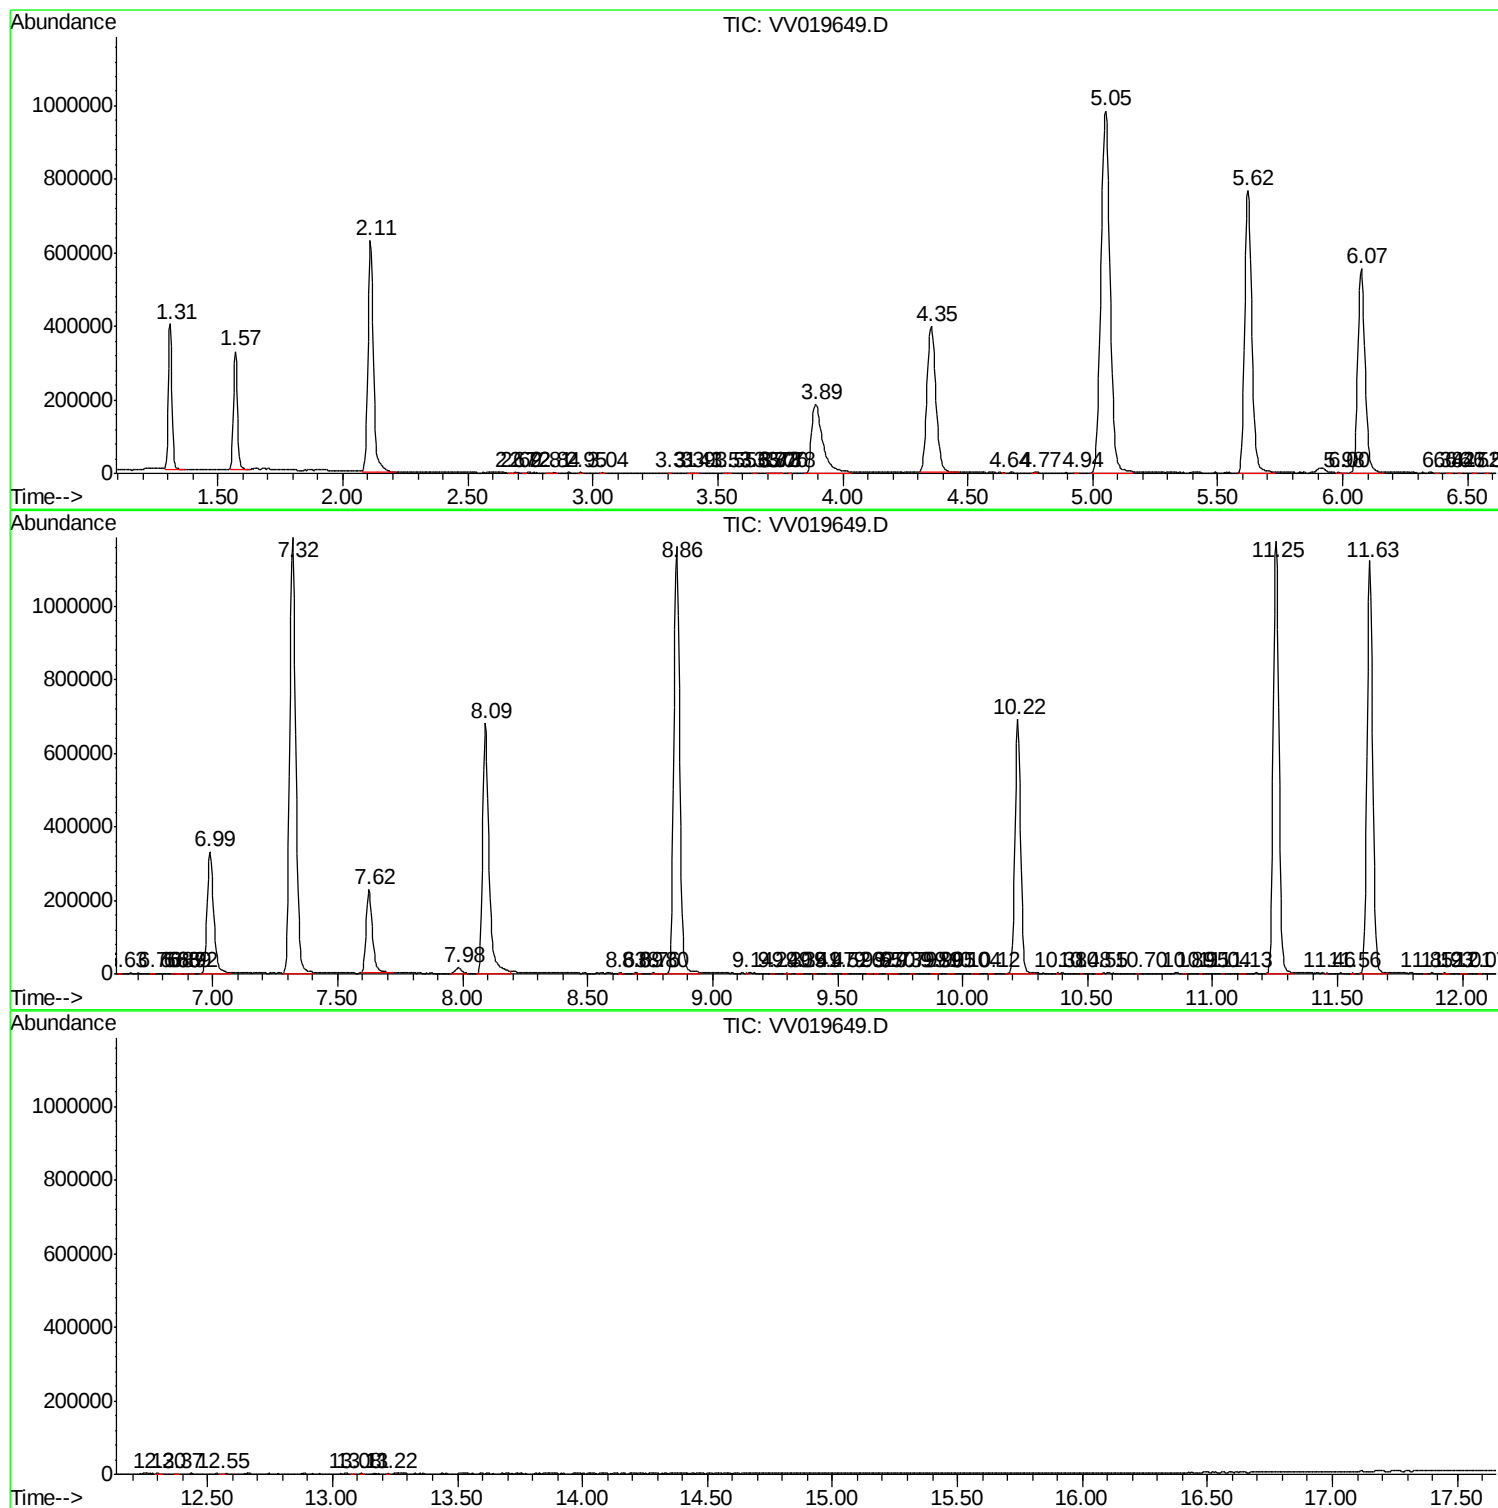

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121520\
Data File : VV019649.D
Acq On : 15 Dec 2020 15:06
Operator : SY/MD
Sample : VIBLK64
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121520\
Data File : VV019649.D
Acq On : 15 Dec 2020 15:06
Operator : SY/MD
Sample : VIBLK64
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK64

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc