

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019652.D
 Acq On : 15 Dec 2020 16:23
 Operator : SY/MD
 Sample : L5099-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	79	rVB	367125	362789	15.57%	1.999%
2	1.569	142	149	161	rVB	288112	315837	13.56%	1.740%
3	2.110	308	317	353	rVB	576793	875757	37.59%	4.824%
4	2.769	519	522	526	rVB4	1183	913	0.04%	0.005%
5	2.859	547	550	553	rBV2	432	283	0.01%	0.002%
6	2.907	563	565	566	rBV	377	168	0.01%	0.001%
7	2.930	569	572	575	rBV3	587	422	0.02%	0.002%
8	3.190	650	653	656	rVB3	297	161	0.01%	0.001%
9	3.209	656	659	661	rBV4	352	261	0.01%	0.001%
10	3.248	668	671	673	rBV2	569	283	0.01%	0.002%
11	3.283	680	682	685	rBV3	361	177	0.01%	0.001%
12	3.309	687	690	691	rVB2	516	228	0.01%	0.001%
13	3.325	693	695	699	rBV2	393	304	0.01%	0.002%
14	3.344	699	701	703	rVB2	565	204	0.01%	0.001%
15	3.447	731	733	736	rBV2	509	426	0.02%	0.002%
16	3.499	743	749	754	rVV5	429	483	0.02%	0.003%
17	3.521	754	756	760	rVB2	279	133	0.01%	0.001%
18	3.557	765	767	772	rVB3	539	338	0.01%	0.002%
19	3.586	772	776	779	rBV4	671	590	0.03%	0.003%
20	3.627	787	789	790	rBV2	326	165	0.01%	0.001%
21	3.663	795	800	801	rBV2	678	474	0.02%	0.003%
22	3.772	833	834	837	rVB	258	123	0.01%	0.001%
23	3.798	837	842	846	rBV3	805	652	0.03%	0.004%
24	3.817	846	848	850	rBV	468	247	0.01%	0.001%
25	3.833	851	853	856	rBV2	295	173	0.01%	0.001%
26	3.897	861	873	914	rBV2	159259	514208	22.07%	2.833%
27	4.354	1000	1015	1048	rVB	362618	899773	38.62%	4.957%
28	4.663	1108	1111	1113	rBV4	531	268	0.01%	0.001%
29	4.904	1182	1186	1189	rBV4	469	341	0.01%	0.002%
30	4.936	1193	1196	1200	rBV4	532	558	0.02%	0.003%
31	4.987	1207	1212	1213	rBV	457	266	0.01%	0.001%
32	5.052	1213	1232	1255	rBV2	918054	2329958	100.00%	12.835%
33	5.479	1361	1365	1366	rBV2	876	574	0.02%	0.003%
34	5.573	1392	1394	1396	rBV2	640	409	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019652.D
 Acq On : 15 Dec 2020 16:23
 Operator : SY/MD
 Sample : L5099-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	5.621	1396	1409	1432	rVV	773871	1529444	65.64%	8.425%
36	6.074	1536	1550	1574	rBV	519260	1049696	45.05%	5.783%
37	6.415	1654	1656	1660	rBV3	322	230	0.01%	0.001%
38	6.437	1660	1663	1665	rVB3	325	200	0.01%	0.001%
39	6.450	1665	1667	1669	rBV2	550	220	0.01%	0.001%
40	6.547	1695	1697	1700	rBV2	411	171	0.01%	0.001%
41	6.563	1700	1702	1704	rBV2	215	108	0.00%	0.001%
42	6.589	1704	1710	1714	rVB5	594	515	0.02%	0.003%
43	6.618	1718	1719	1720	rBV5	514	154	0.01%	0.001%
44	6.740	1753	1757	1760	rBV2	487	460	0.02%	0.003%
45	6.756	1760	1762	1764	rVB2	651	227	0.01%	0.001%
46	6.778	1765	1769	1771	rBV3	569	375	0.02%	0.002%
47	6.814	1778	1780	1782	rBV2	457	226	0.01%	0.001%
48	6.855	1791	1793	1795	rBV	295	116	0.00%	0.001%
49	6.884	1799	1802	1805	rVB2	518	332	0.01%	0.002%
50	6.910	1805	1810	1811	rBV	329	261	0.01%	0.001%
51	6.942	1817	1820	1821	rBV	491	228	0.01%	0.001%
52	6.987	1821	1834	1860	rBV	309990	559259	24.00%	3.081%
53	7.318	1925	1937	1966	rBV	1074907	1865450	80.06%	10.276%
54	7.624	2022	2032	2052	rBV	209906	365181	15.67%	2.012%
55	7.981	2136	2143	2153	rVB5	4945	7950	0.34%	0.044%
56	8.090	2167	2177	2211	rBV	647113	1144481	49.12%	6.305%
57	8.572	2325	2327	2328	rBV2	631	210	0.01%	0.001%
58	8.614	2336	2340	2345	rBV5	758	775	0.03%	0.004%
59	8.797	2395	2397	2399	rBV2	386	225	0.01%	0.001%
60	8.855	2403	2415	2445	rBV	1154401	1853893	79.57%	10.213%
61	9.071	2478	2482	2485	rBV5	1035	856	0.04%	0.005%
62	9.100	2488	2491	2492	rBV	575	310	0.01%	0.002%
63	9.299	2550	2553	2555	rBV3	521	336	0.01%	0.002%
64	9.363	2568	2573	2575	rBV2	716	521	0.02%	0.003%
65	9.396	2580	2583	2584	rBV	455	267	0.01%	0.001%
66	9.463	2602	2604	2609	rVB3	811	662	0.03%	0.004%
67	9.498	2609	2615	2617	rBV3	785	722	0.03%	0.004%
68	9.540	2624	2628	2632	rBV2	556	528	0.02%	0.003%
69	9.576	2637	2639	2645	rVV4	691	602	0.03%	0.003%
70	9.717	2678	2683	2688	rBV4	676	698	0.03%	0.004%
71	9.765	2695	2698	2700	rVB2	374	164	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019652.D
 Acq On : 15 Dec 2020 16:23
 Operator : SY/MD
 Sample : L5099-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	9.778	2700	2702	2703	rBV	462	180	0.01%	0.001%
73	9.823	2714	2716	2720	rVB2	475	313	0.01%	0.002%
74	9.852	2723	2725	2727	rBV3	565	283	0.01%	0.002%
75	10.000	2769	2771	2772	rBV2	479	172	0.01%	0.001%
76	10.035	2779	2782	2783	rBV2	638	297	0.01%	0.002%
77	10.048	2784	2786	2789	rVB	443	170	0.01%	0.001%
78	10.071	2789	2793	2794	rBV3	502	328	0.01%	0.002%
79	10.174	2823	2825	2827	rBV	439	174	0.01%	0.001%
80	10.219	2827	2839	2856	rBV	658082	1024499	43.97%	5.644%
81	10.698	2986	2988	2994	rBV3	343	281	0.01%	0.002%
82	11.100	3111	3113	3116	rVB2	570	295	0.01%	0.002%
83	11.122	3116	3120	3124	rBV2	667	562	0.02%	0.003%
84	11.254	3148	3161	3187	rBV	1156645	1783649	76.55%	9.826%
85	11.630	3265	3278	3300	rBV	1049389	1646980	70.69%	9.073%
86	12.203	3454	3456	3461	rBV2	724	556	0.02%	0.003%


Sum of corrected areas: 18152738

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121520\
Data File : VV019652.D
Acq On : 15 Dec 2020 16:23
Operator : SY/MD
Sample : L5099-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

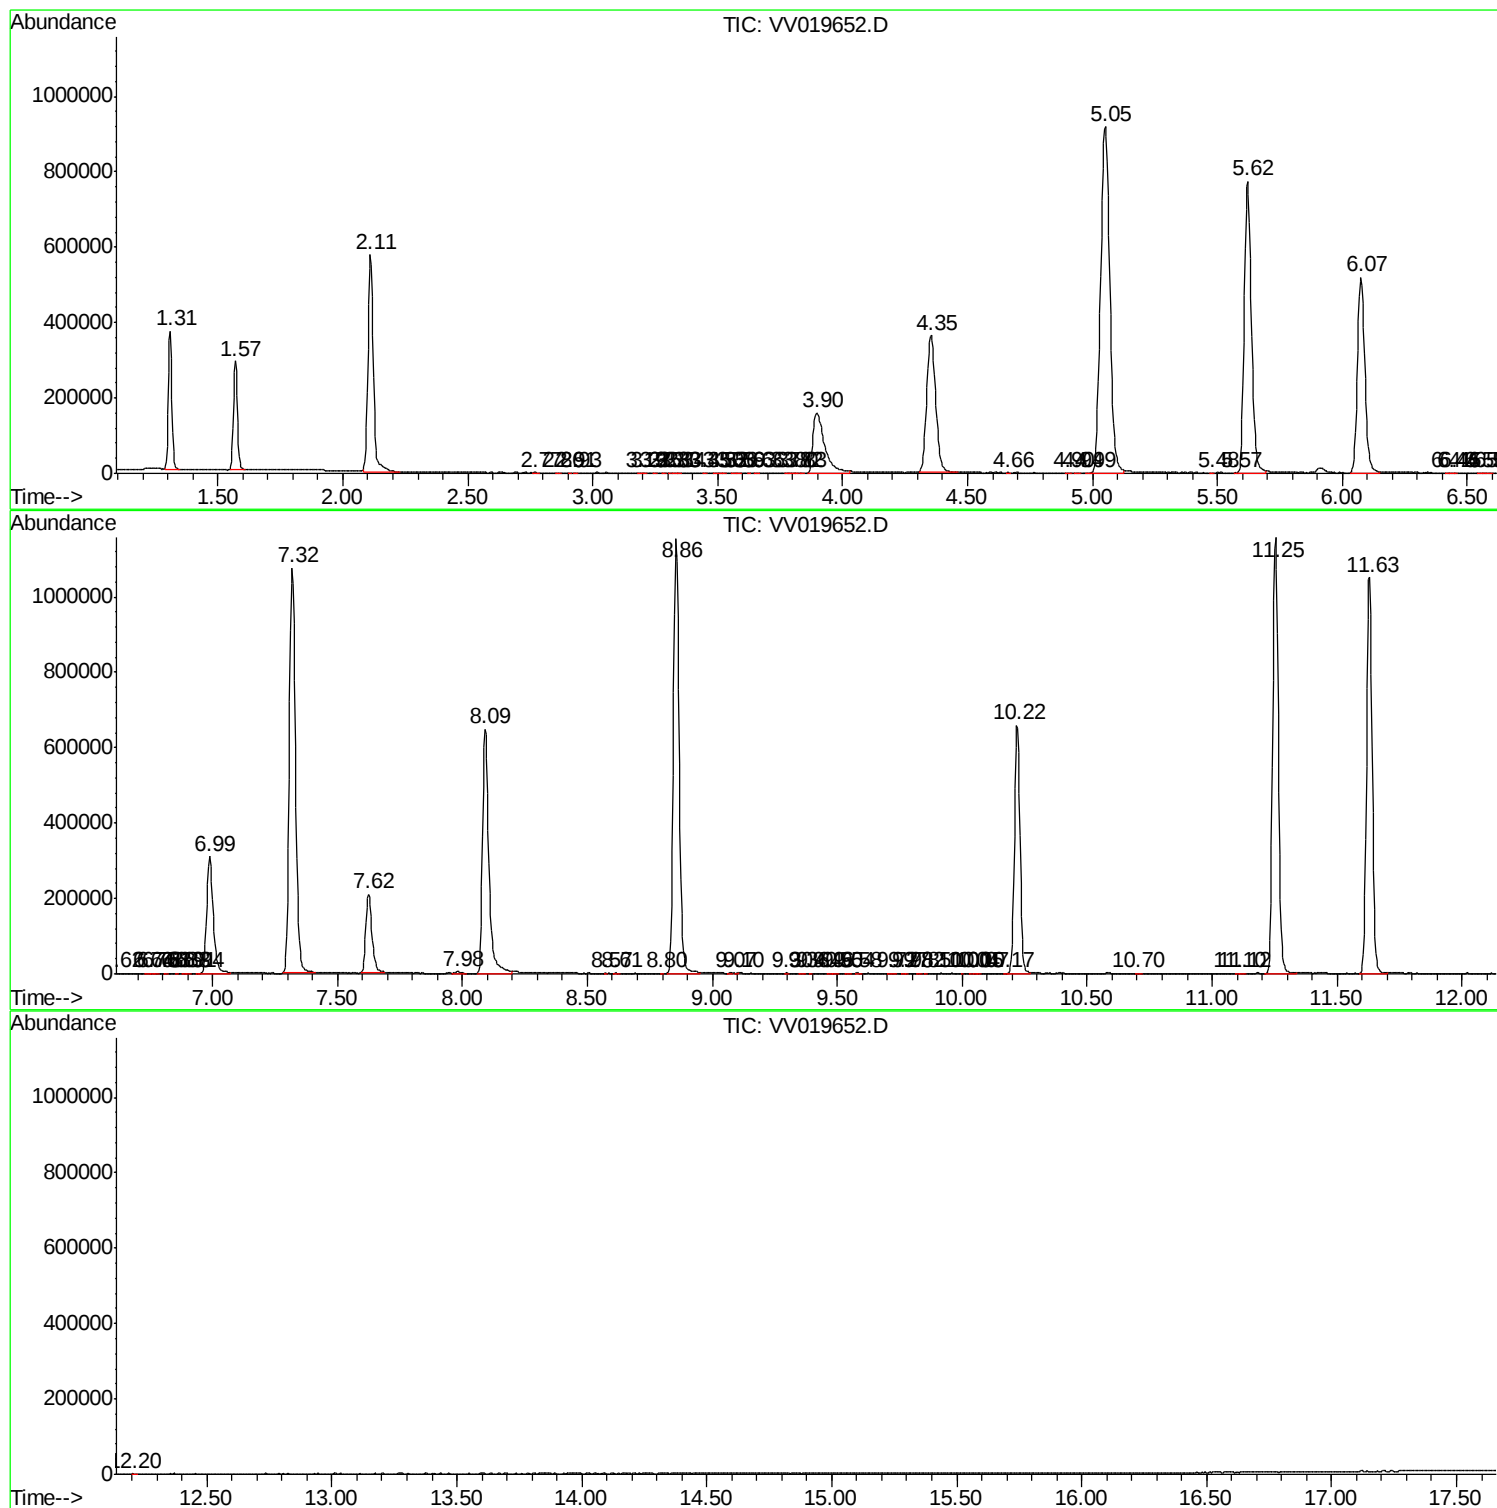

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121520\
Data File : VV019652.D
Acq On : 15 Dec 2020 16:23
Operator : SY/MD
Sample : L5099-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121520\
Data File : VV019652.D
Acq On : 15 Dec 2020 16:23
Operator : SY/MD
Sample : L5099-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
