

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019655.D
 Acq On : 15 Dec 2020 17:35
 Operator : SY/MD
 Sample : L5024-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AY9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	87	rVB	375144	378603	15.67%	2.062%
2	1.569	143	149	163	rVB	286640	325352	13.47%	1.772%
3	2.113	308	318	355	rVB	587858	920022	38.09%	5.011%
4	2.759	513	519	520	rBV2	1044	1035	0.04%	0.006%
5	2.884	555	558	562	rVB3	626	486	0.02%	0.003%
6	2.901	562	563	564	rBV	387	132	0.01%	0.001%
7	3.116	625	630	631	rBV2	644	393	0.02%	0.002%
8	3.405	718	720	723	rBV2	330	208	0.01%	0.001%
9	3.486	743	745	747	rBV2	346	190	0.01%	0.001%
10	3.614	782	785	788	rBV	369	296	0.01%	0.002%
11	3.663	796	800	801	rBV2	274	180	0.01%	0.001%
12	3.727	816	820	822	rBV3	541	457	0.02%	0.002%
13	3.743	822	825	829	rVV4	910	797	0.03%	0.004%
14	3.791	837	840	845	rBV3	523	363	0.02%	0.002%
15	3.817	845	848	853	rBV3	423	363	0.02%	0.002%
16	3.846	853	857	858	rBV2	651	440	0.02%	0.002%
17	3.894	861	872	919	rBV	160529	527083	21.82%	2.871%
18	4.354	1000	1015	1041	rBV	381929	936912	38.79%	5.103%
19	4.746	1134	1137	1140	rBV3	839	564	0.02%	0.003%
20	4.778	1145	1147	1149	rBV3	346	174	0.01%	0.001%
21	4.855	1168	1171	1176	rVB3	602	430	0.02%	0.002%
22	4.888	1178	1181	1183	rBV2	510	377	0.02%	0.002%
23	4.965	1203	1205	1207	rBV2	679	352	0.01%	0.002%
24	5.052	1210	1232	1259	rBV2	945199	2415336	100.00%	13.154%
25	5.463	1358	1360	1362	rVB3	508	157	0.01%	0.001%
26	5.476	1362	1364	1366	rBV2	545	219	0.01%	0.001%
27	5.489	1366	1368	1372	rVB3	640	410	0.02%	0.002%
28	5.547	1383	1386	1387	rBV	697	321	0.01%	0.002%
29	5.556	1387	1389	1391	rVV3	641	284	0.01%	0.002%
30	5.621	1396	1409	1437	rBV	740466	1483791	61.43%	8.081%
31	5.878	1486	1489	1490	rBV2	941	491	0.02%	0.003%
32	5.916	1492	1501	1517	rVB7	13057	28625	1.19%	0.156%
33	6.074	1536	1550	1572	rBV	536945	1084132	44.89%	5.904%
34	6.344	1630	1634	1641	rVB6	813	950	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019655.D
 Acq On : 15 Dec 2020 17:35
 Operator : SY/MD
 Sample : L5024-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AY9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.434	1661	1662	1663	rBV	560	158	0.01%	0.001%
36	6.518	1682	1688	1689	rBV2	507	427	0.02%	0.002%
37	6.563	1699	1702	1704	rBV3	439	312	0.01%	0.002%
38	6.605	1708	1715	1717	rBV3	785	1031	0.04%	0.006%
39	6.707	1745	1747	1751	rVB3	982	559	0.02%	0.003%
40	6.727	1751	1753	1757	rBV2	401	240	0.01%	0.001%
41	6.752	1757	1761	1762	rBV3	408	278	0.01%	0.002%
42	6.804	1775	1777	1783	rVB3	1006	714	0.03%	0.004%
43	6.839	1783	1788	1793	rBV5	683	722	0.03%	0.004%
44	6.862	1793	1795	1796	rBV5	312	122	0.01%	0.001%
45	6.907	1808	1809	1812	rBV	182	86	0.00%	0.000%
46	6.929	1812	1816	1818	rBV3	627	476	0.02%	0.003%
47	6.990	1822	1835	1862	rBV	313046	570092	23.60%	3.105%
48	7.318	1925	1937	1969	rBV	1113312	1927884	79.82%	10.500%
49	7.624	2021	2032	2060	rBV	220660	387290	16.03%	2.109%
50	7.932	2124	2128	2129	rBV2	1107	635	0.03%	0.003%
51	8.090	2166	2177	2212	rBV	619357	1110443	45.97%	6.048%
52	8.736	2374	2378	2379	rBV2	346	183	0.01%	0.001%
53	8.855	2403	2415	2437	rBV	1119105	1792269	74.20%	9.761%
54	9.219	2525	2528	2529	rBV3	570	340	0.01%	0.002%
55	9.466	2603	2605	2608	rVB3	500	296	0.01%	0.002%
56	9.537	2622	2627	2630	rBV4	654	668	0.03%	0.004%
57	9.579	2638	2640	2642	rBV	479	186	0.01%	0.001%
58	9.701	2674	2678	2680	rBV3	270	214	0.01%	0.001%
59	9.833	2716	2719	2721	rBV	457	260	0.01%	0.001%
60	9.945	2751	2754	2759	rBV2	356	344	0.01%	0.002%
61	10.055	2785	2788	2793	rBV2	672	631	0.03%	0.003%
62	10.135	2811	2813	2814	rBV	338	111	0.00%	0.001%
63	10.219	2826	2839	2861	rBV	671631	1044172	43.23%	5.687%
64	10.527	2931	2935	2939	rBV2	842	587	0.02%	0.003%
65	10.630	2966	2967	2973	rBV3	350	239	0.01%	0.001%
66	10.775	3009	3012	3013	rBV2	458	238	0.01%	0.001%
67	10.923	3056	3058	3060	rBV	679	410	0.02%	0.002%
68	11.026	3088	3090	3092	rBV	357	212	0.01%	0.001%
69	11.096	3110	3112	3117	rVB	649	418	0.02%	0.002%
70	11.119	3117	3119	3122	rBV	419	218	0.01%	0.001%
71	11.177	3135	3137	3141	rBV3	662	402	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019655.D
 Acq On : 15 Dec 2020 17:35
 Operator : SY/MD
 Sample : L5024-15
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AY9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	11.254	3148	3161	3185	rBV	1130641	1717667	71.12%	9.355%
73	11.630	3266	3278	3296	rBV	1079764	1686190	69.81%	9.183%
74	12.260	3471	3474	3475	rBV2	409	238	0.01%	0.001%
75	12.305	3485	3488	3491	rBV3	534	333	0.01%	0.002%
76	12.688	3603	3607	3610	rBV	445	310	0.01%	0.002%
77	12.913	3675	3677	3682	rBV3	482	463	0.02%	0.003%
78	13.026	3710	3712	3714	rBV2	652	385	0.02%	0.002%
79	13.228	3772	3775	3777	rBV2	564	361	0.01%	0.002%
80	13.421	3831	3835	3839	rBV2	687	663	0.03%	0.004%
81	13.553	3873	3876	3880	rBV2	806	543	0.02%	0.003%
82	14.254	4092	4094	4098	rBV2	616	443	0.02%	0.002%


Sum of corrected areas: 18361388

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121520\
Data File : VV019655.D
Acq On : 15 Dec 2020 17:35
Operator : SY/MD
Sample : L5024-15
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AY9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

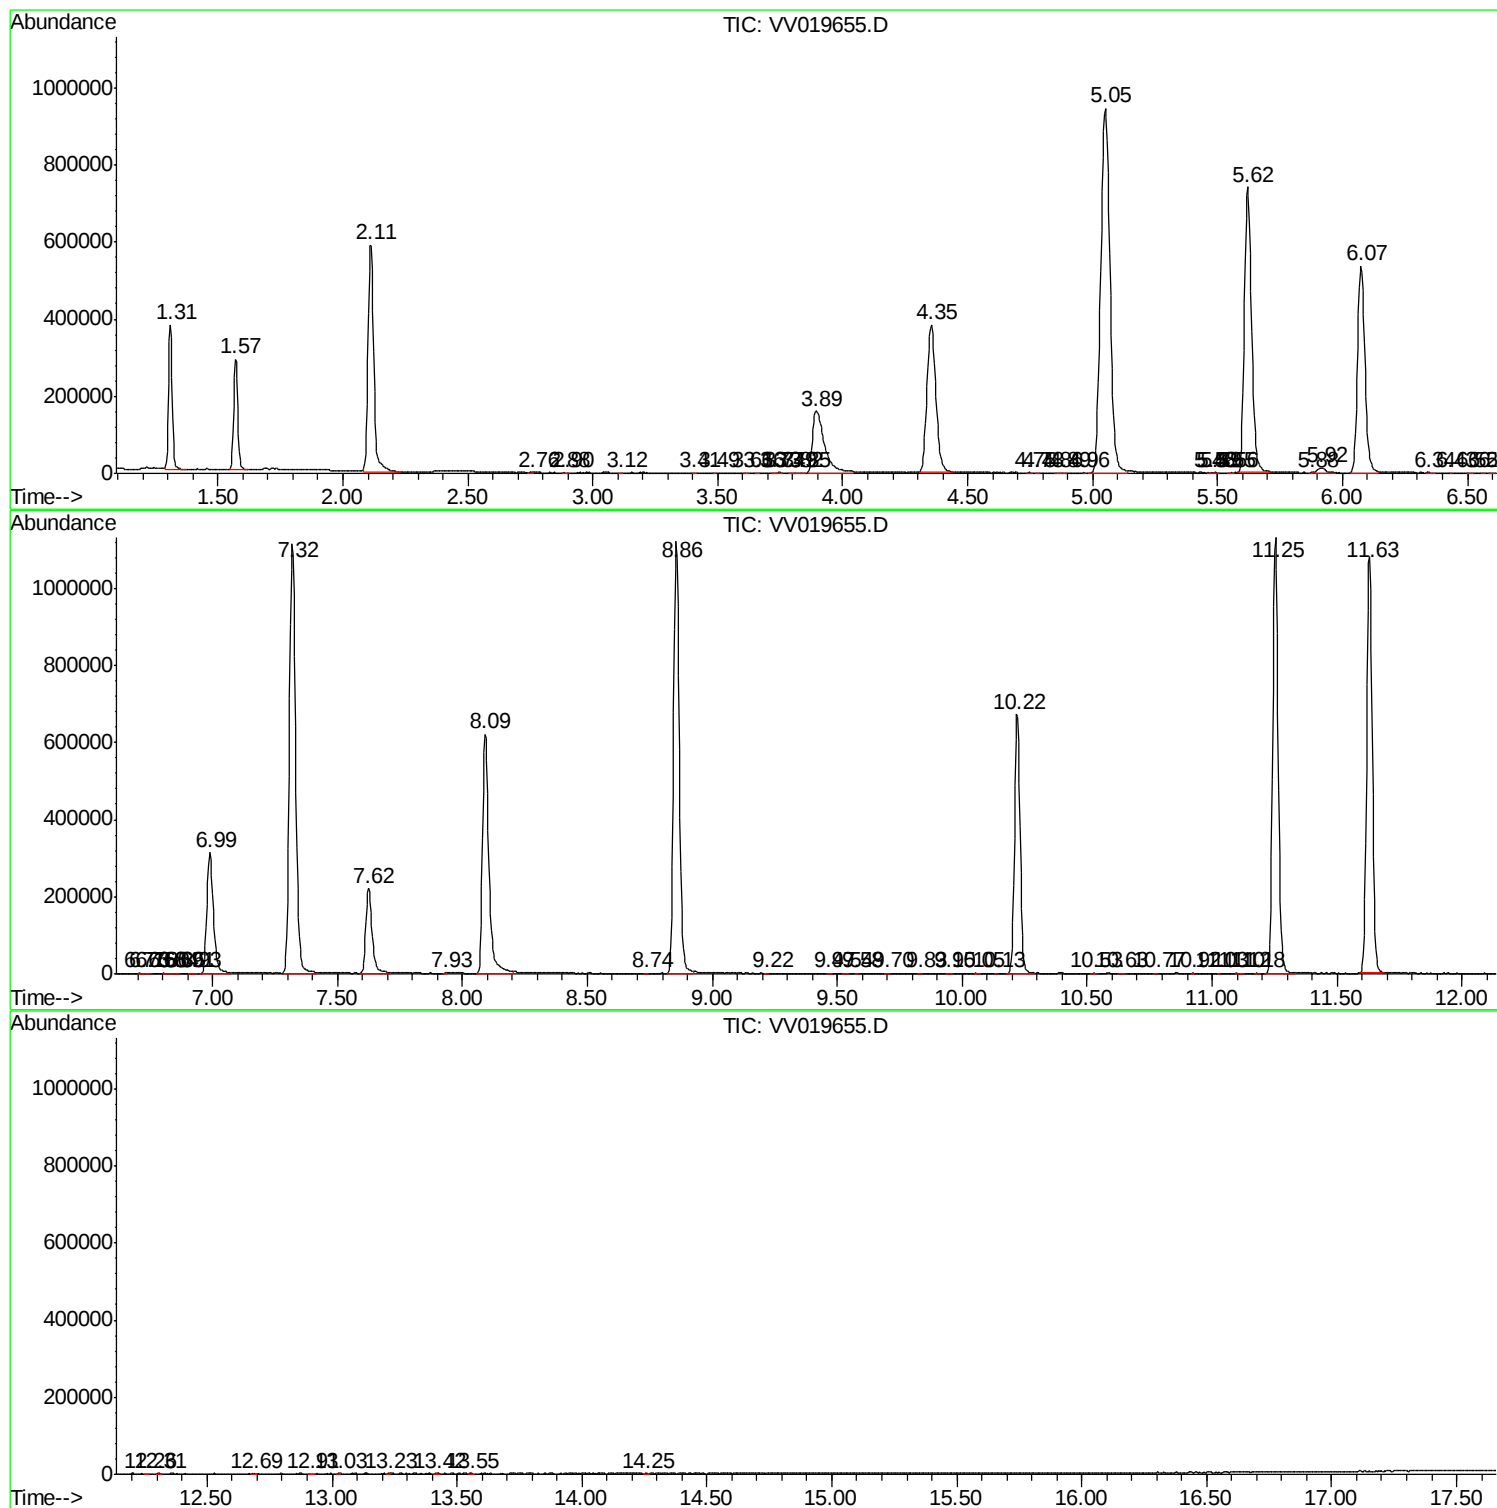

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121520\
Data File : VV019655.D
Acq On : 15 Dec 2020 17:35
Operator : SY/MD
Sample : L5024-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AY9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121520\
Data File : VV019655.D
Acq On : 15 Dec 2020 17:35
Operator : SY/MD
Sample : L5024-15
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AY9

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc