

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019656.D
 Acq On : 15 Dec 2020 17:59
 Operator : SY/MD
 Sample : L5024-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	86	rVB	371258	373522	15.62%	2.047%
2	1.569	142	149	164	rVB	286338	322637	13.49%	1.768%
3	2.109	308	317	356	rVB	586993	913295	38.18%	5.006%
4	3.171	644	647	648	rBV	346	195	0.01%	0.001%
5	3.244	668	670	674	rBV2	378	149	0.01%	0.001%
6	3.273	676	679	682	rBV2	484	349	0.01%	0.002%
7	3.341	698	700	702	rBV3	543	244	0.01%	0.001%
8	3.418	719	724	725	rBV2	737	434	0.02%	0.002%
9	3.511	748	753	761	rBV5	845	1155	0.05%	0.006%
10	3.543	761	763	765	rVV	413	151	0.01%	0.001%
11	3.553	765	766	770	rVB	459	264	0.01%	0.001%
12	3.650	792	796	799	rBV2	353	355	0.01%	0.002%
13	3.675	800	804	808	rVV2	371	359	0.02%	0.002%
14	3.733	820	822	824	rBV2	342	149	0.01%	0.001%
15	3.823	848	850	851	rBV	339	177	0.01%	0.001%
16	3.897	858	873	915	rBV	171846	571563	23.90%	3.133%
17	4.354	1000	1015	1047	rVB	374681	928218	38.81%	5.087%
18	4.682	1113	1117	1123	rBV6	783	1066	0.04%	0.006%
19	4.823	1160	1161	1162	rBV6	271	87	0.00%	0.000%
20	4.852	1168	1170	1172	rBV2	441	275	0.01%	0.002%
21	4.894	1181	1183	1185	rBV	518	275	0.01%	0.002%
22	4.990	1210	1213	1214	rBV2	626	323	0.01%	0.002%
23	5.051	1214	1232	1260	rBV2	934637	2391879	100.00%	13.109%
24	5.621	1396	1409	1437	rBV	726847	1444476	60.39%	7.917%
25	5.830	1470	1474	1477	rBV4	661	548	0.02%	0.003%
26	5.913	1491	1500	1516	rVB6	14594	32345	1.35%	0.177%
27	6.010	1526	1530	1533	rBV3	597	470	0.02%	0.003%
28	6.074	1536	1550	1580	rVV	533167	1079426	45.13%	5.916%
29	6.431	1657	1661	1665	rBV4	1089	689	0.03%	0.004%
30	6.453	1665	1668	1672	rBV3	812	611	0.03%	0.003%
31	6.514	1686	1687	1690	rBV	373	192	0.01%	0.001%
32	6.572	1701	1705	1708	rVB2	858	591	0.02%	0.003%
33	6.595	1708	1712	1713	rBV	503	248	0.01%	0.001%
34	6.666	1732	1734	1738	rBV3	625	495	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019656.D
 Acq On : 15 Dec 2020 17:59
 Operator : SY/MD
 Sample : L5024-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.730	1749	1754	1756	rBV3	448	351	0.01%	0.002%
36	6.752	1760	1761	1764	rBV2	230	117	0.00%	0.001%
37	6.775	1765	1768	1770	rBV4	661	359	0.02%	0.002%
38	6.836	1785	1787	1792	rVB2	480	425	0.02%	0.002%
39	6.865	1792	1796	1800	rBV3	773	548	0.02%	0.003%
40	6.894	1800	1805	1808	rBV3	561	476	0.02%	0.003%
41	6.929	1813	1816	1820	rVB3	567	403	0.02%	0.002%
42	6.990	1822	1835	1859	rBV	315113	565561	23.65%	3.100%
43	7.193	1895	1898	1901	rBV4	707	657	0.03%	0.004%
44	7.318	1924	1937	1961	rBV	1103263	1904621	79.63%	10.439%
45	7.624	2021	2032	2061	rBV	218569	382973	16.01%	2.099%
46	8.016	2151	2154	2159	rVB3	1112	997	0.04%	0.005%
47	8.051	2159	2165	2166	rBV4	928	782	0.03%	0.004%
48	8.090	2167	2177	2220	rBV	635401	1149220	48.05%	6.299%
49	8.691	2357	2364	2370	rBV7	874	1381	0.06%	0.008%
50	8.772	2386	2389	2393	rBV2	832	617	0.03%	0.003%
51	8.855	2403	2415	2444	rBV	1096398	1758305	73.51%	9.637%
52	9.138	2500	2503	2505	rBV2	720	453	0.02%	0.002%
53	9.174	2510	2514	2518	rBV5	587	614	0.03%	0.003%
54	9.247	2535	2537	2543	rVB4	641	483	0.02%	0.003%
55	9.460	2602	2603	2605	rBV	332	100	0.00%	0.001%
56	9.543	2625	2629	2631	rBV2	790	633	0.03%	0.003%
57	9.598	2644	2646	2648	rBV	289	169	0.01%	0.001%
58	9.611	2648	2650	2651	rBV	316	118	0.00%	0.001%
59	9.794	2705	2707	2709	rBV2	448	222	0.01%	0.001%
60	9.849	2722	2724	2727	rBB4	554	331	0.01%	0.002%
61	9.874	2729	2732	2734	rBV2	555	278	0.01%	0.002%
62	10.093	2798	2800	2807	rVB2	544	381	0.02%	0.002%
63	10.122	2807	2809	2810	rBV2	433	210	0.01%	0.001%
64	10.222	2827	2840	2865	rBV	653441	1041221	43.53%	5.707%
65	10.540	2937	2939	2942	rBV3	361	213	0.01%	0.001%
66	10.556	2942	2944	2945	rBV	347	84	0.00%	0.000%
67	10.665	2975	2978	2980	rBV2	433	309	0.01%	0.002%
68	10.733	2996	2999	3000	rBV2	354	200	0.01%	0.001%
69	10.845	3031	3034	3035	rBV2	359	212	0.01%	0.001%
70	10.855	3035	3037	3038	rBV	812	378	0.02%	0.002%
71	10.903	3050	3052	3054	rBV	529	285	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121520\
 Data File : VV019656.D
 Acq On : 15 Dec 2020 17:59
 Operator : SY/MD
 Sample : L5024-17
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AZ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	11.045	3094	3096	3100	rVB2	394	245	0.01%	0.001%
73	11.154	3126	3130	3133	rBV4	757	674	0.03%	0.004%
74	11.193	3140	3142	3148	rBV2	621	434	0.02%	0.002%
75	11.254	3149	3161	3184	rBV	1079769	1676982	70.11%	9.191%
76	11.546	3248	3252	3254	rBV2	1043	820	0.03%	0.004%
77	11.630	3266	3278	3304	rBV	1077226	1681193	70.29%	9.214%
78	12.074	3413	3416	3418	rBV5	697	411	0.02%	0.002%
79	12.260	3472	3474	3478	rVB2	665	319	0.01%	0.002%
80	12.424	3523	3525	3528	rBV2	584	389	0.02%	0.002%
81	12.485	3542	3544	3546	rBV2	677	302	0.01%	0.002%
82	12.553	3563	3565	3567	rBV2	347	202	0.01%	0.001%
83	12.588	3573	3576	3579	rBV2	612	546	0.02%	0.003%
84	12.636	3588	3591	3593	rBV2	296	219	0.01%	0.001%
85	12.652	3594	3596	3597	rBV	617	257	0.01%	0.001%
86	12.807	3642	3644	3649	rBV3	533	306	0.01%	0.002%
87	13.003	3702	3705	3706	rBV	504	259	0.01%	0.001%
88	13.424	3834	3836	3838	rBV2	621	322	0.01%	0.002%


Sum of corrected areas: 18245779

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121520\
Data File : VV019656.D
Acq On : 15 Dec 2020 17:59
Operator : SY/MD
Sample : L5024-17
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0A22

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

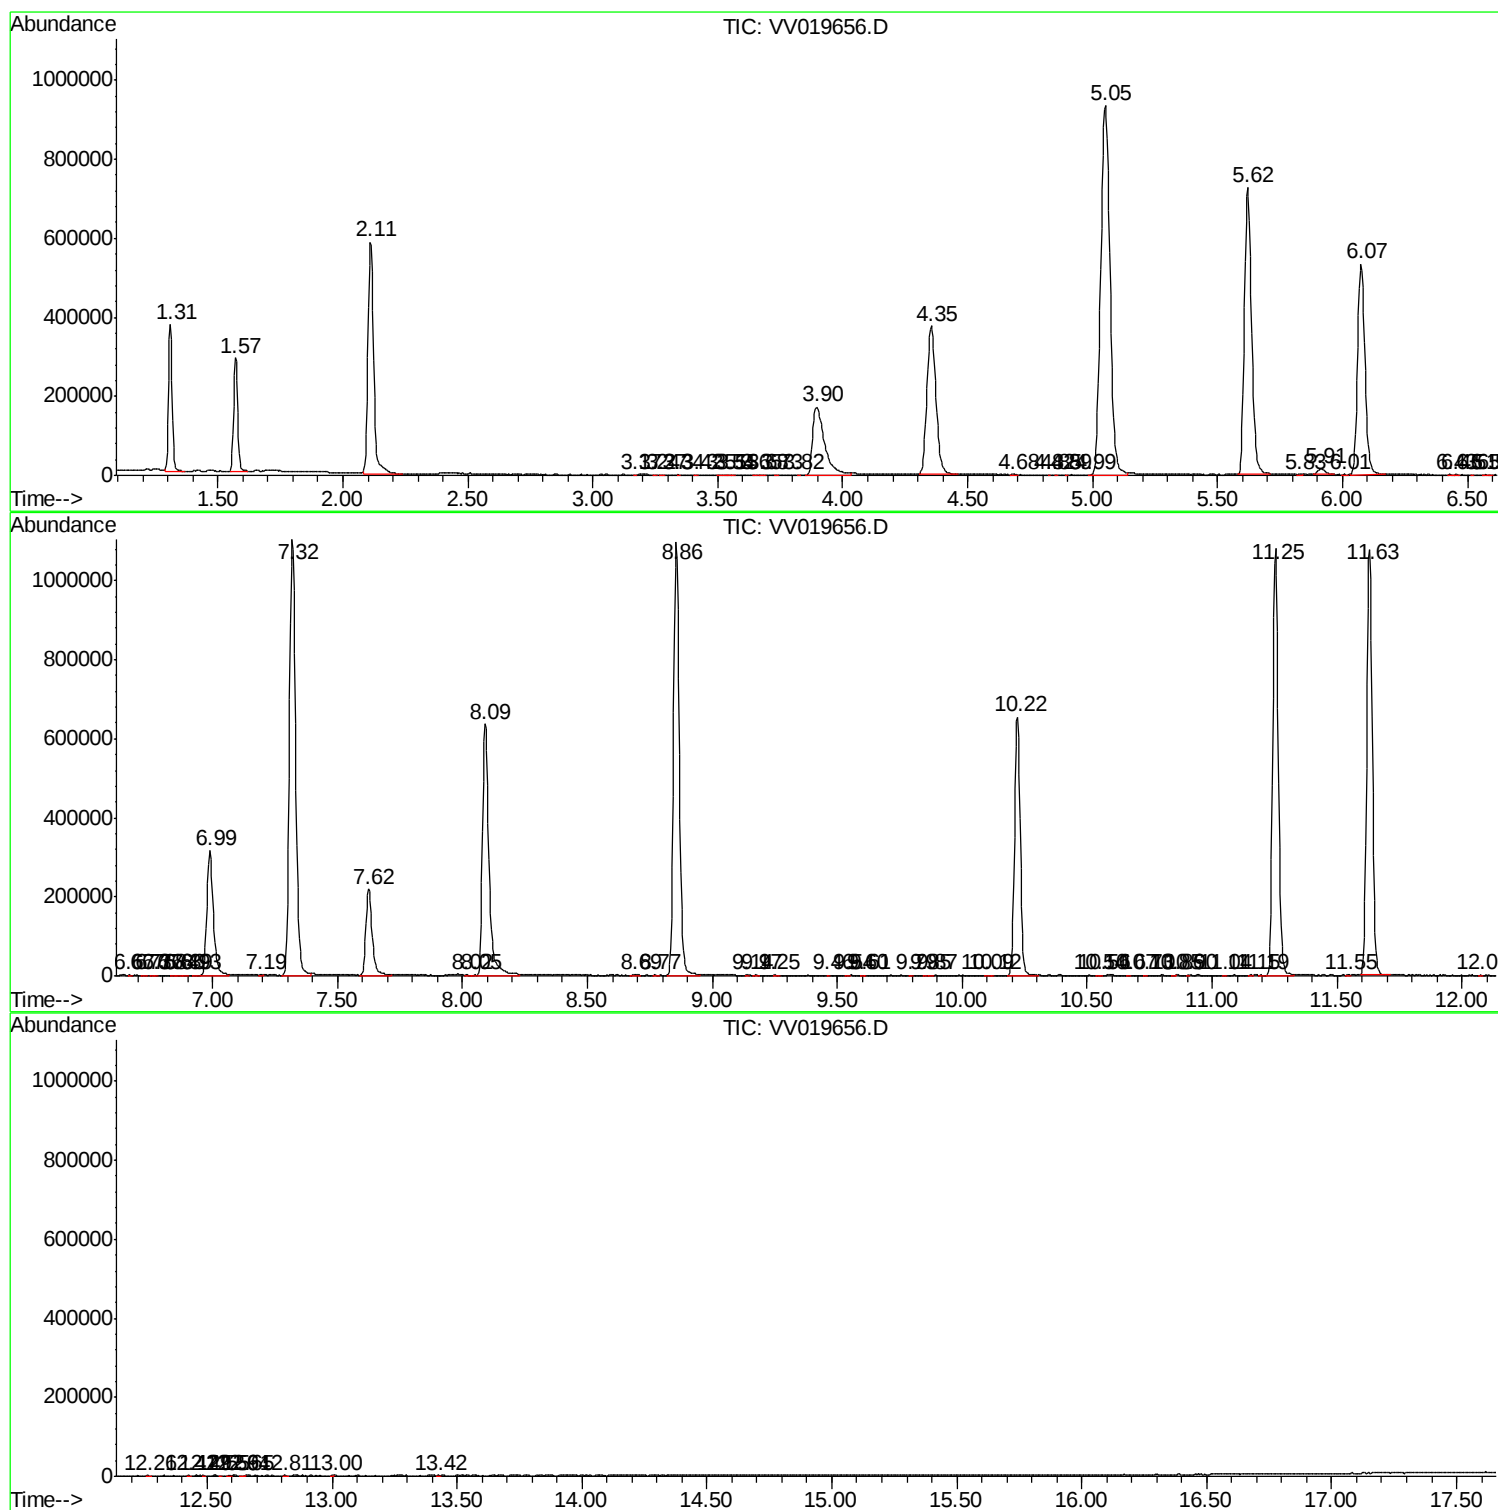

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121520\
Data File : VV019656.D
Acq On : 15 Dec 2020 17:59
Operator : SY/MD
Sample : L5024-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AZ2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121520\
Data File : VV019656.D
Acq On : 15 Dec 2020 17:59
Operator : SY/MD
Sample : L5024-17
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AZ2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc